

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
 Data File : P0078608.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2021 11:35
 Operator : DD\AJ
 Sample : M2640-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260098L0K-END-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:14:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 05:39:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.615	1084378	465564	14.197	14.736
2) SA Decachlor...	9.950	8.803	719963	423504	17.756	17.613

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
Data File : P0078608.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2021 11:35
Operator : DD\AJ
Sample : M2640-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC260098L0K-END-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:14:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 05:39:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

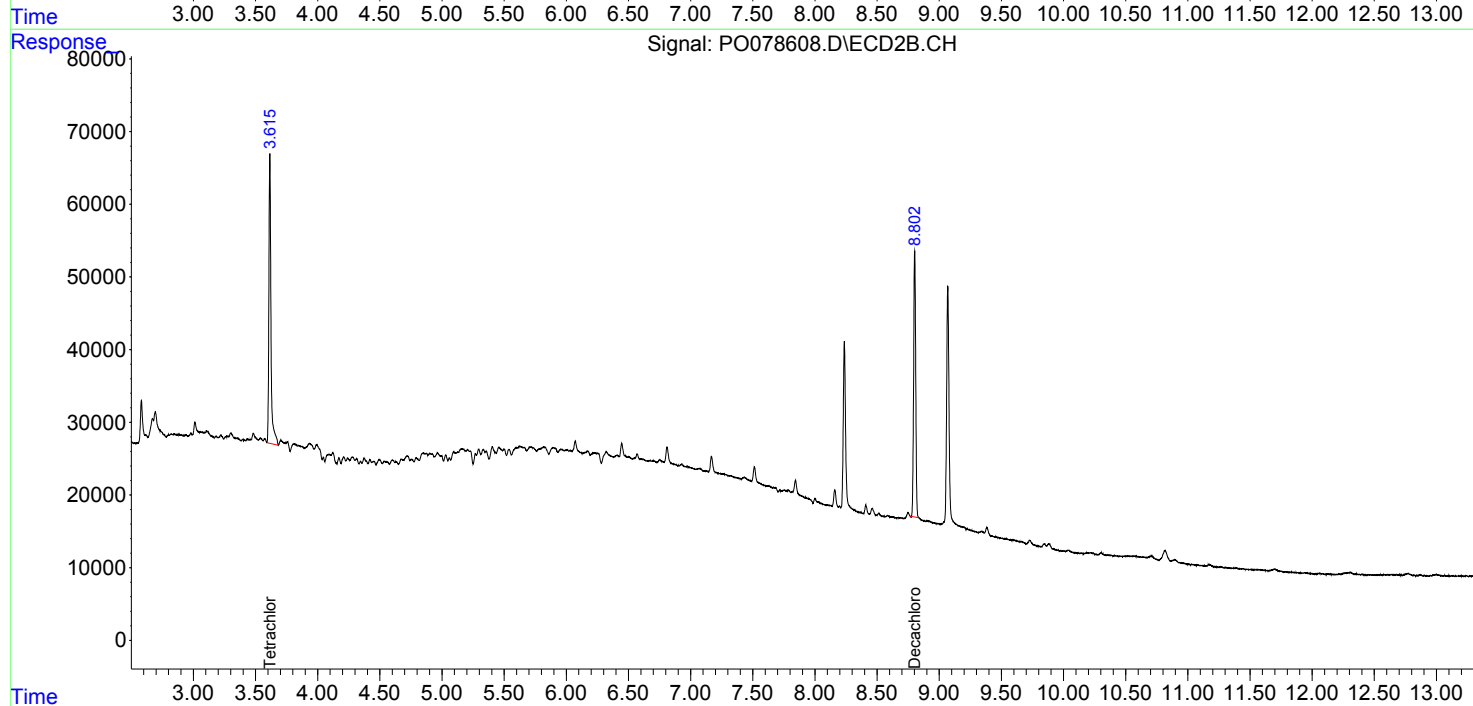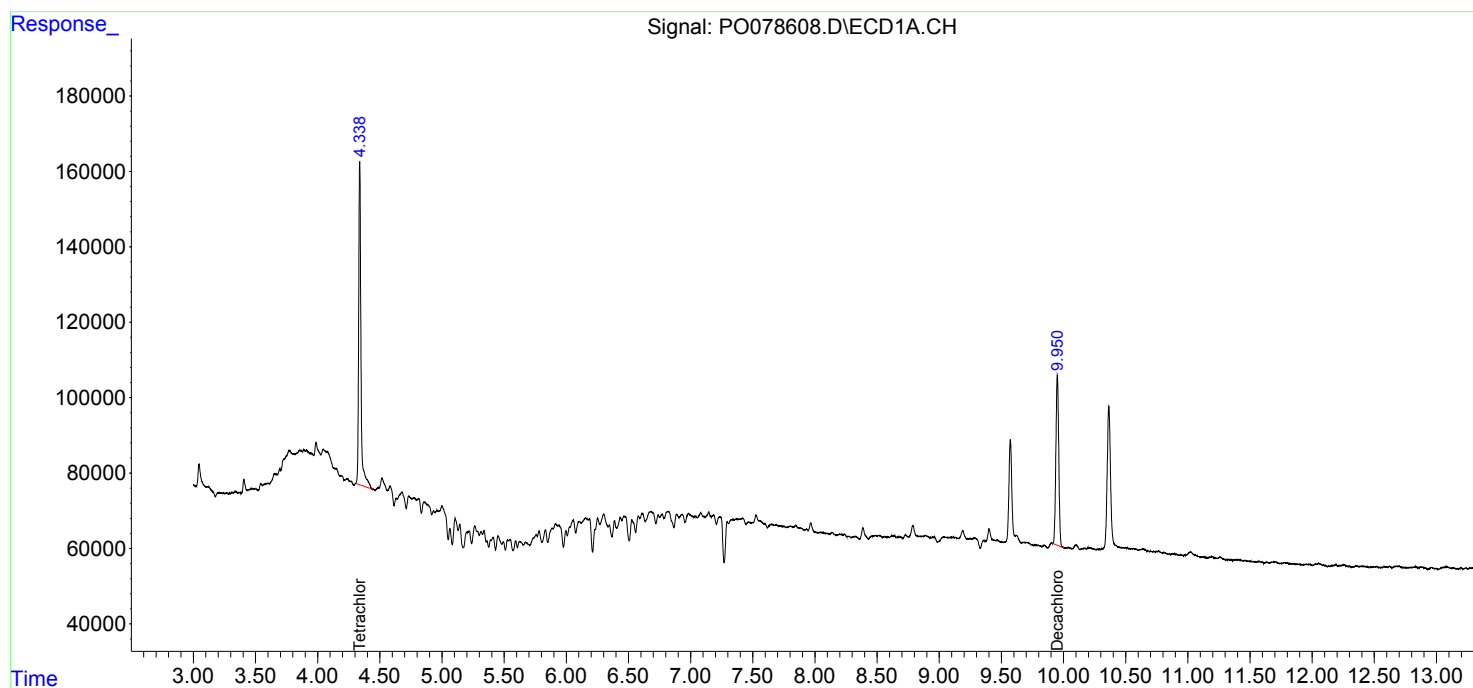


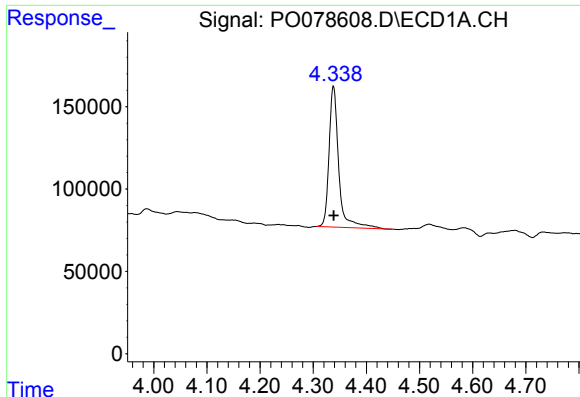

#1 Tetrachloro-m-xylene


R.T.: 4.338 min
Delta R.T.: -0.001 min
Response: 1084378
Conc: 14.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260098L0K-END-1-1

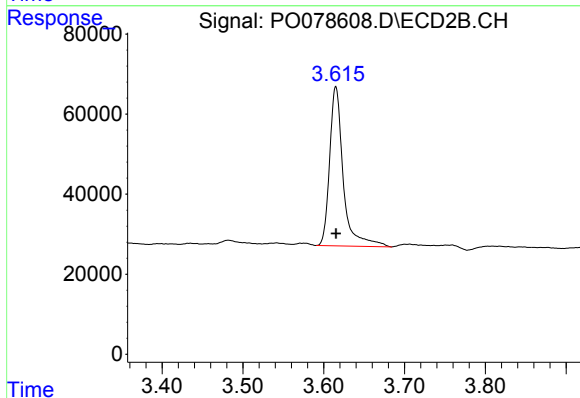


#1 Tetrachloro-m-xylene

R.T.: 3.615 min
Delta R.T.: 0.000 min
Response: 465564
Conc: 14.74 ng/ml

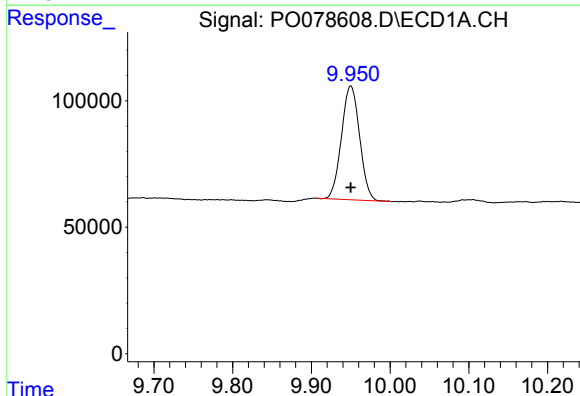

#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: 0.000 min
Response: 719963
Conc: 17.76 ng/ml

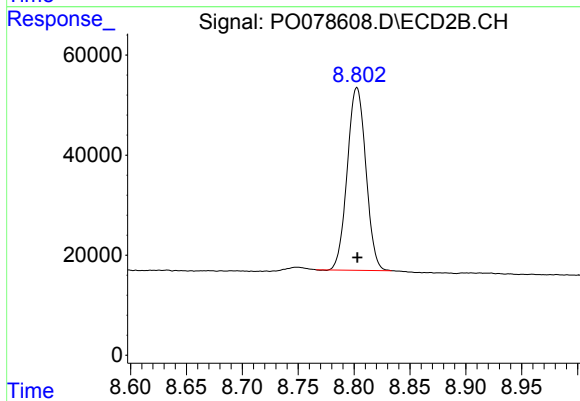

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 423504
Conc: 17.61 ng/ml