

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
 Data File : P0078609.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2021 11:52
 Operator : DD\AJ
 Sample : M2640-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260098L0K-END-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:15:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 05:39:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.615	1100135	582594	14.403	18.441 #
2) SA Decachlor...	9.950	8.803	781386	488985	19.271	20.336

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
Data File : P0078609.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2021 11:52
Operator : DD\AJ
Sample : M2640-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC260098L0K-END-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:15:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 05:39:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

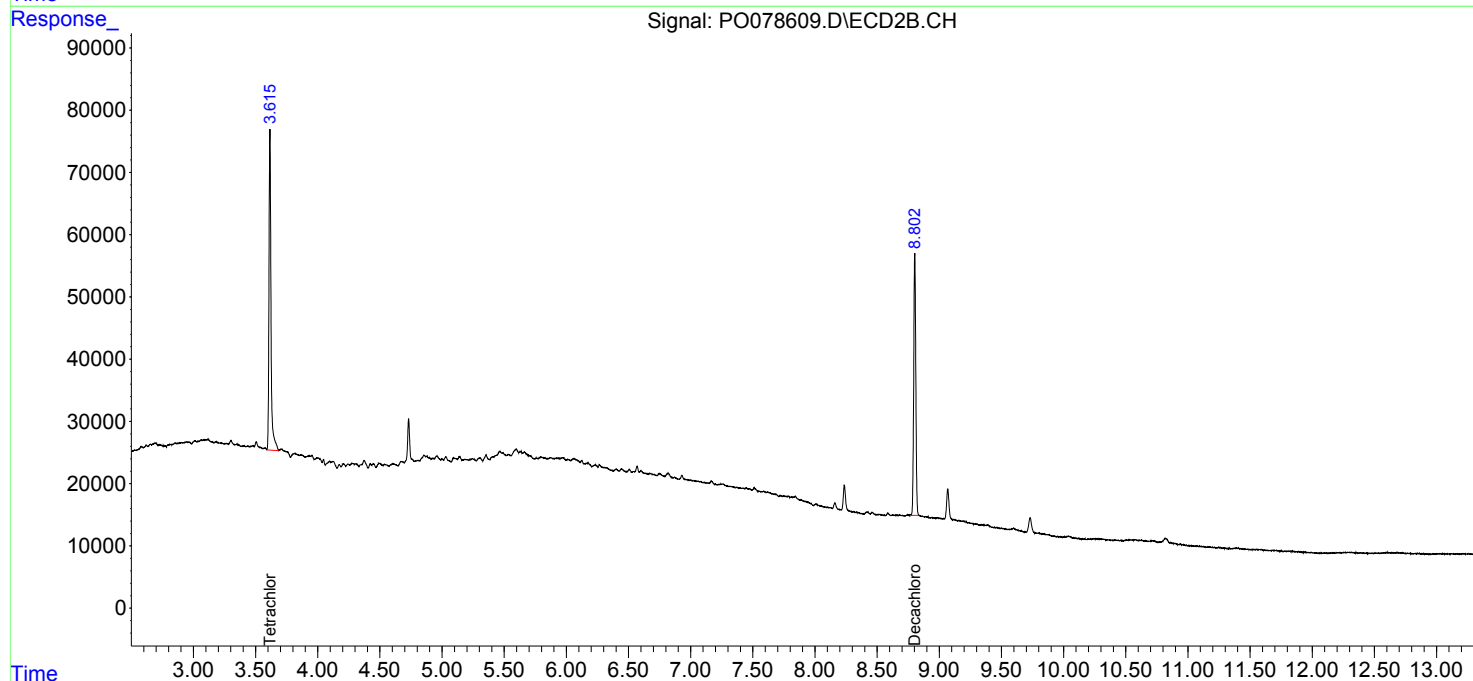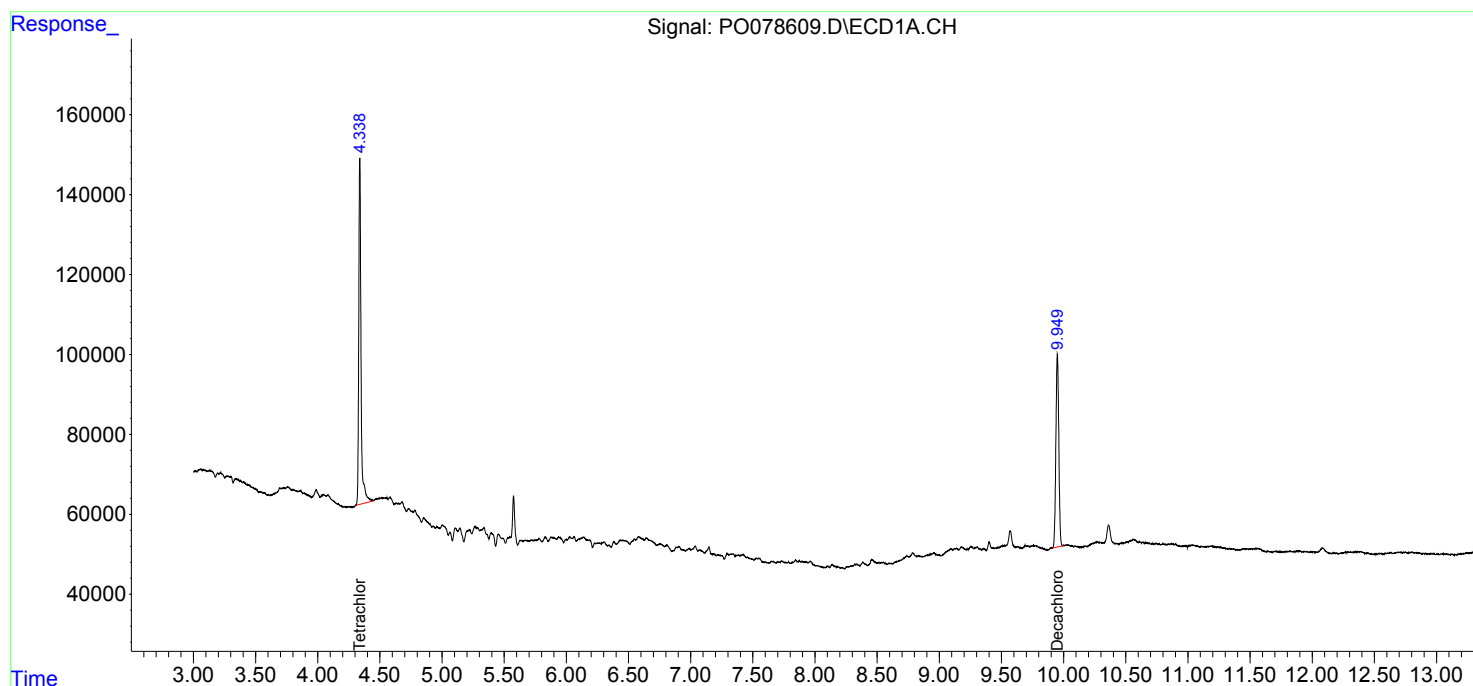


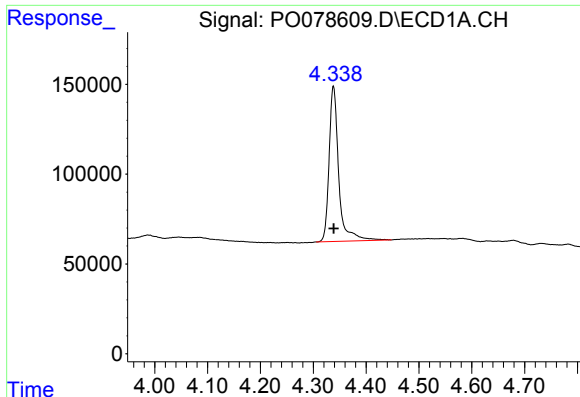

#1 Tetrachloro-m-xylene


R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 1100135
Conc: 14.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260098L0K-END-1-2

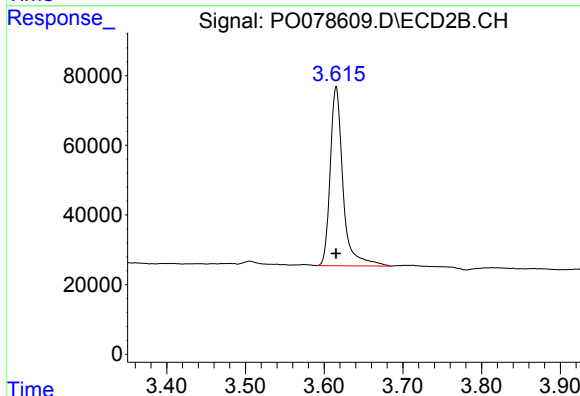


#1 Tetrachloro-m-xylene

R.T.: 3.615 min
Delta R.T.: 0.000 min
Response: 582594
Conc: 18.44 ng/ml

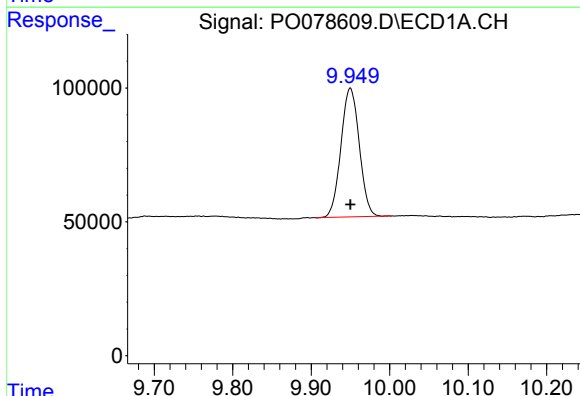

#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: 0.000 min
Response: 781386
Conc: 19.27 ng/ml

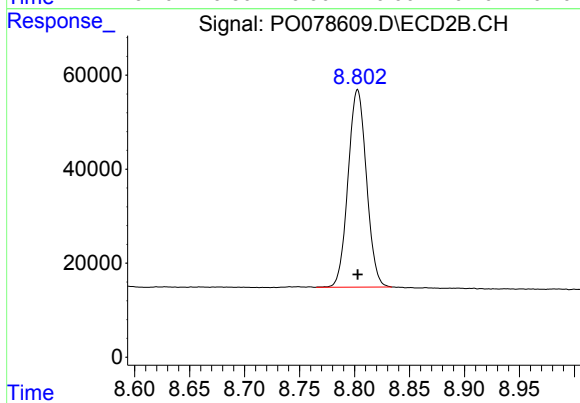

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 488985
Conc: 20.34 ng/ml