

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
 Data File : P0078622.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2021 17:44
 Operator : DD\AJ
 Sample : M2657-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HT-PIER

Manual Integrations
 APPROVED

Ankita
 6/11/2021 1:42:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:20:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 05:39:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.335	3.611	1755249	737525	22.980	23.345
2) SA Decachlor...	9.946	8.796	935397	580813	23.069	24.155
Target Compounds						
31) L7 AR-1260-1	7.293	6.400	37157	17108	12.673	10.782
32) L7 AR-1260-2	7.558	6.597	45182	31081	13.735	16.687
33) L7 AR-1260-3	7.916	6.746	24350	37273	10.283m	21.006m#
34) L7 AR-1260-4	8.141	7.223	32767	14126	12.740	9.640
35) L7 AR-1260-5	8.457	7.472	86449	70518	17.000m	20.210

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
Data File : P0078622.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2021 17:44
Operator : DD\AJ
Sample : M2657-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HT-PIER


Manual Integrations
APPROVED

Ankita
6/11/2021 1:42:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:20:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 05:39:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

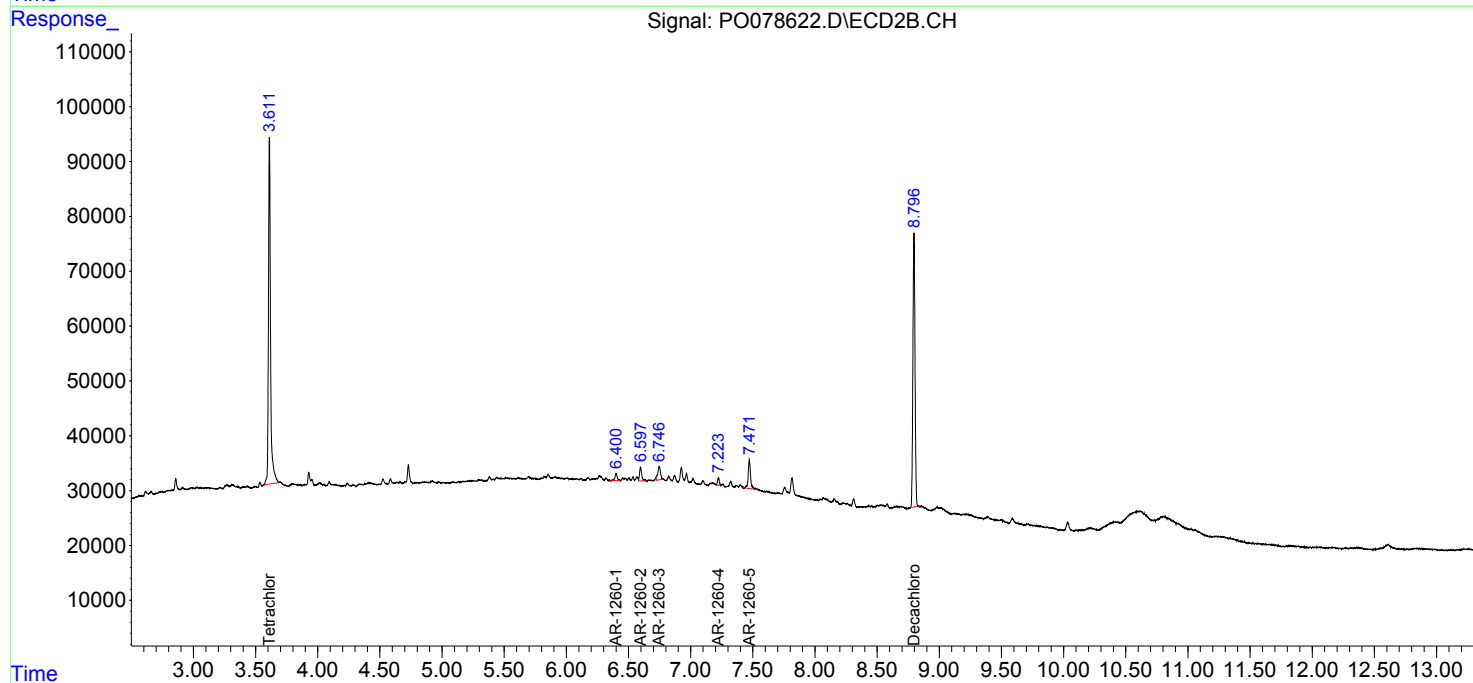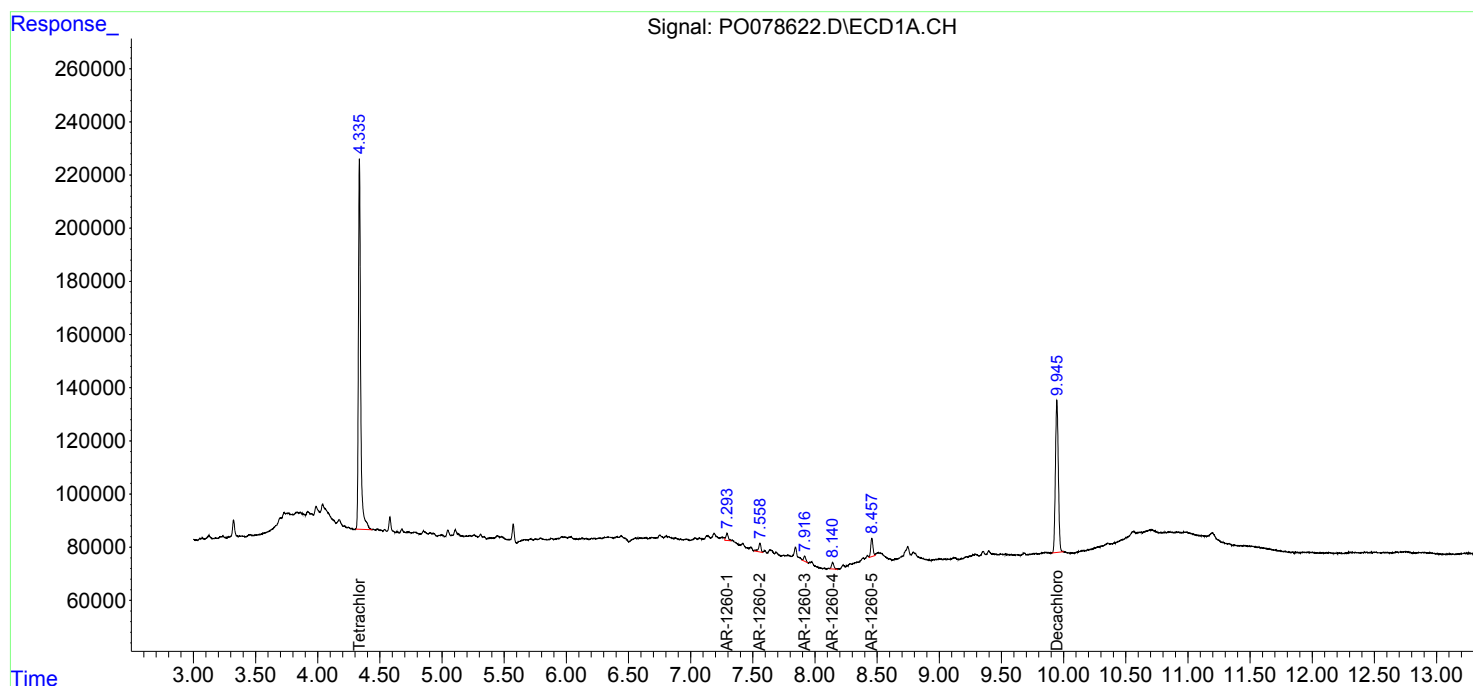

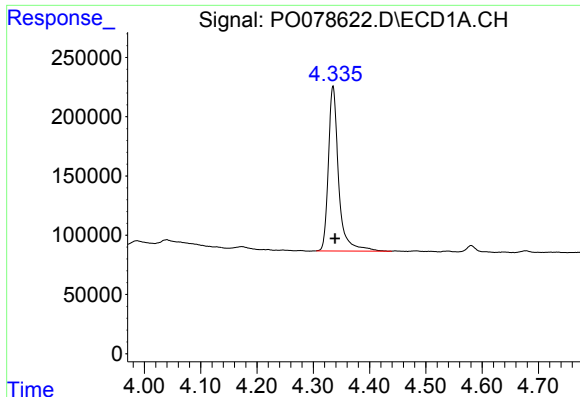


#1 Tetrachloro-m-xylene

R.T.: 4.335 min
Delta R.T.: -0.004 min
Response: 1755249
Conc: 22.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
HT-PIER


Manual Integrations
APPROVED

Ankita
6/11/2021 1:42:44 PM

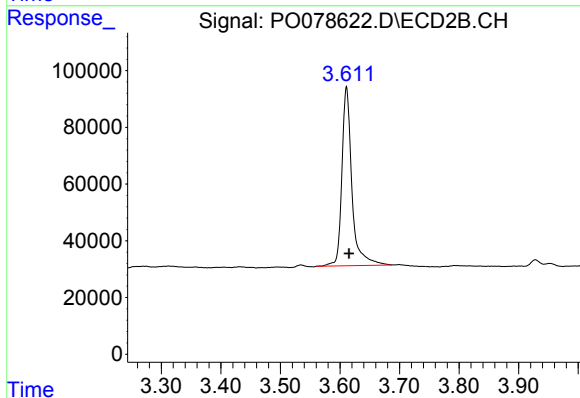


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.004 min
Response: 737525
Conc: 23.34 ng/ml

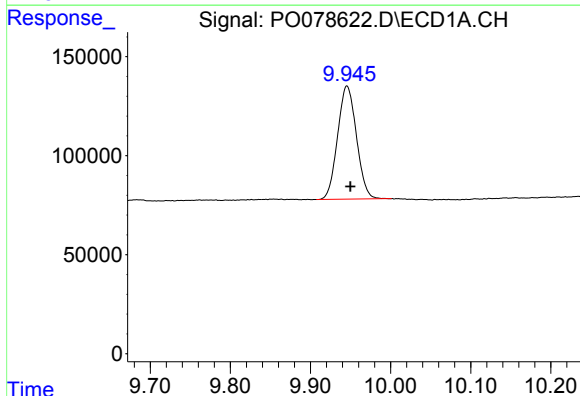


#2 Decachlorobiphenyl

R.T.: 9.946 min
Delta R.T.: -0.004 min
Response: 935397
Conc: 23.07 ng/ml

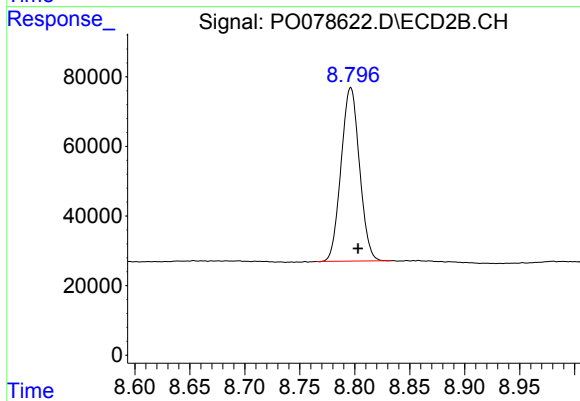

#2 Decachlorobiphenyl

R.T.: 8.796 min
Delta R.T.: -0.007 min
Response: 580813
Conc: 24.15 ng/ml

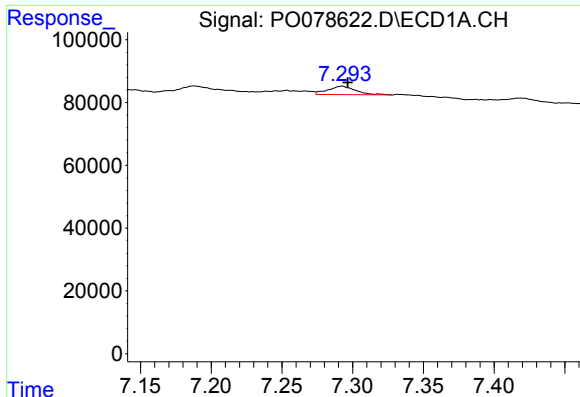


#31 AR-1260-1

R.T.: 7.293 min
Delta R.T.: -0.004 min
Response: 37157
Conc: 12.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
HT-PIER


Manual Integrations
APPROVED

Ankita
6/11/2021 1:42:44 PM

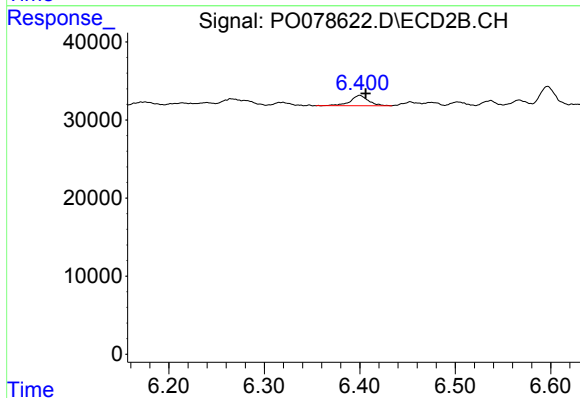


#31 AR-1260-1

R.T.: 6.400 min
Delta R.T.: -0.006 min
Response: 17108
Conc: 10.78 ng/ml

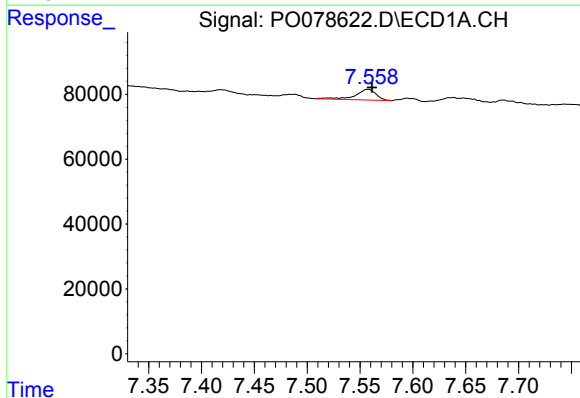


#32 AR-1260-2

R.T.: 7.558 min
Delta R.T.: -0.004 min
Response: 45182
Conc: 13.73 ng/ml

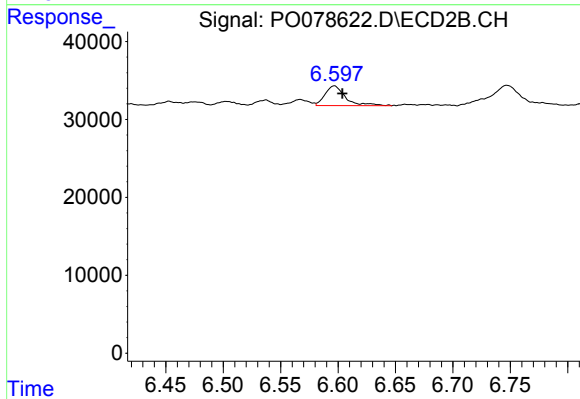

#32 AR-1260-2

R.T.: 6.597 min
Delta R.T.: -0.007 min
Response: 31081
Conc: 16.69 ng/ml

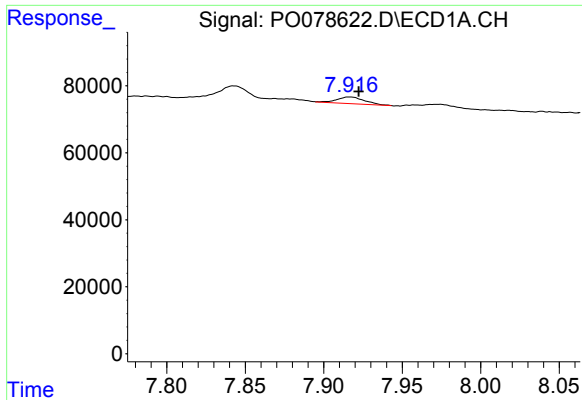


#33 AR-1260-3

R.T.: 7.916 min
Delta R.T.: -0.007 min
Response: 24350
Conc: 10.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HT-PIER


Manual Integrations
APPROVED

Ankita
6/11/2021 1:42:44 PM

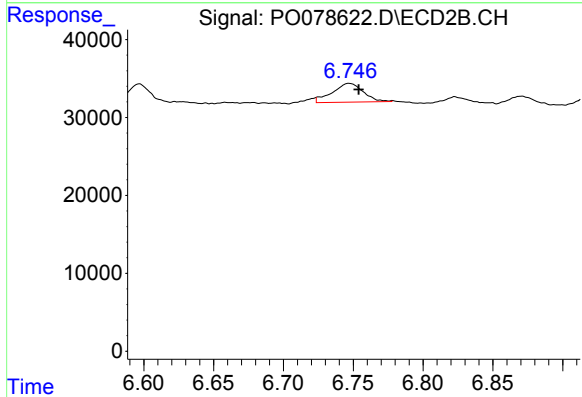


#33 AR-1260-3

R.T.: 6.746 min
Delta R.T.: -0.008 min
Response: 37273
Conc: 21.01 ng/ml m

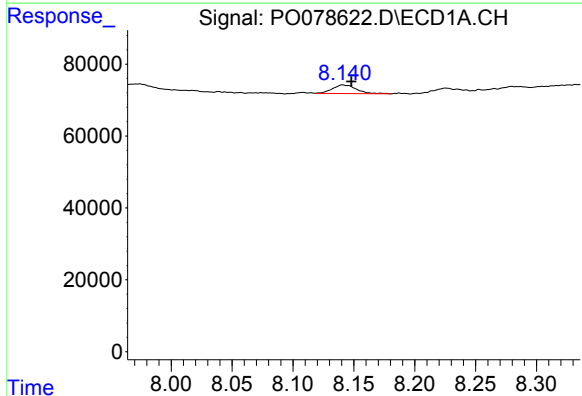


#34 AR-1260-4

R.T.: 8.141 min
Delta R.T.: -0.007 min
Response: 32767
Conc: 12.74 ng/ml

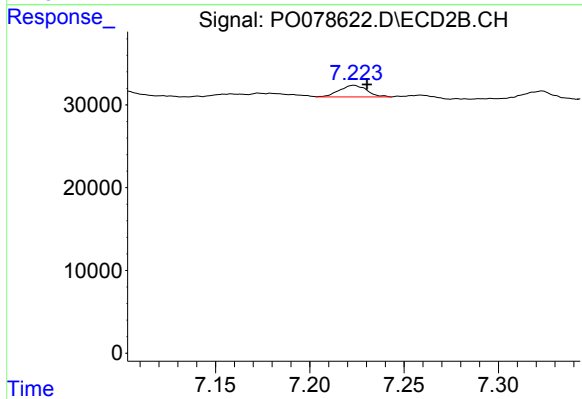

#34 AR-1260-4

R.T.: 7.223 min
Delta R.T.: -0.007 min
Response: 14126
Conc: 9.64 ng/ml

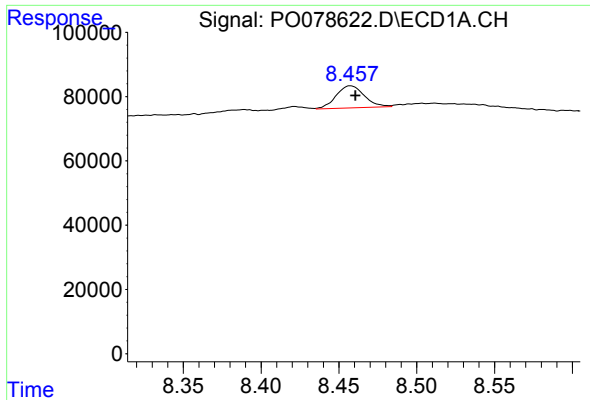


#35 AR-1260-5

R.T.: 8.457 min
Delta R.T.: -0.004 min
Response: 86449
Conc: 17.00 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HT-PIER

Manual Integrations
APPROVED

Ankita
6/11/2021 1:42:44 PM

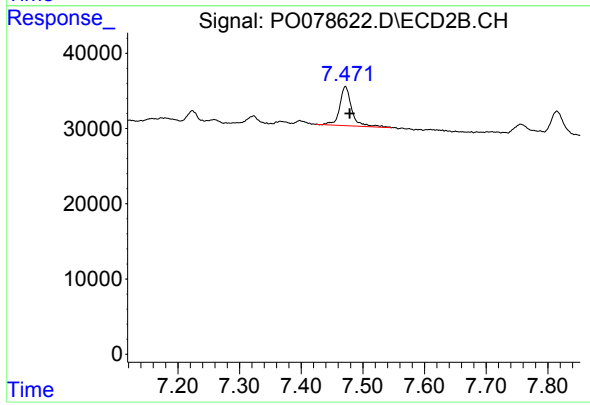

#35 AR-1260-5

R.T.: 7.472 min
Delta R.T.: -0.007 min
Response: 70518
Conc: 20.21 ng/ml