

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061119\
 Data File : P0057078.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jun 2019 16:05
 Operator : SM/SJ
 Sample : IDOC BL
 Misc : FOR RC WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 06:32:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.252	3.562	778309	643292	20.330	19.506
2)	SA Decachlor...	9.823	8.493	877784	584901	17.883	16.404

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061119\
Data File : P0057078.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jun 2019 16:05
Operator : SM/SJ
Sample : IDOC BL
Misc : FOR RC WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDOC BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 06:32:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

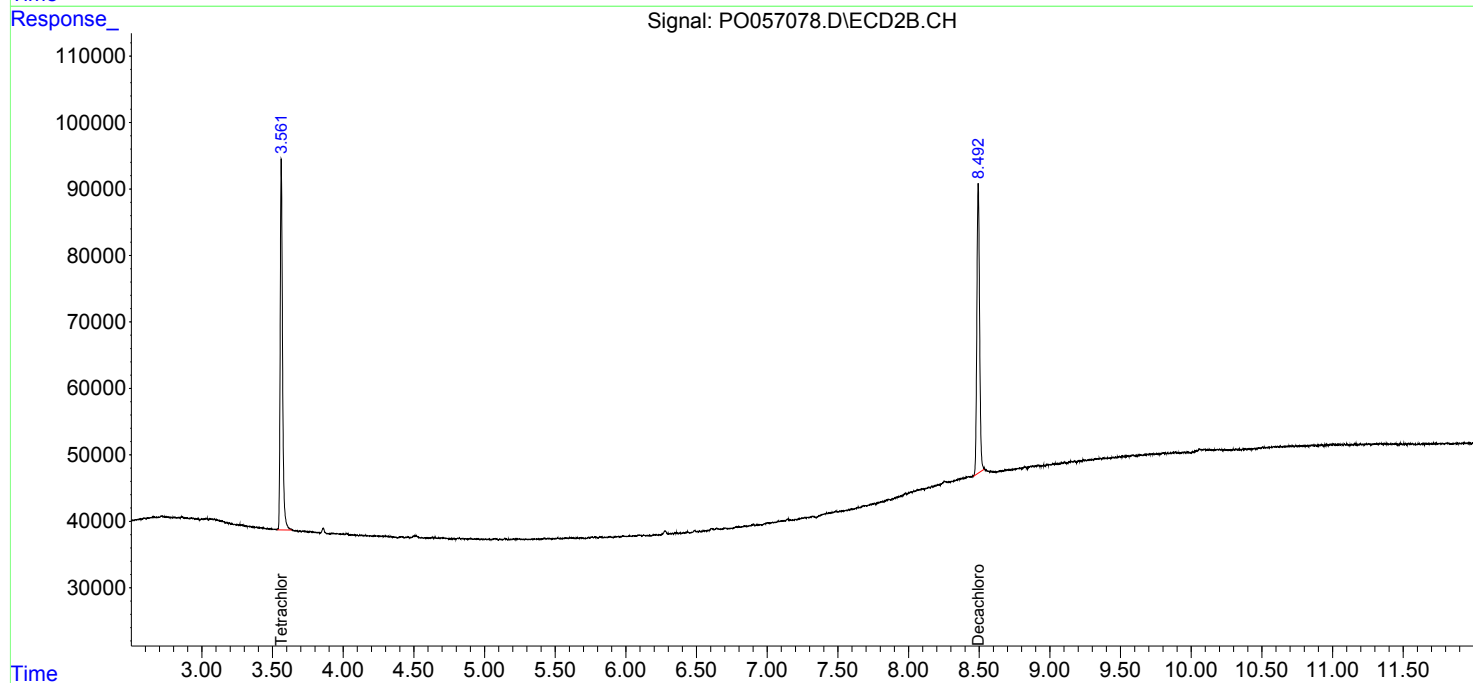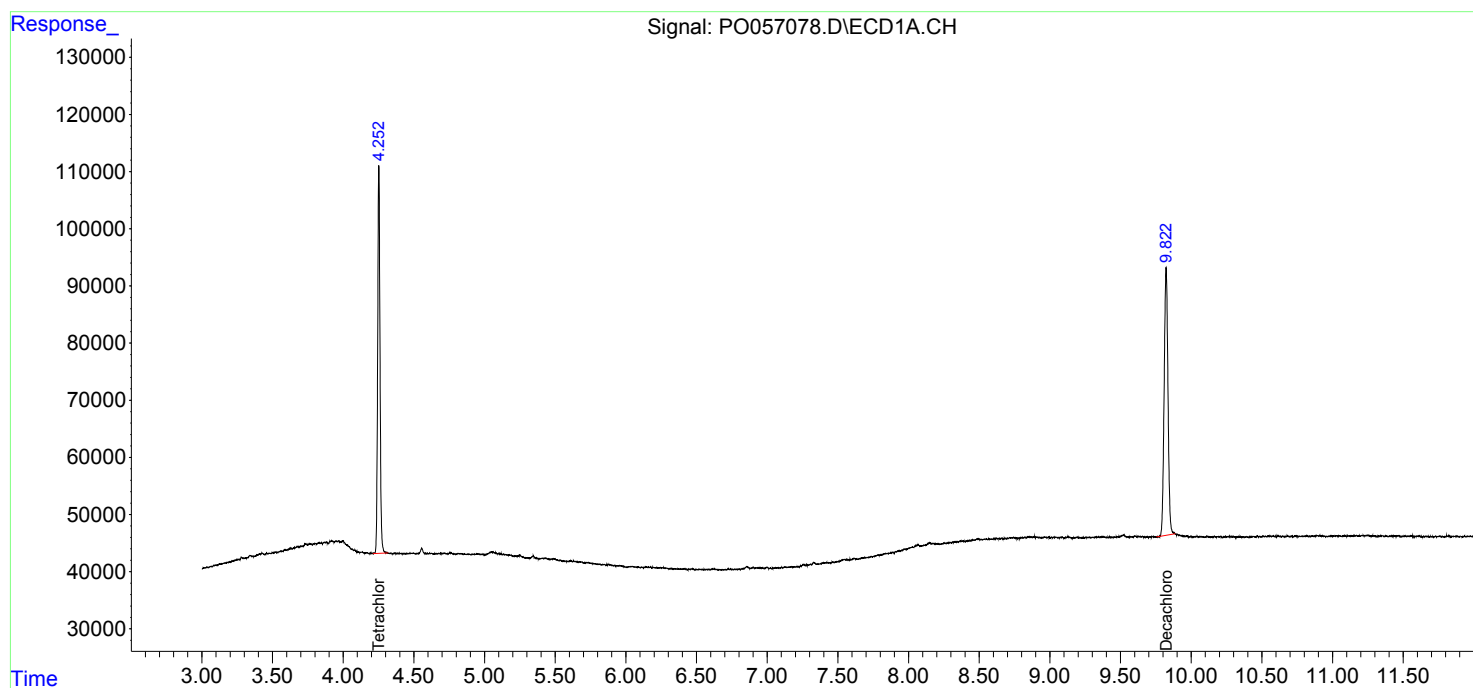


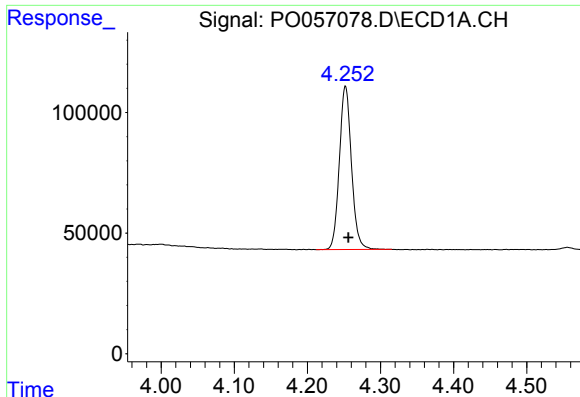

#1 Tetrachloro-m-xylene


R.T.: 4.252 min
Delta R.T.: -0.004 min
Response: 778309
Conc: 20.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDOC BL

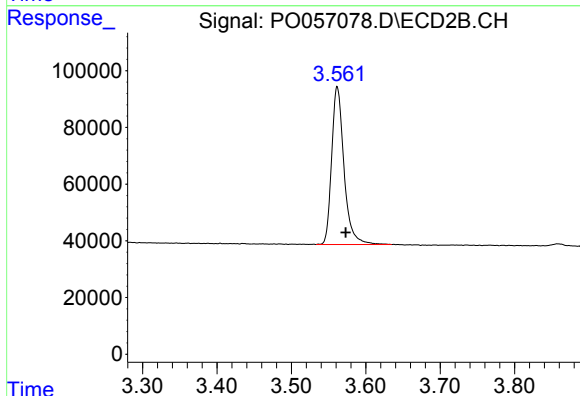


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.011 min
Response: 643292
Conc: 19.51 ng/ml

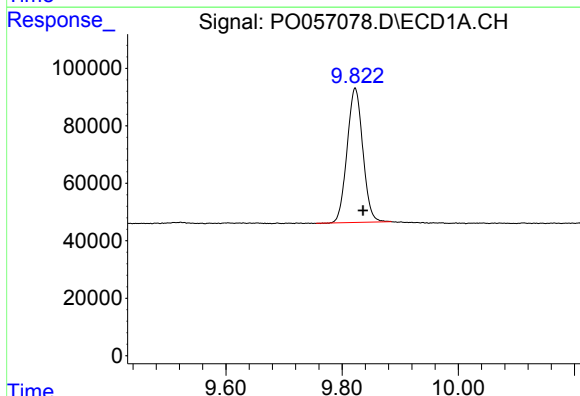

#2 Decachlorobiphenyl

R.T.: 9.823 min
Delta R.T.: -0.014 min
Response: 877784
Conc: 17.88 ng/ml

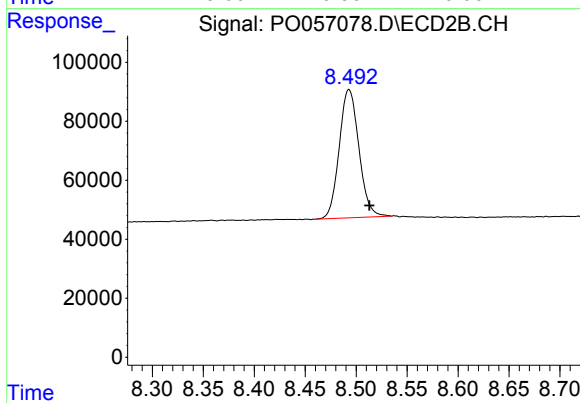

#2 Decachlorobiphenyl

R.T.: 8.493 min
Delta R.T.: -0.020 min
Response: 584901
Conc: 16.40 ng/ml