

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061119\
 Data File : P0057070.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jun 2019 12:51
 Operator : SM/SJ
 Sample : K3158-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-03-060619

Manual Integrations
 APPROVED

Ankita
 6/12/2019 2:29:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 13:22:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.252	3.563	1229464	950332	32.115m	28.817
2) SA Decachlor...	9.821	8.494	1150715	718254	23.444	20.144

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061119\
Data File : PO057070.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jun 2019 12:51
Operator : SM/SJ
Sample : K3158-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-03-060619


Manual Integrations
APPROVED

Ankita
6/12/2019 2:29:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 13:22:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

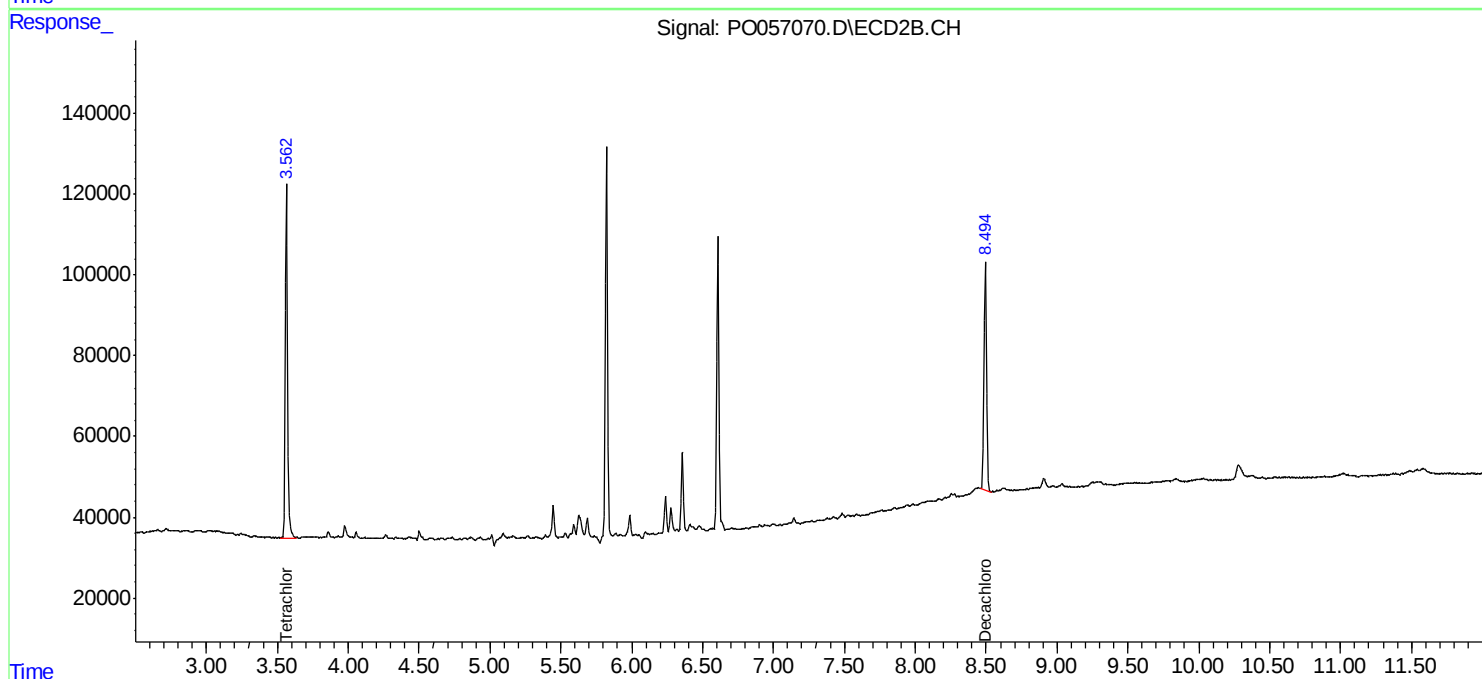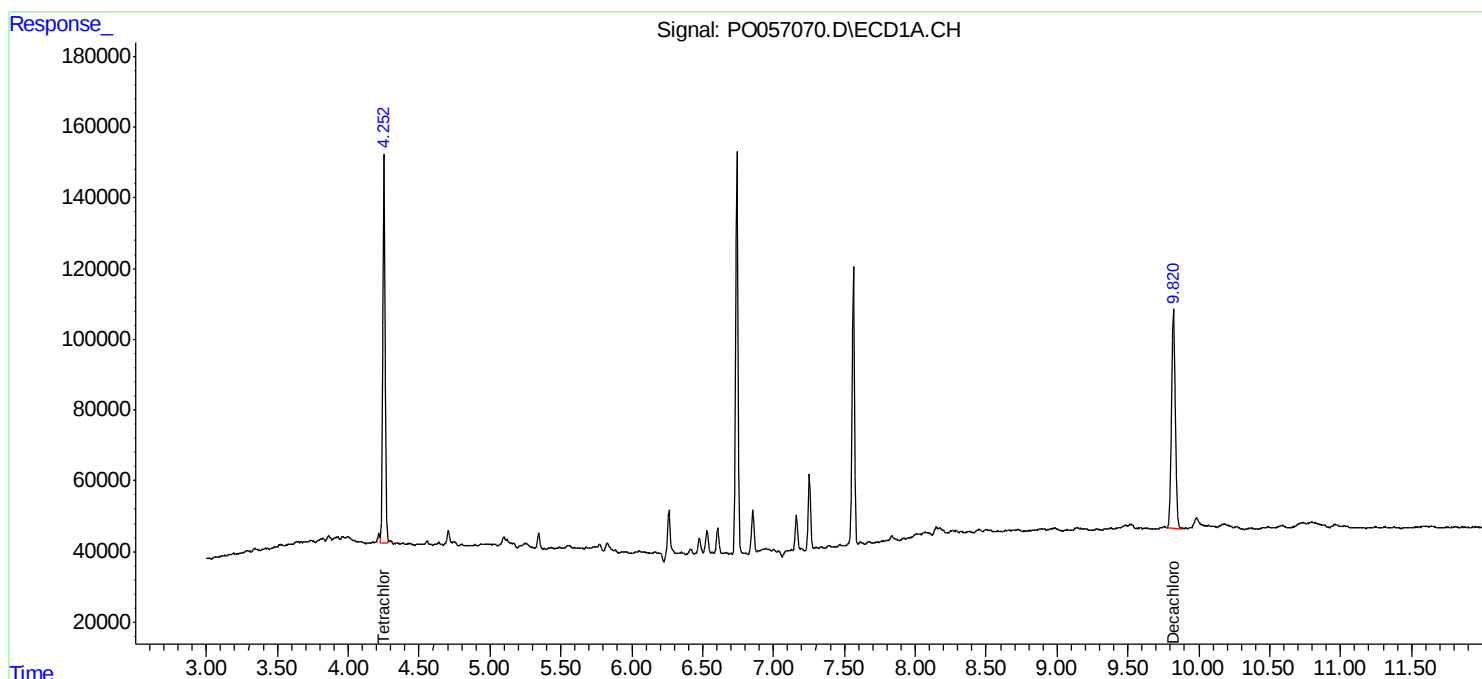

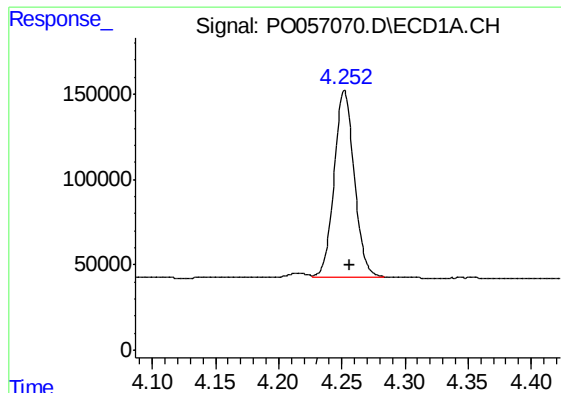


#1 Tetrachloro-m-xylene

R.T.: 4.252 min
Delta R.T.: -0.004 min
Response: 1229464
Conc: 32.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-03-060619


Manual Integrations
APPROVED

Ankita
6/12/2019 2:29:13 PM

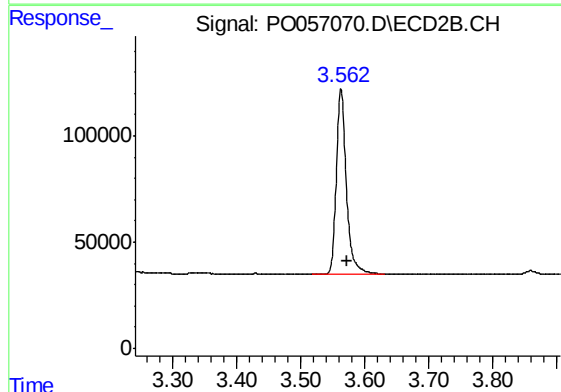


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.010 min
Response: 950332
Conc: 28.82 ng/ml

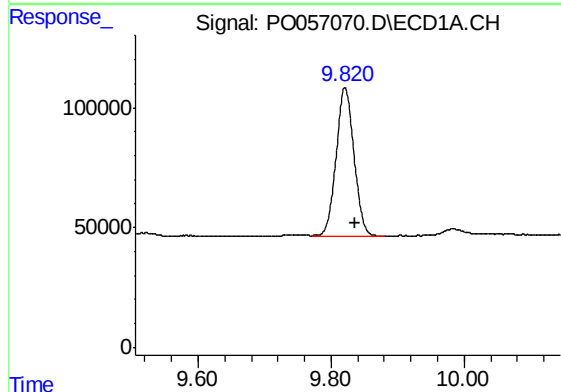

#2 Decachlorobiphenyl

R.T.: 9.821 min
Delta R.T.: -0.015 min
Response: 1150715
Conc: 23.44 ng/ml

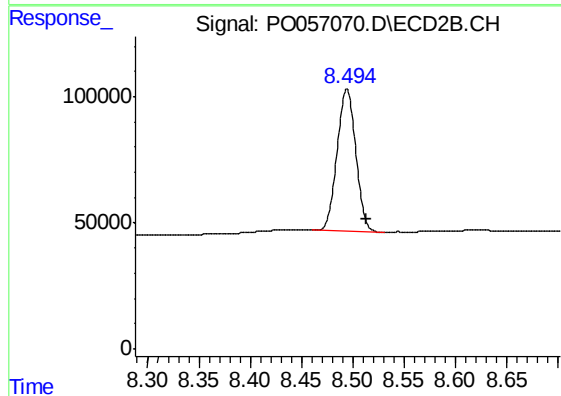

#2 Decachlorobiphenyl

R.T.: 8.494 min
Delta R.T.: -0.019 min
Response: 718254
Conc: 20.14 ng/ml