

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061119\
 Data File : P0057088.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jun 2019 18:58
 Operator : SM/SJ
 Sample : K3282-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 25082-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 06:36:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.241	3.562	714484	583576	18.663	17.696
2) SA Decachlor...	9.807	8.490	706354	451004	14.391	12.648

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061119\
Data File : P0057088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jun 2019 18:58
Operator : SM/SJ
Sample : K3282-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
25082-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 06:36:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

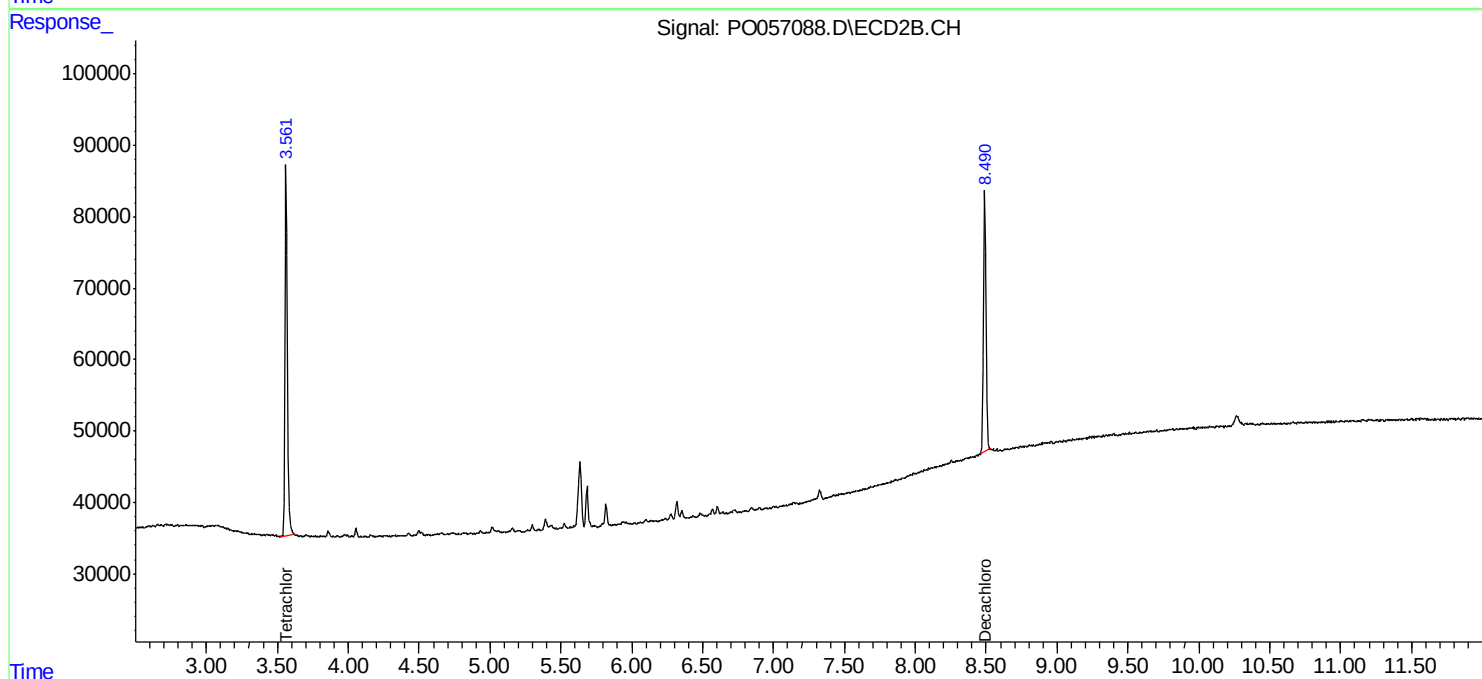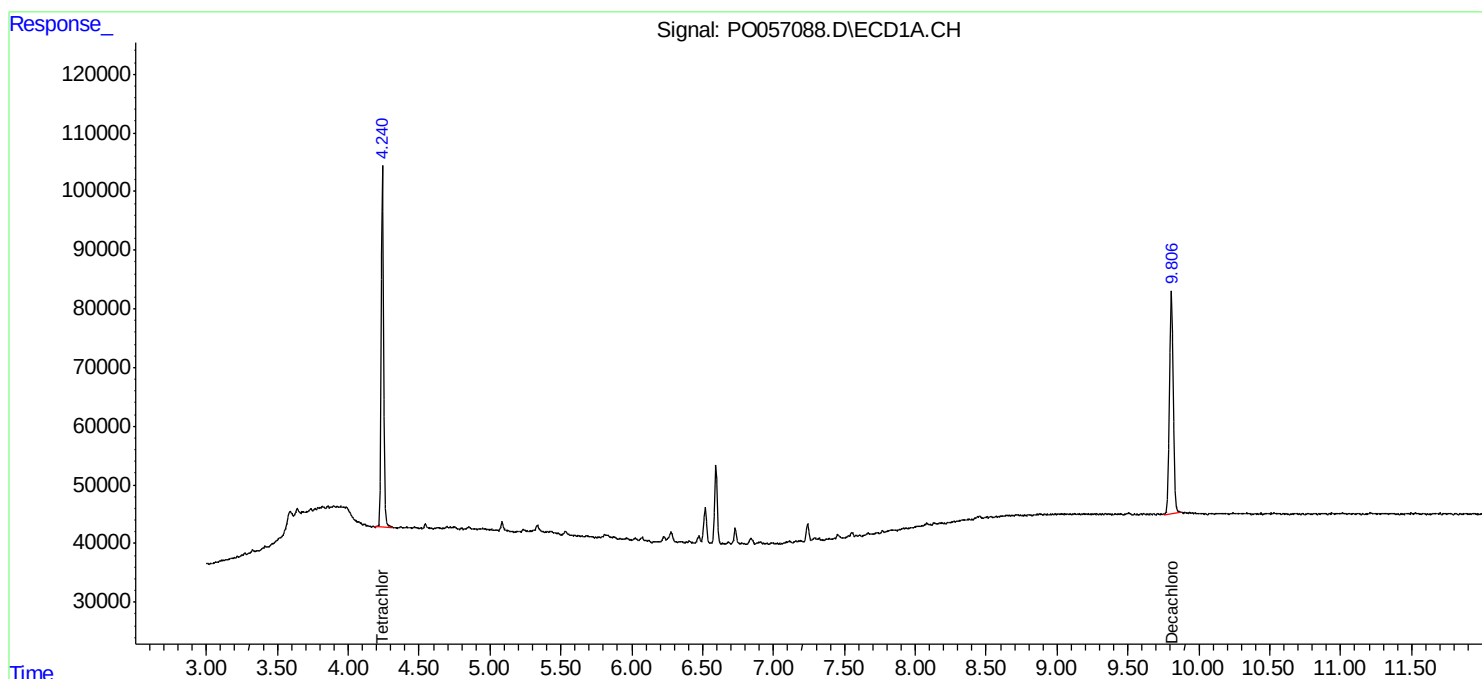


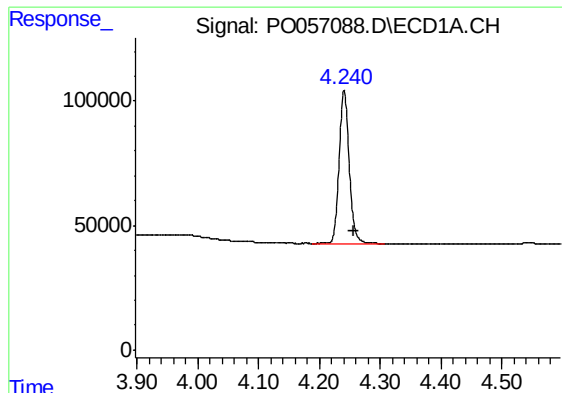

#1 Tetrachloro-m-xylene


R.T.: 4.241 min
Delta R.T.: -0.015 min
Response: 714484
Conc: 18.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
25082-2022

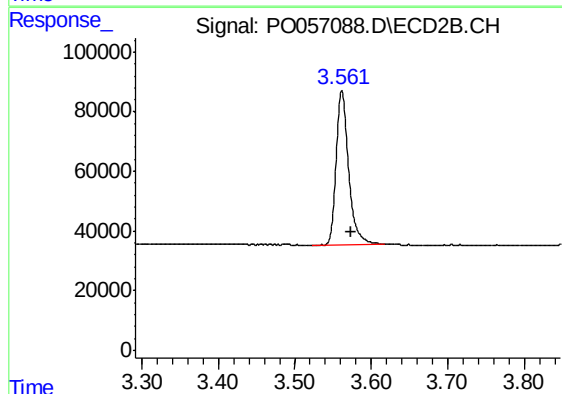


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.011 min
Response: 583576
Conc: 17.70 ng/ml

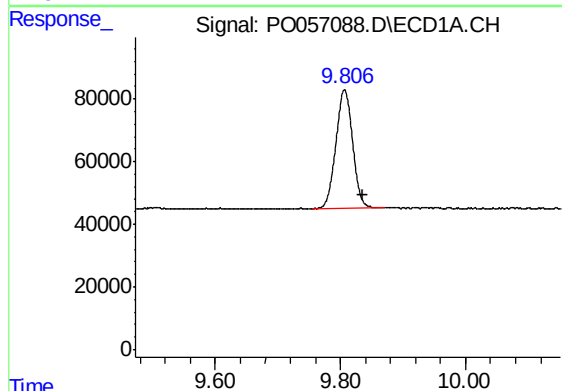

#2 Decachlorobiphenyl

R.T.: 9.807 min
Delta R.T.: -0.030 min
Response: 706354
Conc: 14.39 ng/ml

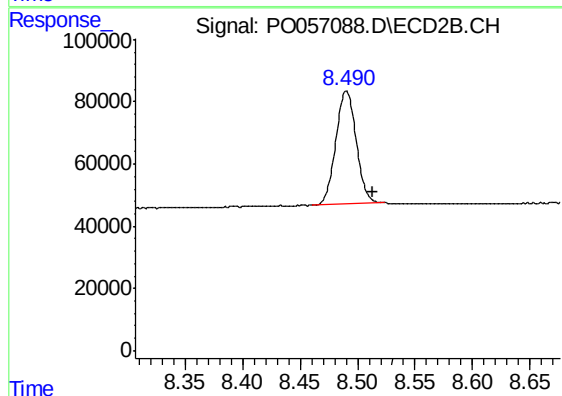

#2 Decachlorobiphenyl

R.T.: 8.490 min
Delta R.T.: -0.023 min
Response: 451004
Conc: 12.65 ng/ml