

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0061121\
 Data File : P0078653.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jun 2021 11:30
 Operator : DD\AJ
 Sample : M2658-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 T-FLOOR

Manual Integrations
 APPROVED

Ankita
 6/14/2021 2:29:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 14:11:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 05:39:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.334	3.610	1830898	799418	23.971	25.304
2)	SA Decachlor...	9.944	8.795	1308634	759365	32.274	31.580
Target Compounds							
26)	L6 AR-1254-1	6.533	5.692	598510	210010	236.504m	121.679m#
27)	L6 AR-1254-2	6.751	5.851	488827	169000	123.095m	105.395m
28)	L6 AR-1254-3	7.128	6.263	611242	234750	147.159m	98.115m#
29)	L6 AR-1254-4	7.421	6.501	300684	116738	102.263m	79.771m
30)	L6 AR-1254-5	7.843	6.924	168619	136213	52.588	59.746m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061121\
Data File : P0078653.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jun 2021 11:30
Operator : DD\AJ
Sample : M2658-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
T-FLOOR


Manual Integrations
APPROVED

Ankita
6/14/2021 2:29:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 14:11:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 05:39:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

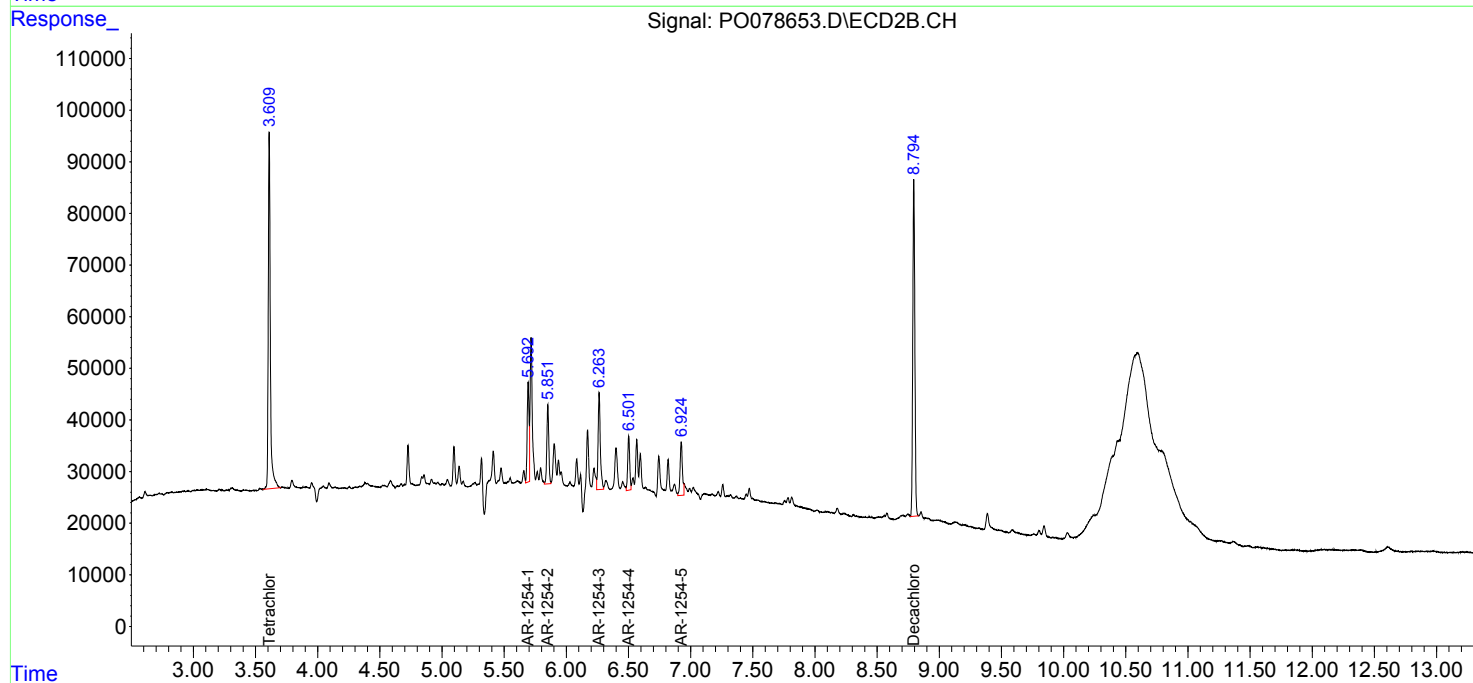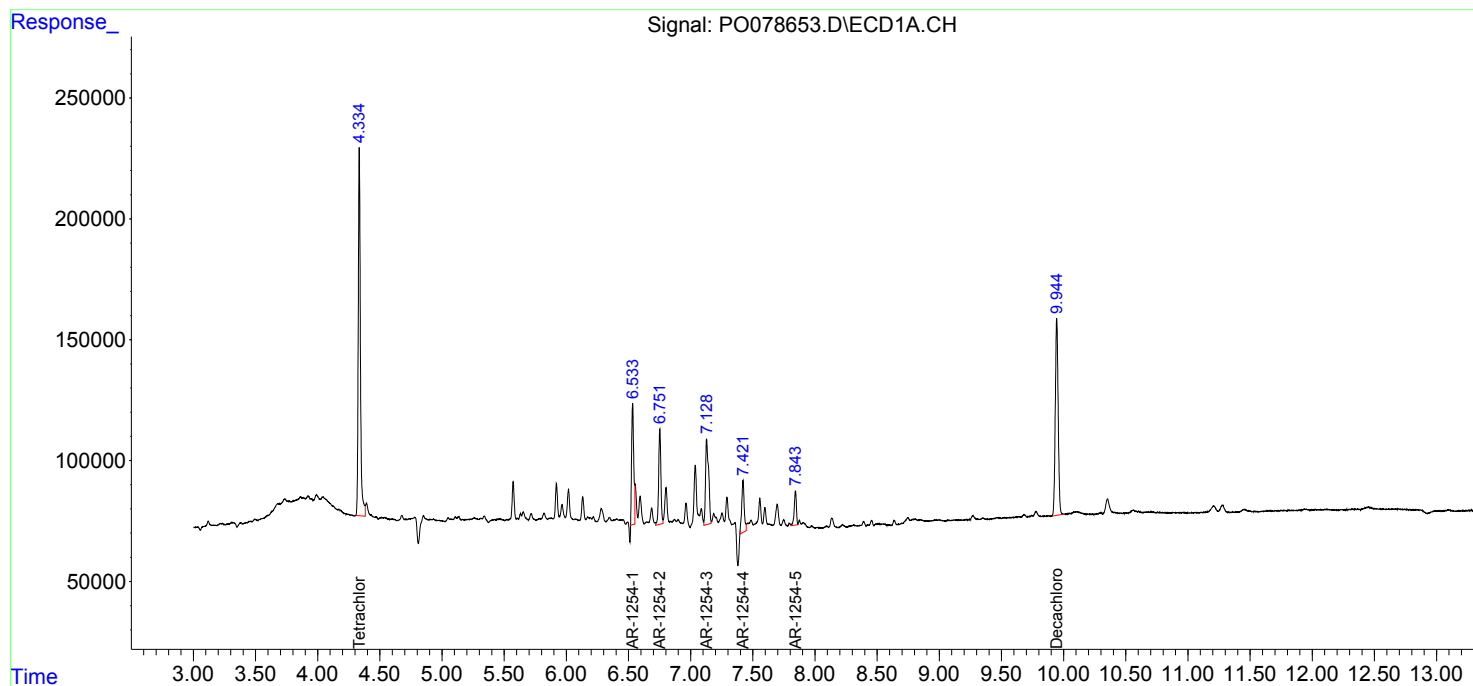

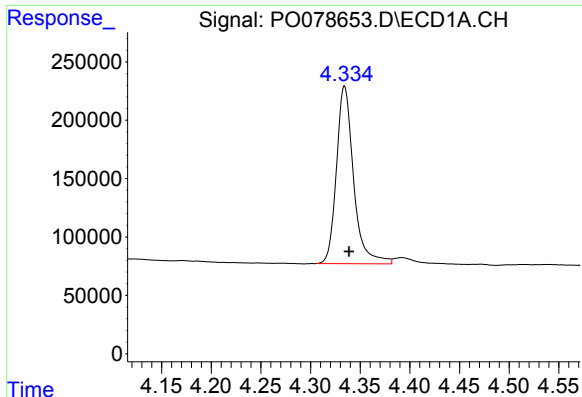


#1 Tetrachloro-m-xylene

R.T.: 4.334 min
Delta R.T.: -0.005 min
Response: 1830898
Conc: 23.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
T-FLOOR


Manual Integrations
APPROVED

Ankita
6/14/2021 2:29:40 PM

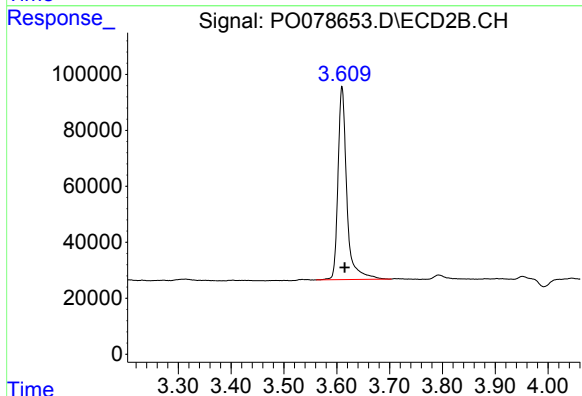


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.005 min
Response: 799418
Conc: 25.30 ng/ml

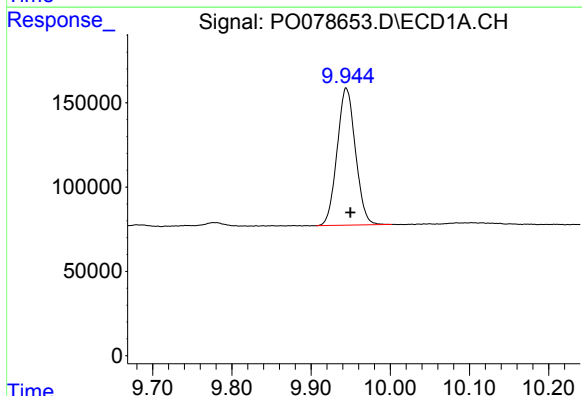


#2 Decachlorobiphenyl

R.T.: 9.944 min
Delta R.T.: -0.005 min
Response: 1308634
Conc: 32.27 ng/ml

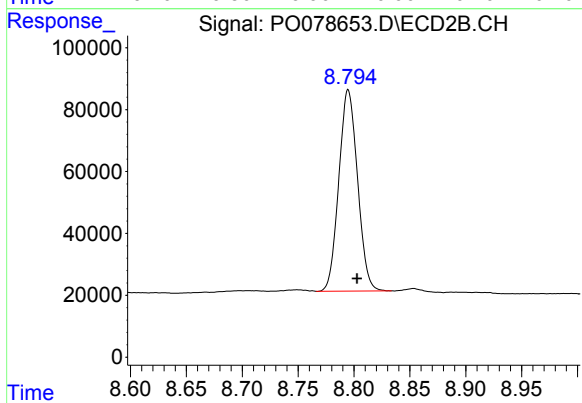

#2 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: -0.008 min
Response: 759365
Conc: 31.58 ng/ml

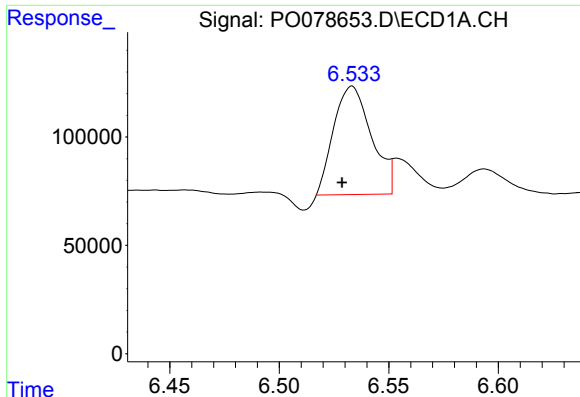


#26 AR-1254-1

R.T.: 6.533 min
Delta R.T.: 0.004 min
Response: 598510
Conc: 236.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
T-FLOOR


Manual Integrations
APPROVED

Ankita
6/14/2021 2:29:40 PM

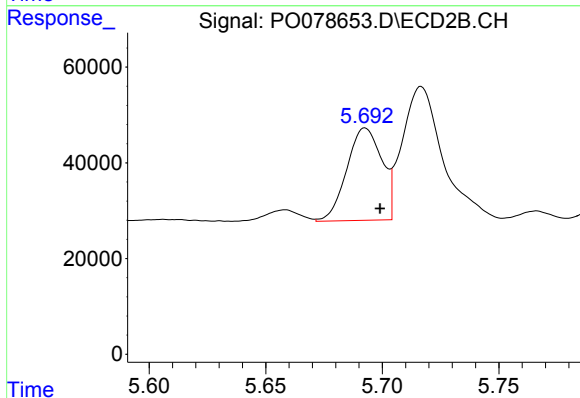


#26 AR-1254-1

R.T.: 5.692 min
Delta R.T.: -0.007 min
Response: 210010
Conc: 121.68 ng/ml m

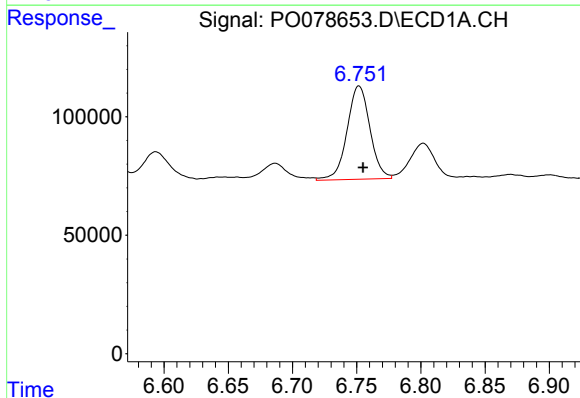


#27 AR-1254-2

R.T.: 6.751 min
Delta R.T.: -0.004 min
Response: 488827
Conc: 123.09 ng/ml m

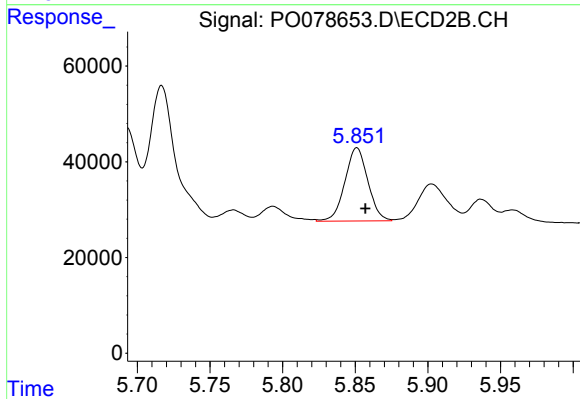

#27 AR-1254-2

R.T.: 5.851 min
Delta R.T.: -0.006 min
Response: 169000
Conc: 105.39 ng/ml m

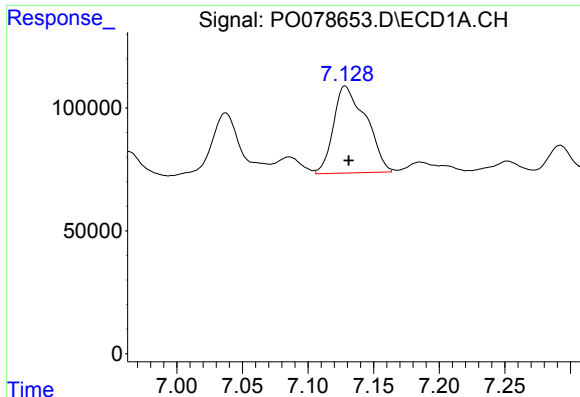


#28 AR-1254-3

R.T.: 7.128 min
Delta R.T.: -0.003 min
Response: 611242
Conc: 147.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
T-FLOOR


Manual Integrations
APPROVED

Ankita
6/14/2021 2:29:40 PM

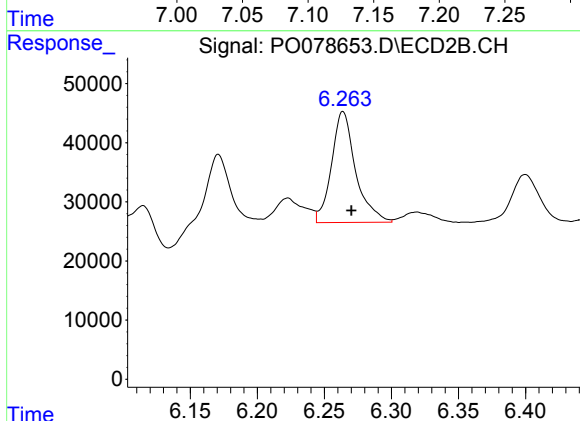


#28 AR-1254-3

R.T.: 6.263 min
Delta R.T.: -0.007 min
Response: 234750
Conc: 98.12 ng/ml m

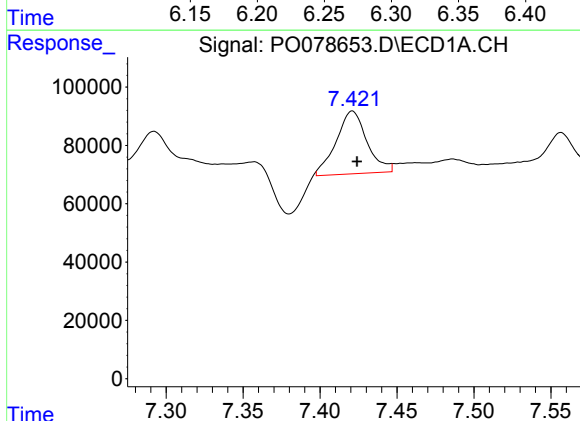


#29 AR-1254-4

R.T.: 7.421 min
Delta R.T.: -0.003 min
Response: 300684
Conc: 102.26 ng/ml m

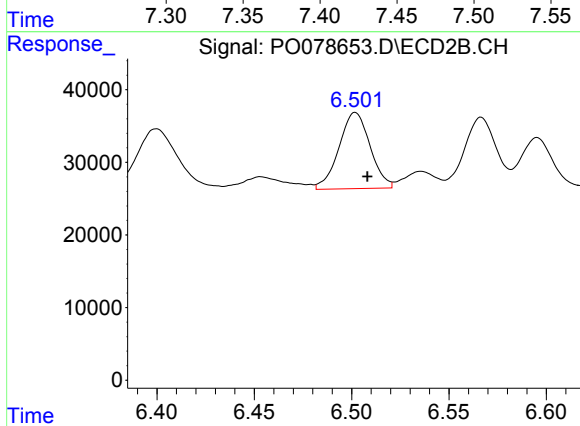

#29 AR-1254-4

R.T.: 6.501 min
Delta R.T.: -0.007 min
Response: 116738
Conc: 79.77 ng/ml m

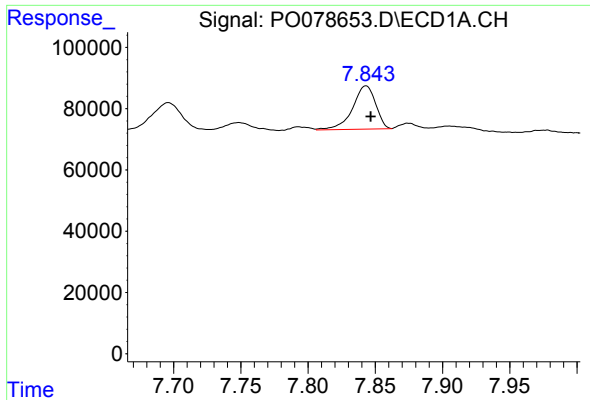


#30 AR-1254-5

R.T.: 7.843 min
Delta R.T.: -0.004 min
Response: 168619
Conc: 52.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
T-FLOOR

Manual Integrations
APPROVED

Ankita
6/14/2021 2:29:40 PM

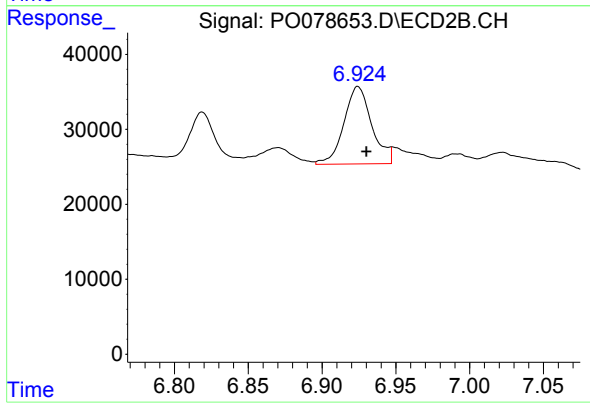

#30 AR-1254-5

R.T.: 6.924 min
Delta R.T.: -0.006 min
Response: 136213
Conc: 59.75 ng/ml m