

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061121\
 Data File : P0078709.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2021 8:14
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 6/14/2021 2:30:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 00:44:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 05:39:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.333	3.610	3759415	1503509	49.220	47.590
2) SA Decachlor...	9.941	8.792	2525896	1360128	62.294	56.565
Target Compounds						
21) L5 AR-1248-1	5.629	4.836	649756	309476	477.902	478.861
22) L5 AR-1248-2	5.919	5.095	910618	452962	468.978	464.543
23) L5 AR-1248-3	6.130	5.138	1071454	455173	474.095	469.149
24) L5 AR-1248-4	6.553	5.318	1142684	535597	482.321	462.381m
25) L5 AR-1248-5	6.590	5.734	1132341	522465	486.579	476.529

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061121\
Data File : P0078709.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2021 8:14
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/14/2021 2:30:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 00:44:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 05:39:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

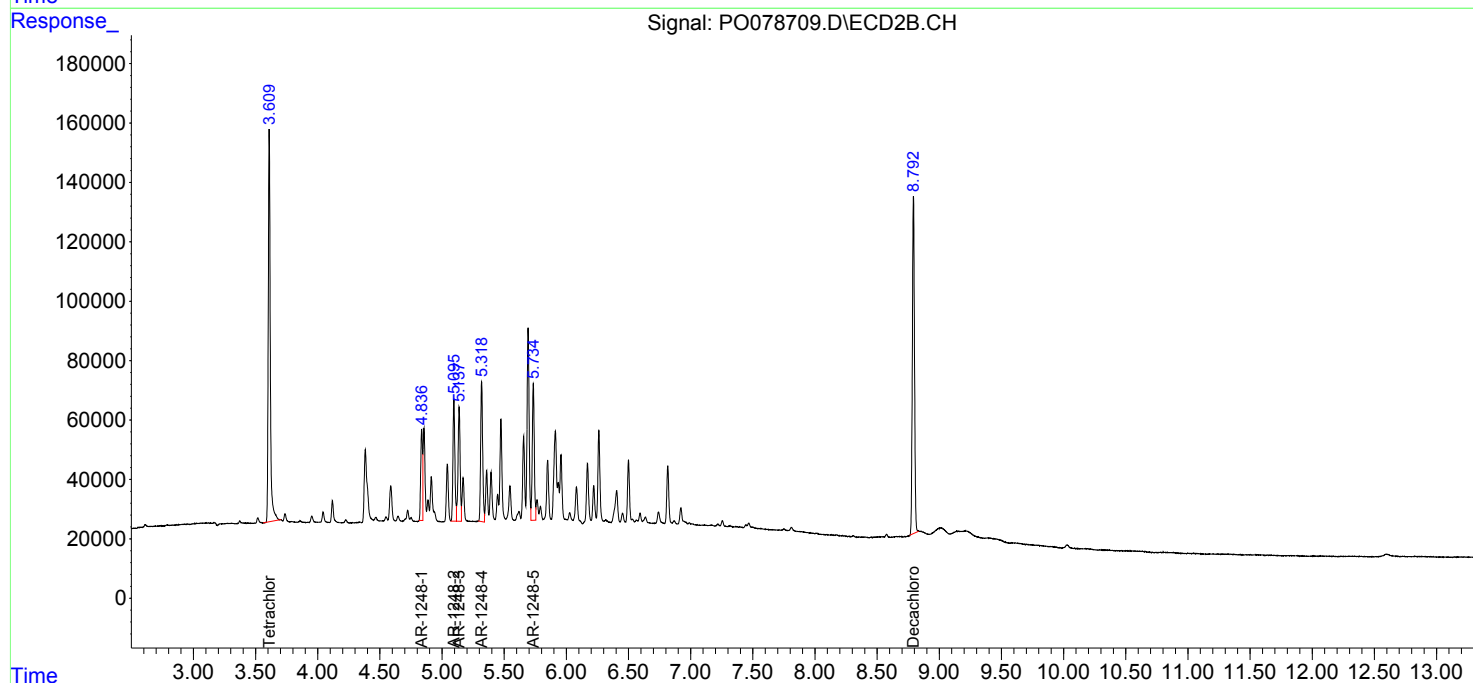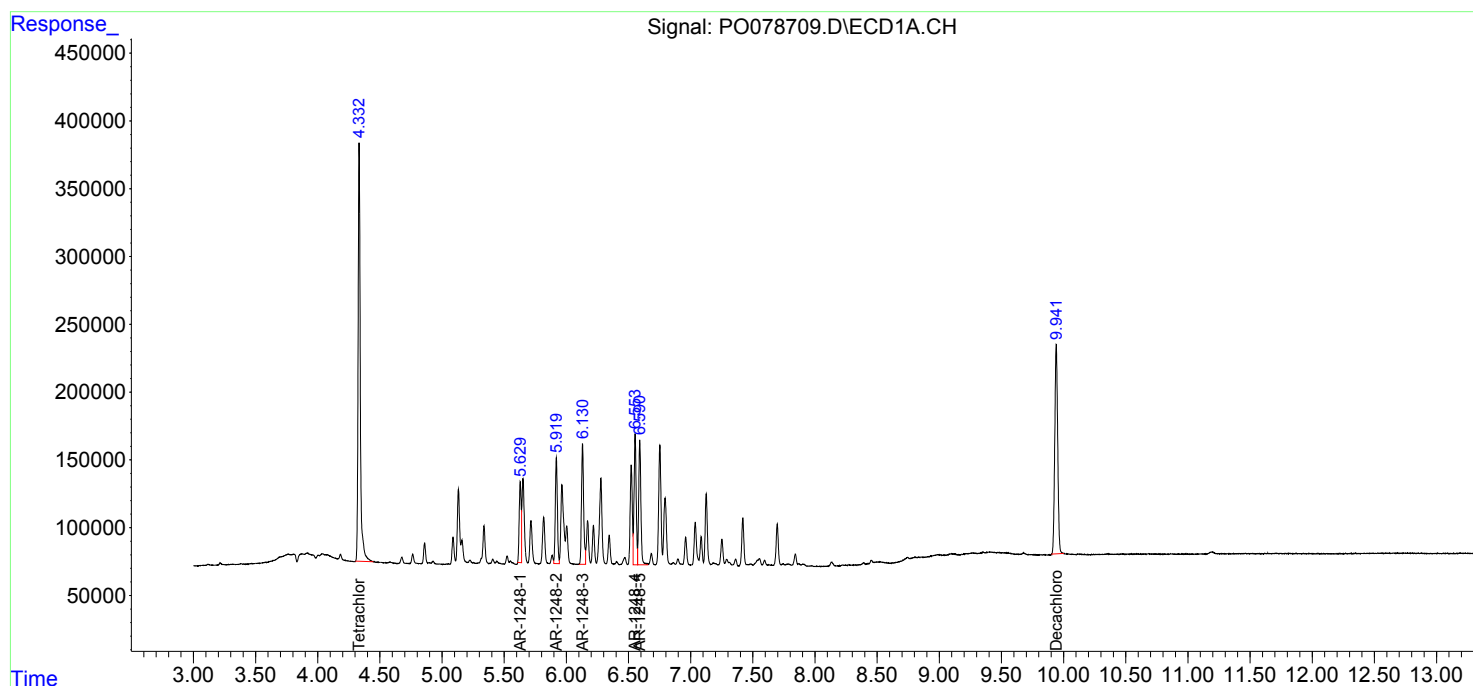

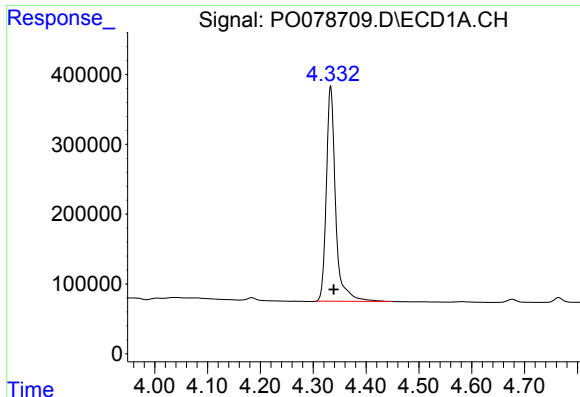


#1 Tetrachloro-m-xylene

R.T.: 4.333 min
Delta R.T.: -0.006 min
Response: 3759415
Conc: 49.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/14/2021 2:30:06 PM

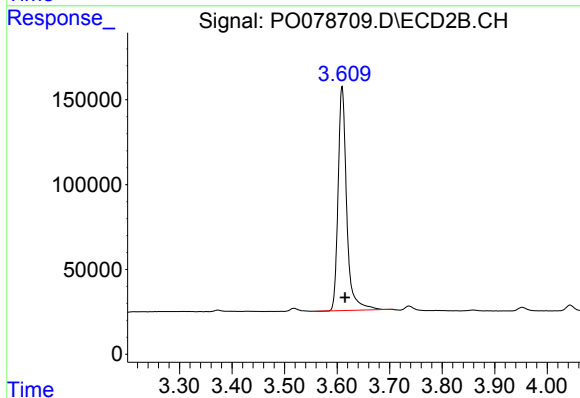


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.006 min
Response: 1503509
Conc: 47.59 ng/ml

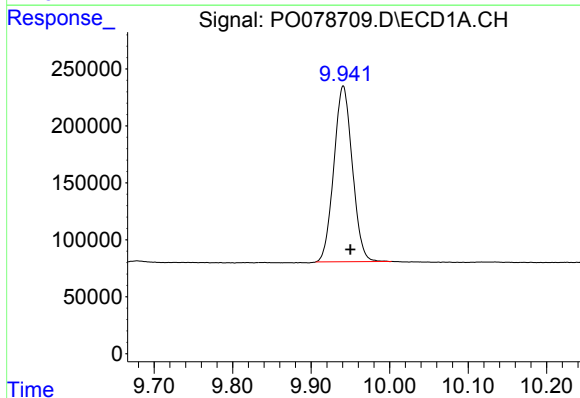


#2 Decachlorobiphenyl

R.T.: 9.941 min
Delta R.T.: -0.009 min
Response: 2525896
Conc: 62.29 ng/ml

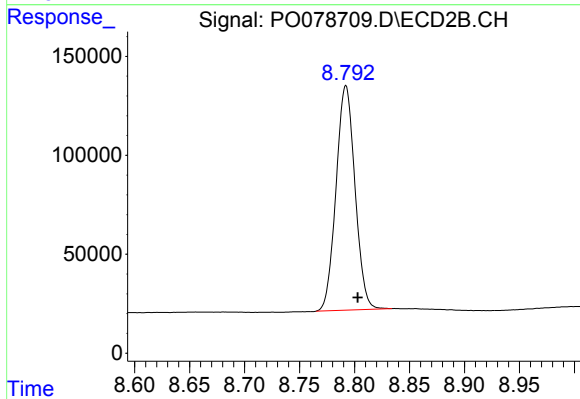

#2 Decachlorobiphenyl

R.T.: 8.792 min
Delta R.T.: -0.011 min
Response: 1360128
Conc: 56.56 ng/ml

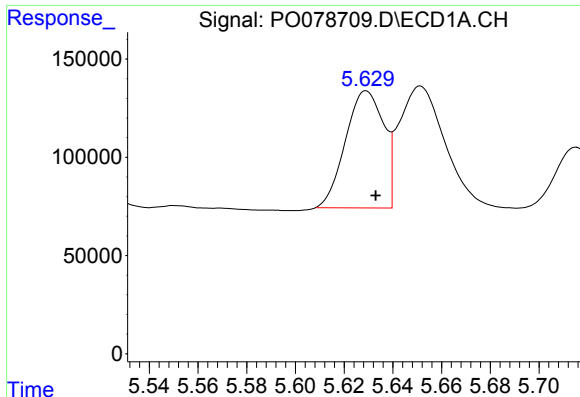


#21 AR-1248-1

R.T.: 5.629 min
Delta R.T.: -0.004 min
Response: 649756
Conc: 477.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/14/2021 2:30:06 PM

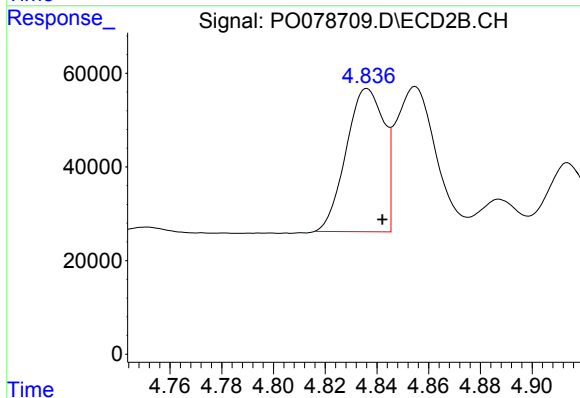


#21 AR-1248-1

R.T.: 4.836 min
Delta R.T.: -0.006 min
Response: 309476
Conc: 478.86 ng/ml

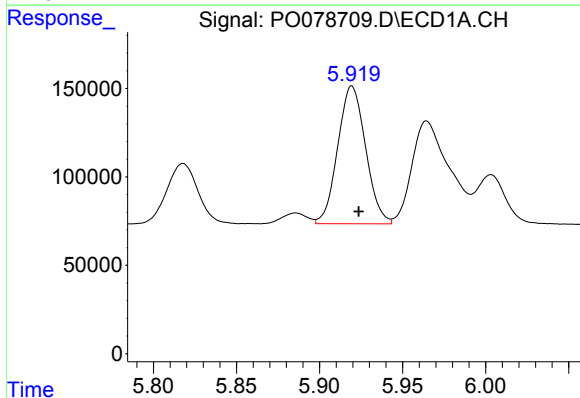


#22 AR-1248-2

R.T.: 5.919 min
Delta R.T.: -0.004 min
Response: 910618
Conc: 468.98 ng/ml

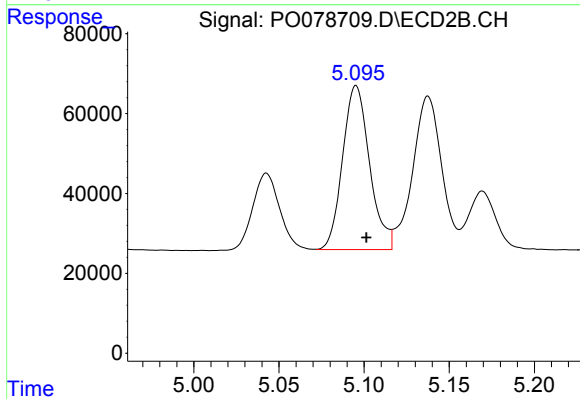

#22 AR-1248-2

R.T.: 5.095 min
Delta R.T.: -0.006 min
Response: 452962
Conc: 464.54 ng/ml

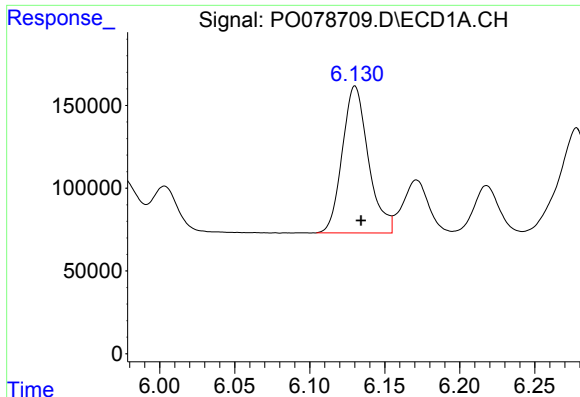


#23 AR-1248-3

R.T.: 6.130 min
Delta R.T.: -0.004 min
Response: 1071454
Conc: 474.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/14/2021 2:30:06 PM

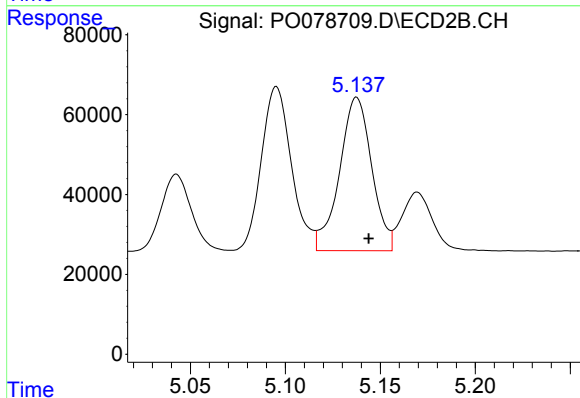


#23 AR-1248-3

R.T.: 5.138 min
Delta R.T.: -0.006 min
Response: 455173
Conc: 469.15 ng/ml

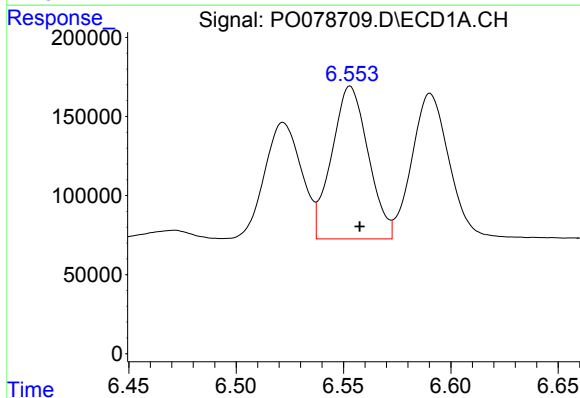


#24 AR-1248-4

R.T.: 6.553 min
Delta R.T.: -0.004 min
Response: 1142684
Conc: 482.32 ng/ml

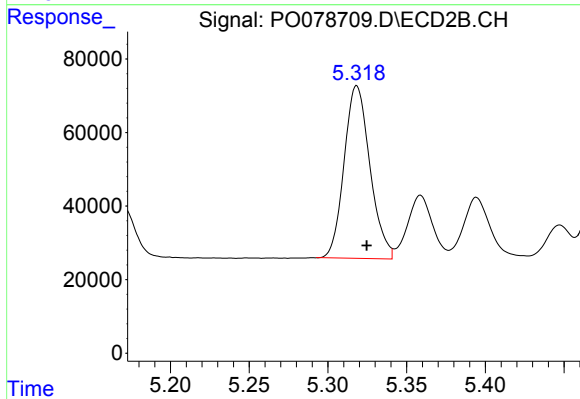

#24 AR-1248-4

R.T.: 5.318 min
Delta R.T.: -0.007 min
Response: 535597
Conc: 462.38 ng/ml m

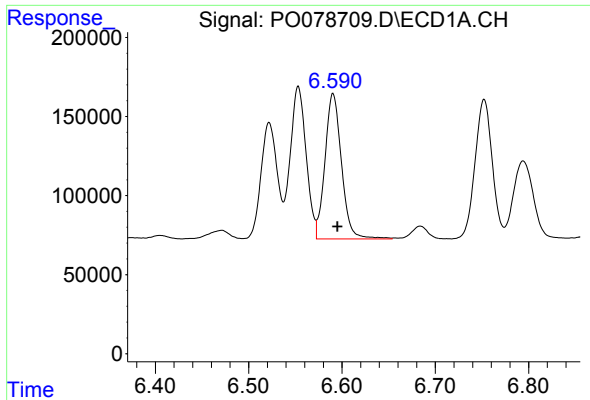


#25 AR-1248-5

R.T.: 6.590 min
Delta R.T.: -0.005 min
Response: 1132341
Conc: 486.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
6/14/2021 2:30:06 PM

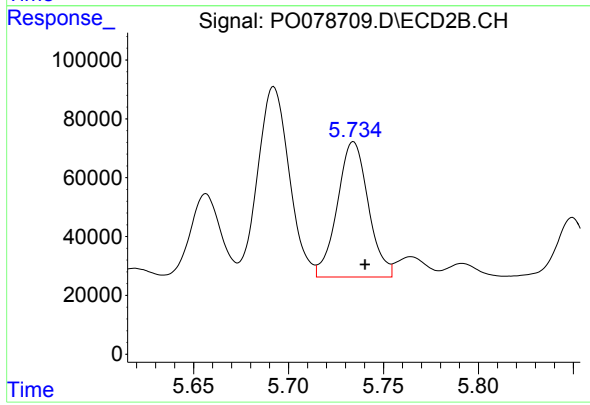

#25 AR-1248-5

R.T.: 5.734 min
Delta R.T.: -0.006 min
Response: 522465
Conc: 476.53 ng/ml