

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061220\
 Data File : P0068927.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2020 15:40
 Operator : DD\AJ
 Sample : L2932-13 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-042720-SR-13

Manual Integrations
 APPROVED

Sohil
 6/15/2020 3:57:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:40:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 13 01:32:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.410	3.567	67068	93998	2.458	2.646
2) SA Decachlor...	10.077	8.791	895813	891534	19.949	17.422m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061220\
Data File : P0068927.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2020 15:40
Operator : DD\AJ
Sample : L2932-13 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-042720-SR-13


Manual Integrations
APPROVED

Sohil
6/15/2020 3:57:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:40:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 13 01:32:21 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

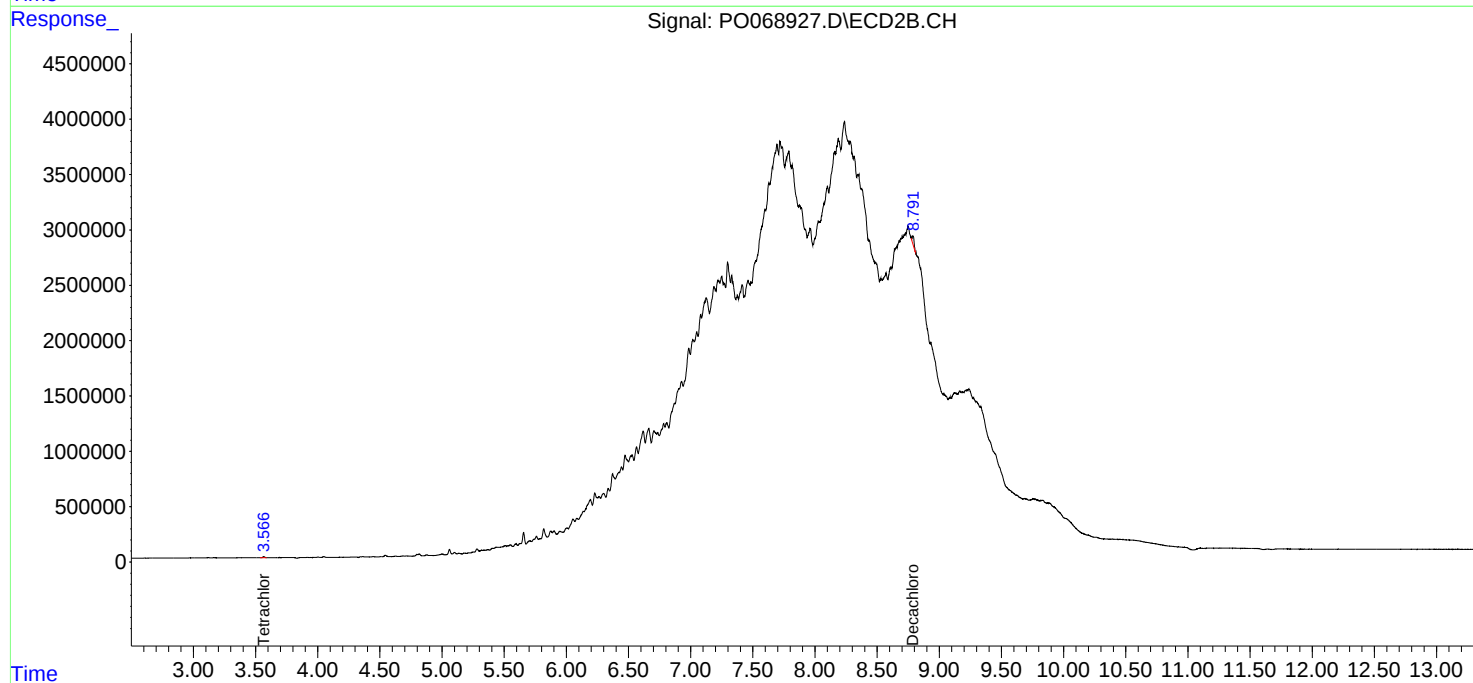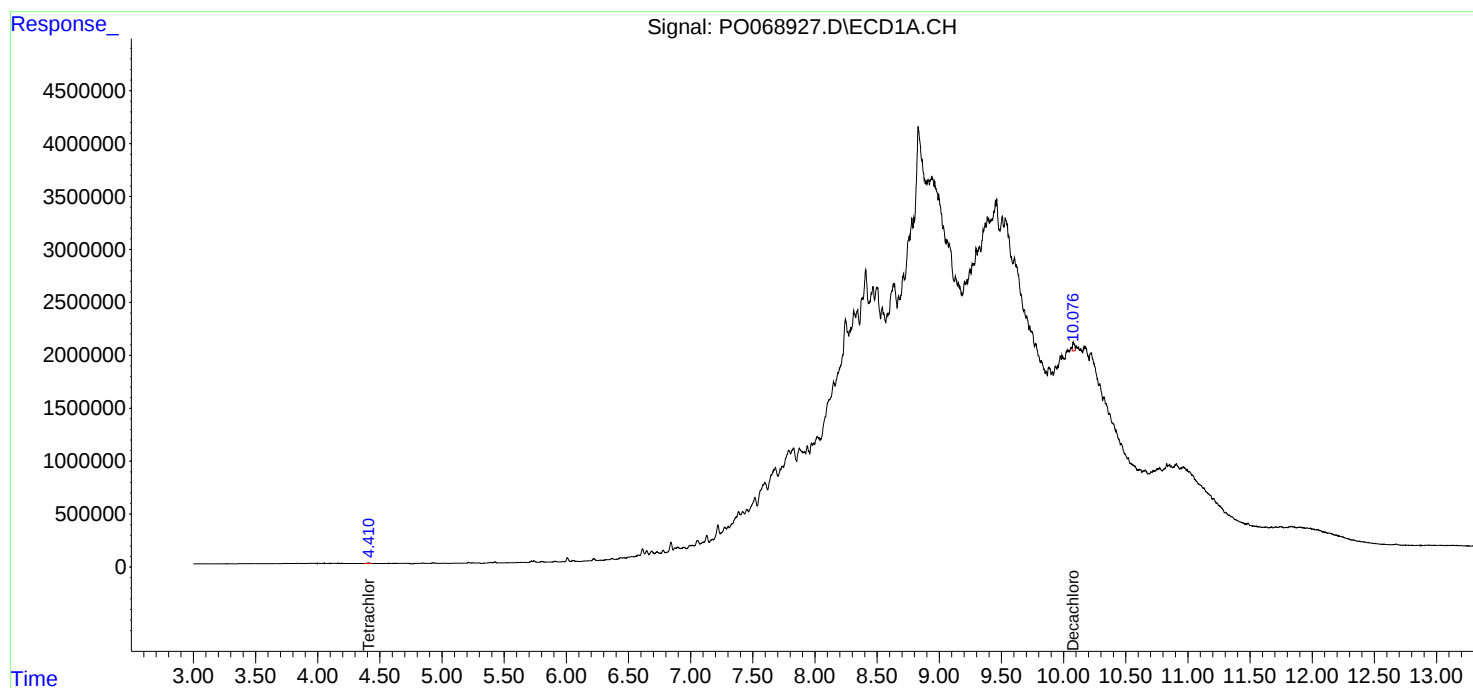

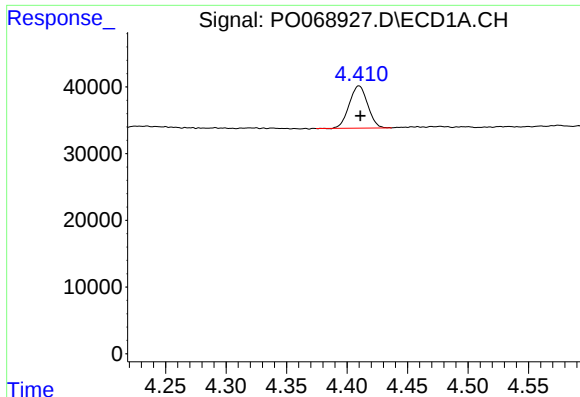


#1 Tetrachloro-m-xylene

R.T.: 4.410 min
Delta R.T.: -0.001 min
Response: 67068
Conc: 2.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-042720-SR-13


Manual Integrations
APPROVED

Sohil
6/15/2020 3:57:05 PM

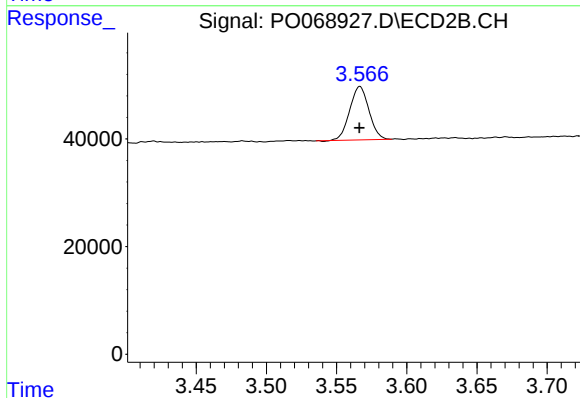


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 93998
Conc: 2.65 ng/ml

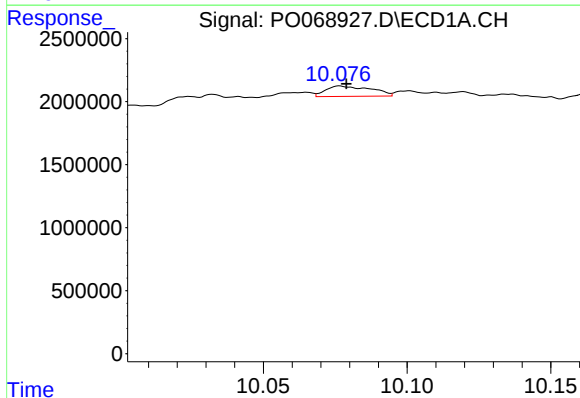

#2 Decachlorobiphenyl

R.T.: 10.077 min
Delta R.T.: -0.002 min
Response: 895813
Conc: 19.95 ng/ml

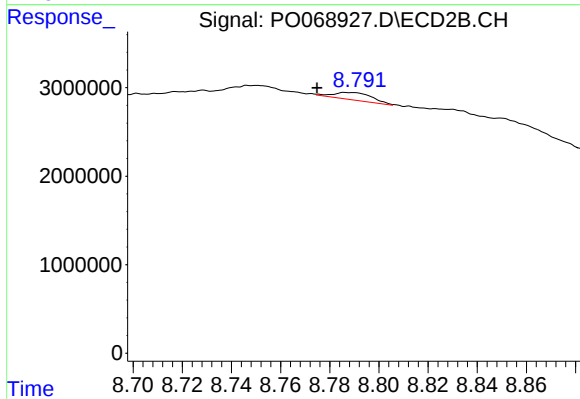

#2 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.016 min
Response: 891534
Conc: 17.42 ng/ml m