

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061321\
 Data File : P0078735.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2021 16:10
 Operator : DD\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 6/14/2021 4:49:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:04:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 02:03:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.606	413985	185933	4.989	5.609
2) SA Decachlor...	9.937	8.789	328798	182306	5.774	6.121m
Target Compounds						
26) L6 AR-1254-1	6.521	5.689	154065	102770	56.634	59.072
27) L6 AR-1254-2	6.747	5.847	240322	96084	57.439	60.848
28) L6 AR-1254-3	7.123	6.260	241579	143718	55.627	60.547
29) L6 AR-1254-4	7.417	6.498	167010	86585	54.370	58.828
30) L6 AR-1254-5	7.839	6.920	184194	126991	53.233m	55.633

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061321\
Data File : P0078735.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2021 16:10
Operator : DD\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/14/2021 4:49:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:04:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 02:03:15 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

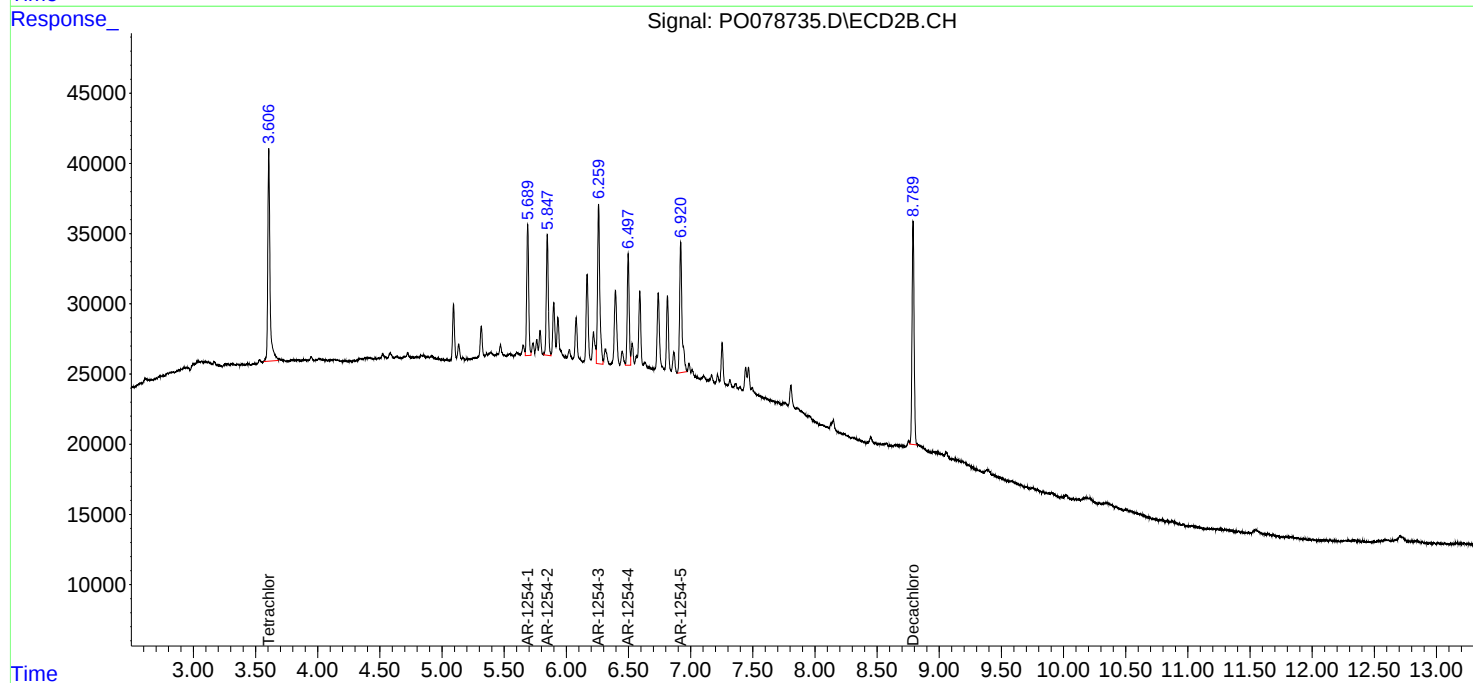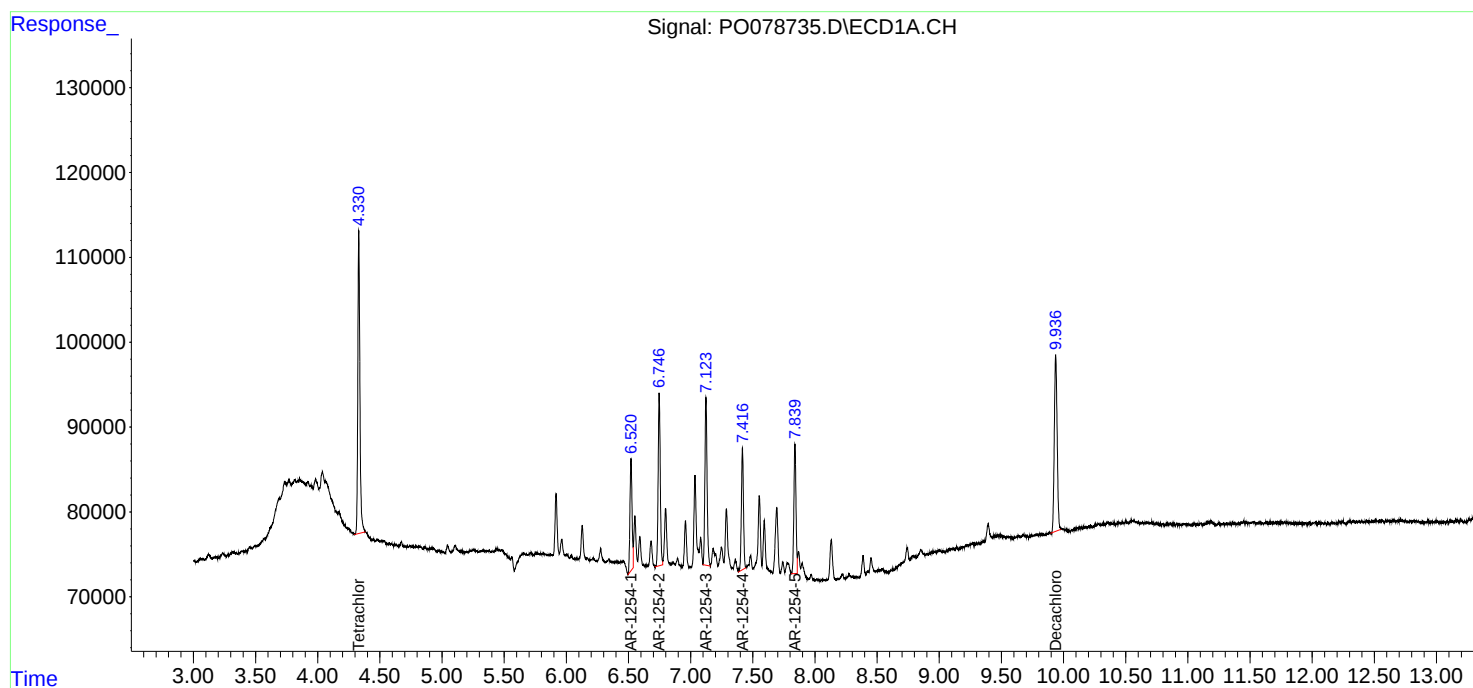

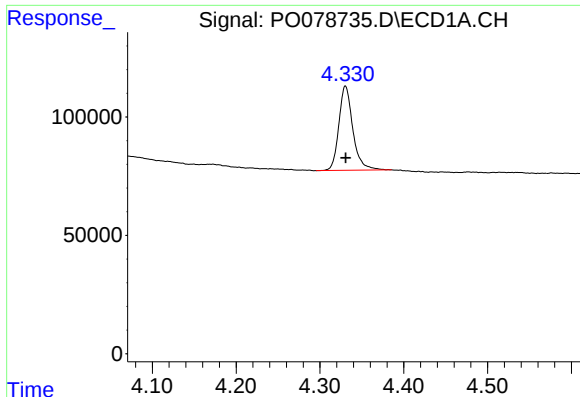


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 413985
Conc: 4.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/14/2021 4:49:02 PM

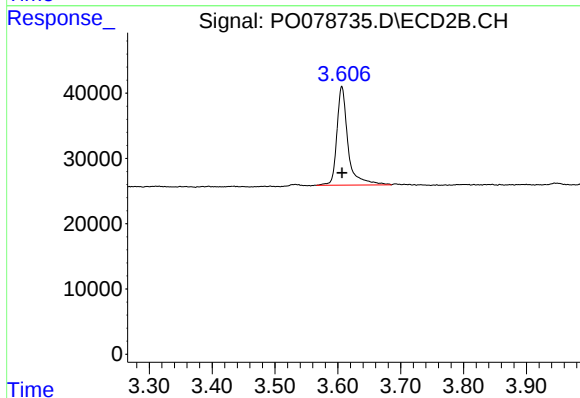


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 185933
Conc: 5.61 ng/ml

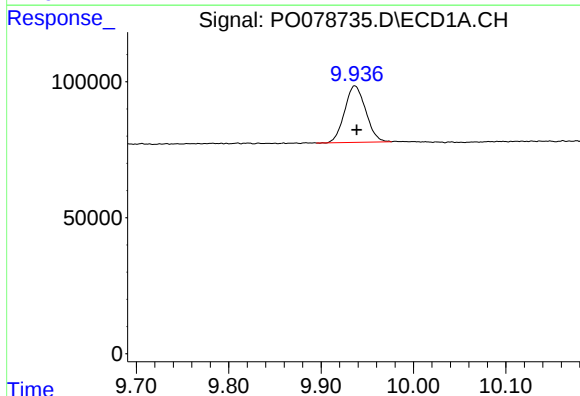


#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.002 min
Response: 328798
Conc: 5.77 ng/ml

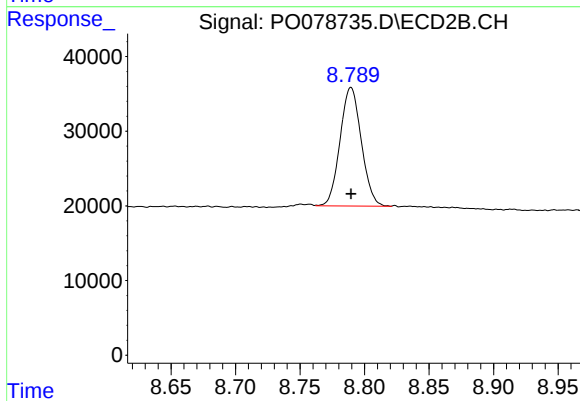

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 182306
Conc: 6.12 ng/ml m

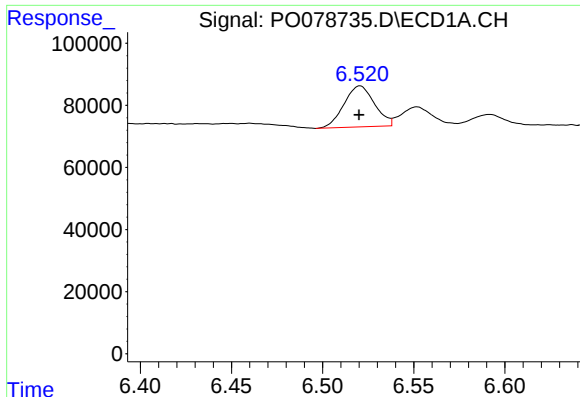


#26 AR-1254-1

R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 154065
Conc: 56.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/14/2021 4:49:02 PM

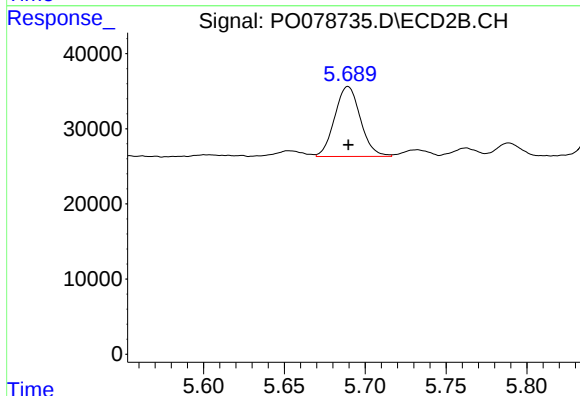


#26 AR-1254-1

R.T.: 5.689 min
Delta R.T.: 0.000 min
Response: 102770
Conc: 59.07 ng/ml

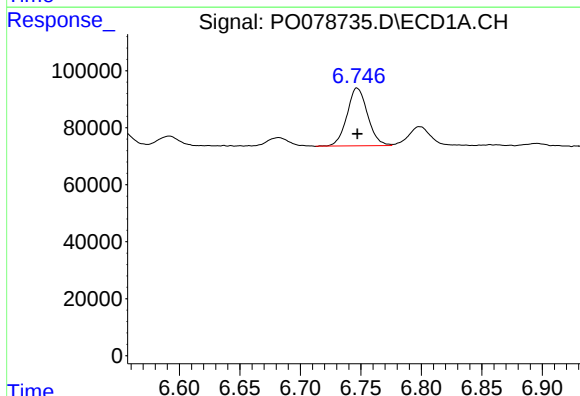


#27 AR-1254-2

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 240322
Conc: 57.44 ng/ml

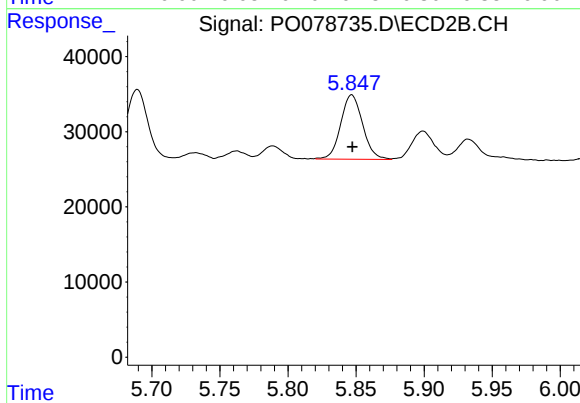

#27 AR-1254-2

R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 96084
Conc: 60.85 ng/ml

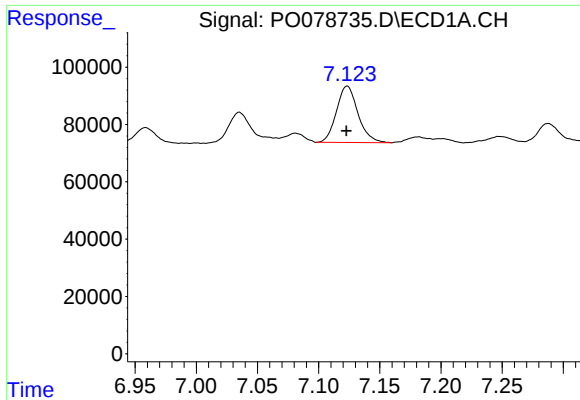


#28 AR-1254-3

R.T.: 7.123 min
Delta R.T.: 0.000 min
Response: 241579
Conc: 55.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/14/2021 4:49:02 PM

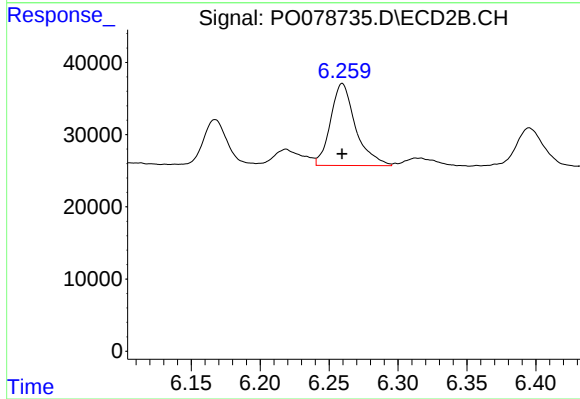


#28 AR-1254-3

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 143718
Conc: 60.55 ng/ml

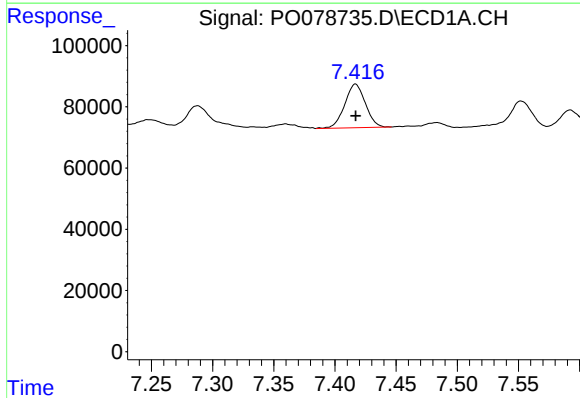


#29 AR-1254-4

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 167010
Conc: 54.37 ng/ml

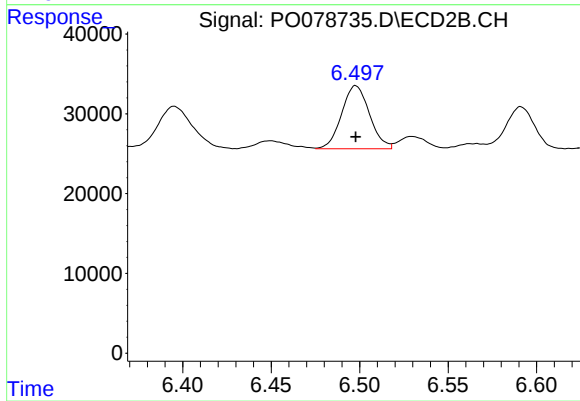

#29 AR-1254-4

R.T.: 6.498 min
Delta R.T.: 0.000 min
Response: 86585
Conc: 58.83 ng/ml

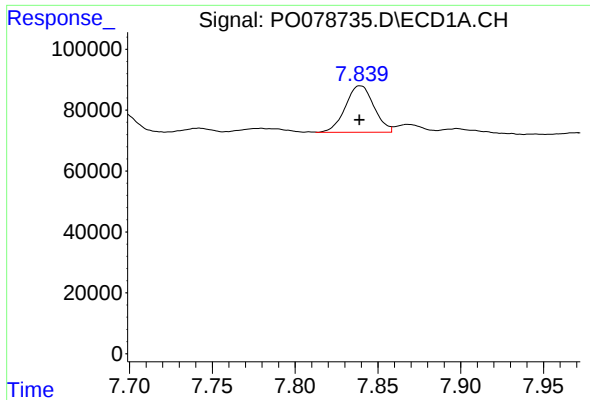


#30 AR-1254-5

R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 184194
Conc: 53.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
6/14/2021 4:49:02 PM

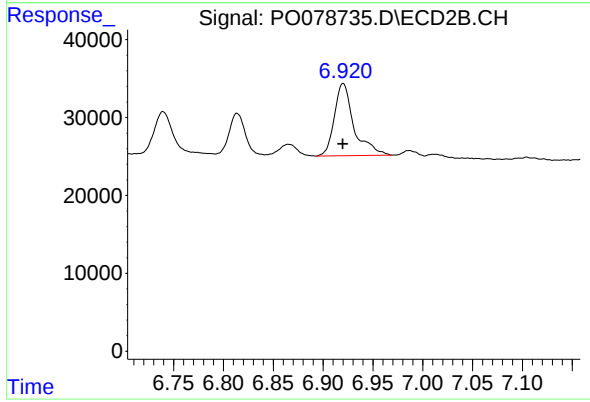

#30 AR-1254-5

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 126991
Conc: 55.63 ng/ml