

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061322\
 Data File : P0087123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2022 17:21
 Operator : YP/AJ
 Sample : N3304-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-14A-1A-9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/14/2022
 Supervised By :Ankita Jodhani 06/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 17:55:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.498	3.650	30976751	18193616	13.255m	16.159m
2) SA Decachlor...	10.377	8.679	28621103	14181145	15.552	18.036

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061322\
Data File : PO087123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2022 17:21
Operator : YP/AJ
Sample : N3304-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-14A-1A-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 17:55:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

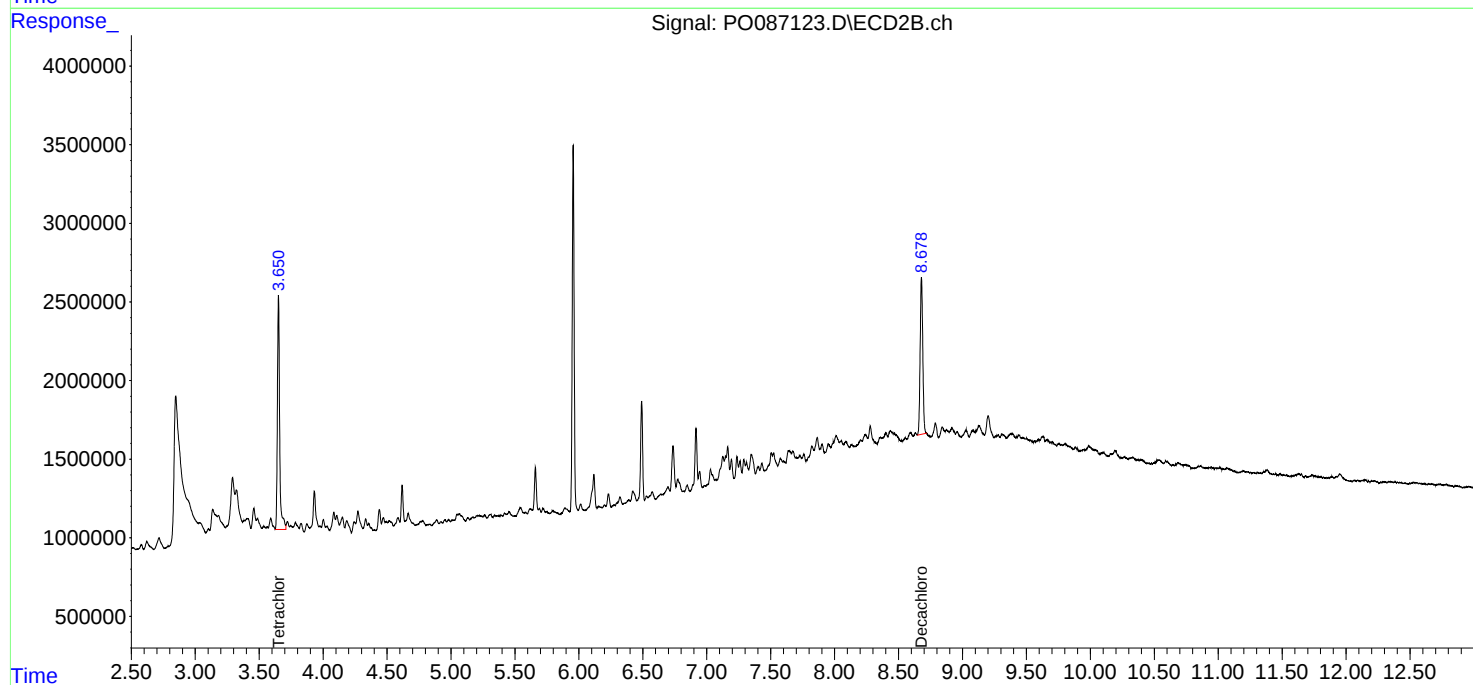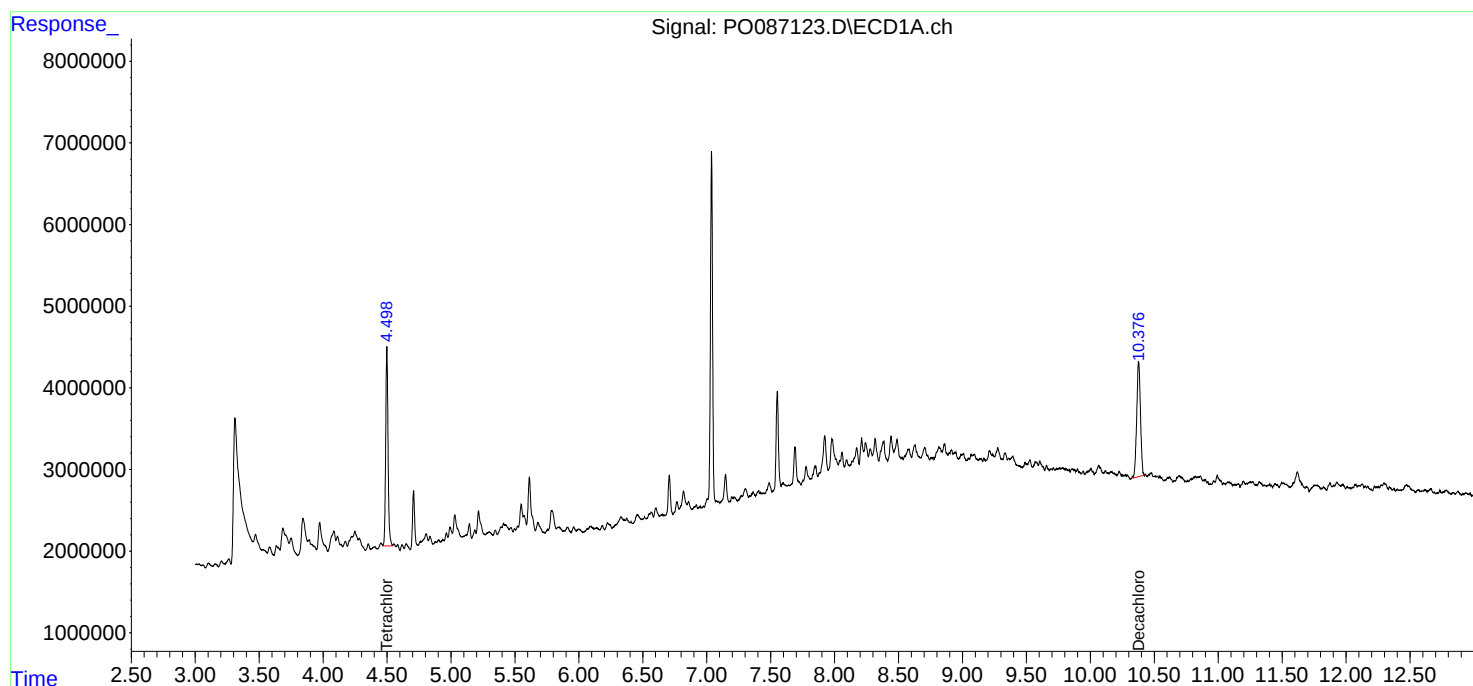

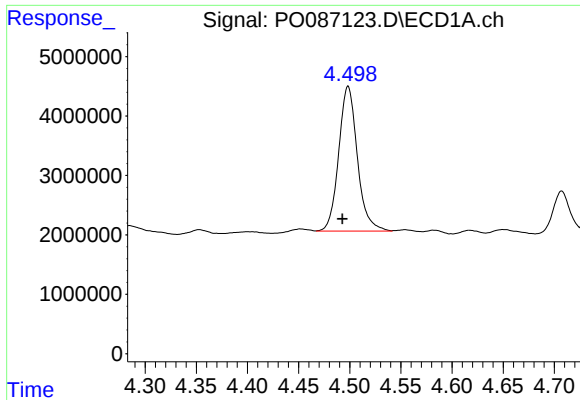


#1 Tetrachloro-m-xylene

R.T.: 4.498 min
Delta R.T.: 0.005 min
Response: 30976751
Conc: 13.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-14A-1A-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

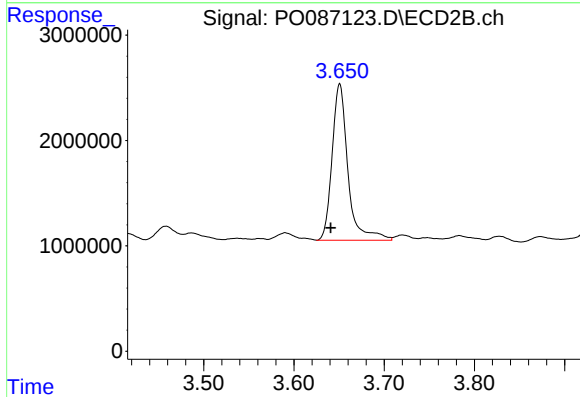


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.009 min
Response: 18193616
Conc: 16.16 ng/ml m

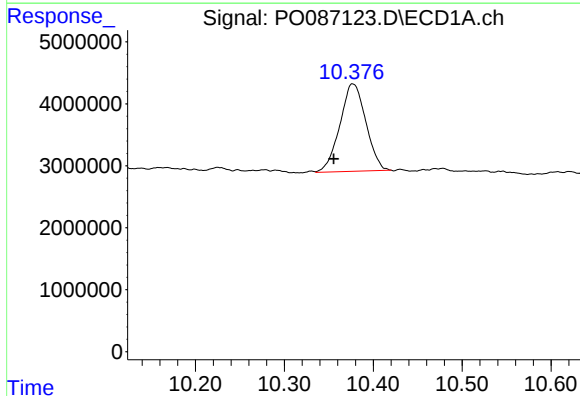

#2 Decachlorobiphenyl

R.T.: 10.377 min
Delta R.T.: 0.021 min
Response: 28621103
Conc: 15.55 ng/ml

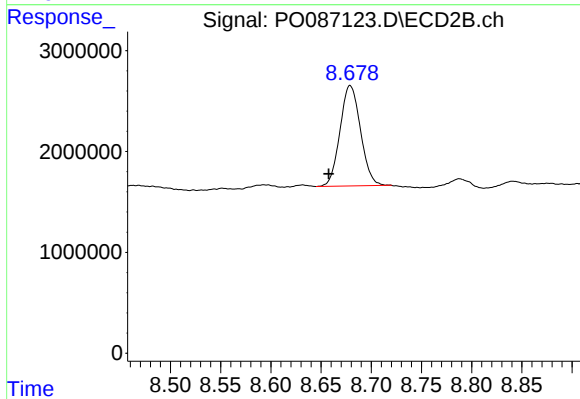

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: 0.022 min
Response: 14181145
Conc: 18.04 ng/ml