

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045784.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2018 19:57
Operator : SM/UA
Sample : PB110225BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB110225BL

Manual Integrations
APPROVED

ugo
6/15/2018 6:56:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 08:35:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

	System Monitoring Compounds						
1)	SA Tetrachlo...	4.395	3.623	3414118	1895792	17.401	20.229
2)	SA Decachlor...	10.061	8.609	2766383	1375461	13.725m	17.413 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045784.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2018 19:57
Operator : SM/UA
Sample : PB110225BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB110225BL


Manual Integrations
APPROVED

ugo
6/15/2018 6:56:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 08:35:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

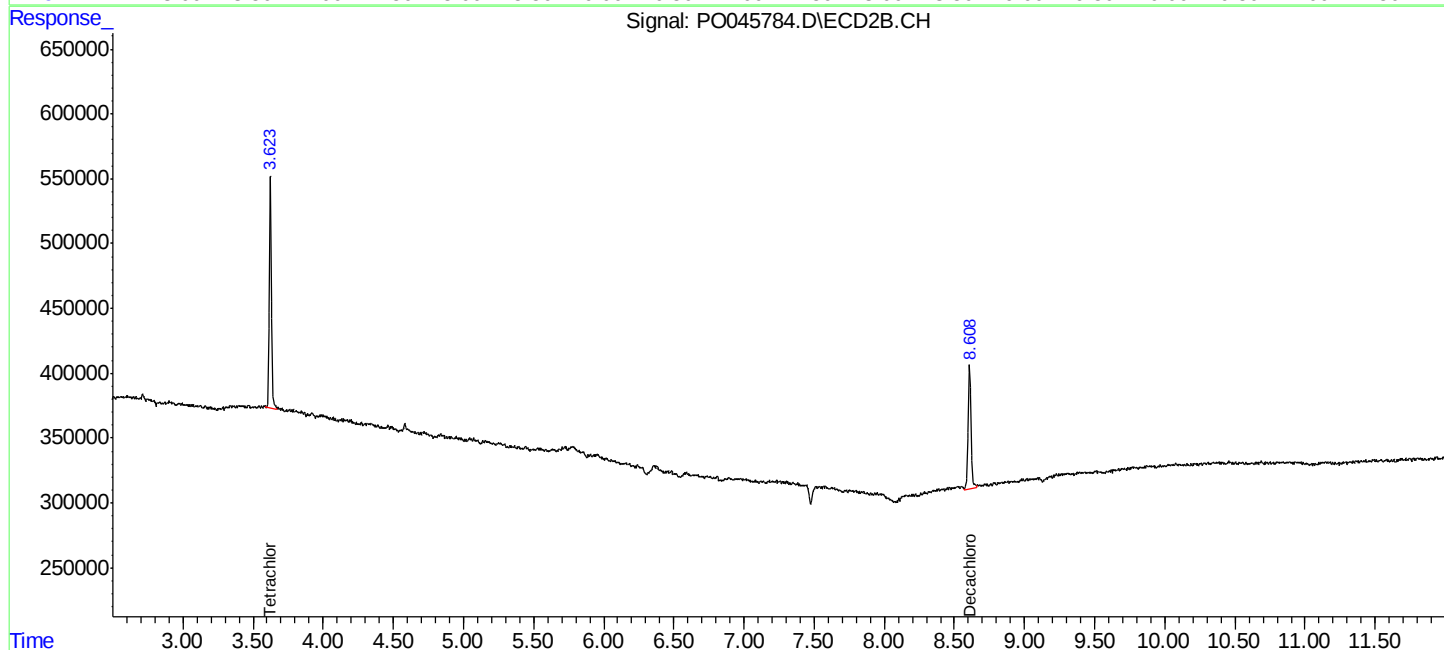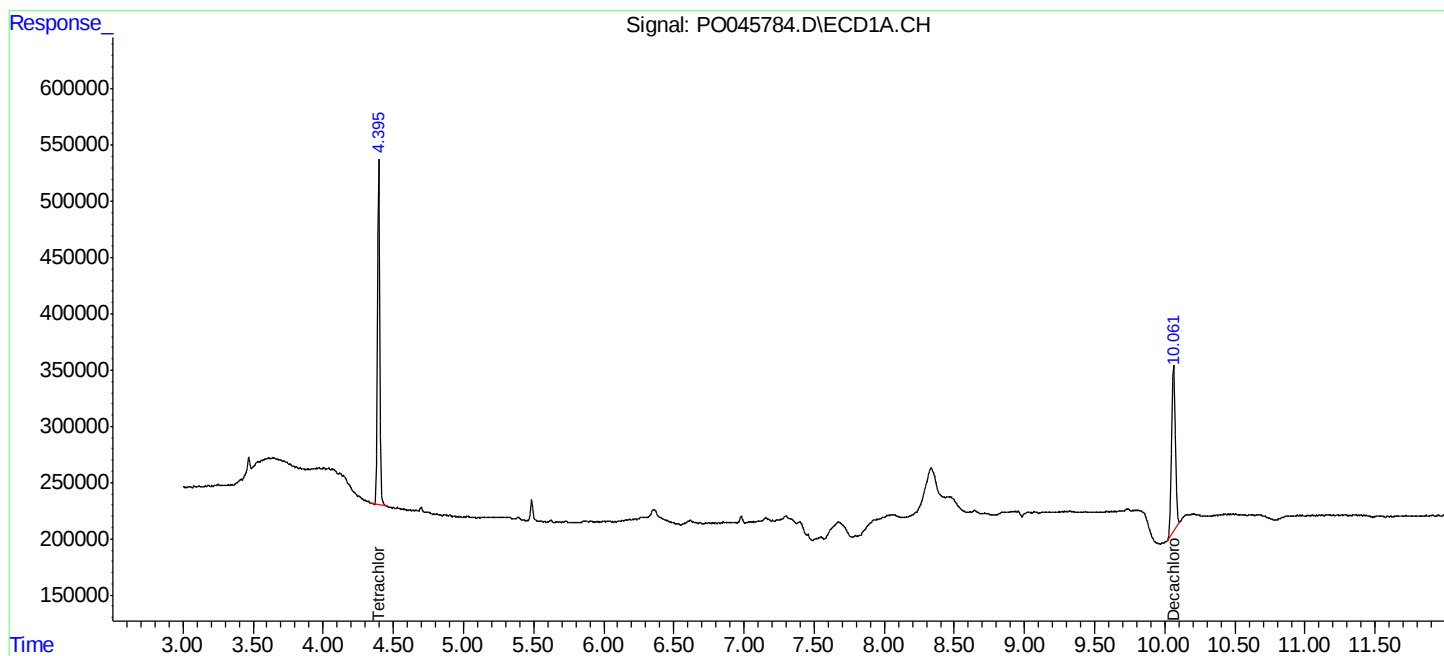

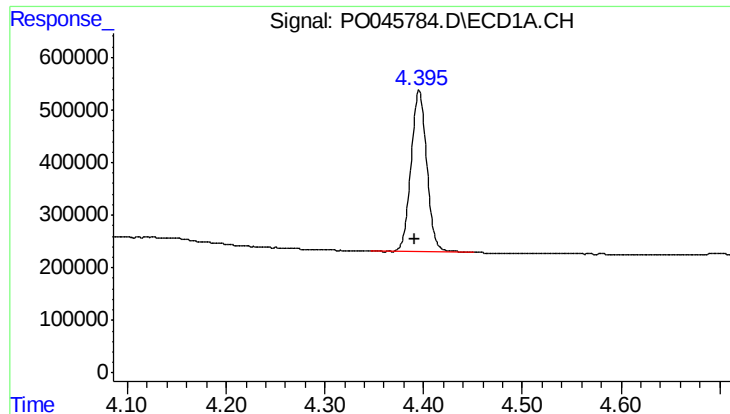


#1 Tetrachloro-m-xylene

R.T.: 4.395 min
Delta R.T.: 0.005 min
Response: 3414118
Conc: 17.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB110225BL


Manual Integrations
APPROVED

ugo
6/15/2018 6:56:45 PM

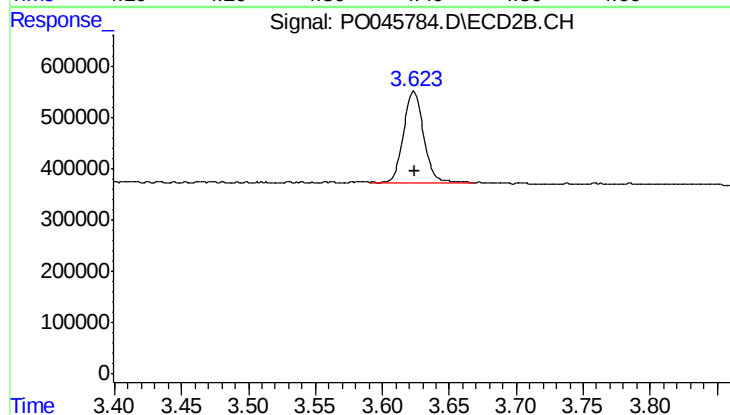


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.001 min
Response: 1895792
Conc: 20.23 ng/ml

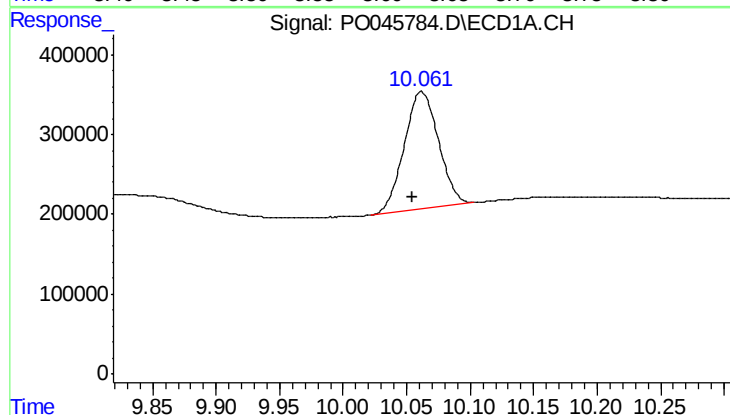

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: 0.006 min
Response: 2766383
Conc: 13.73 ng/ml m

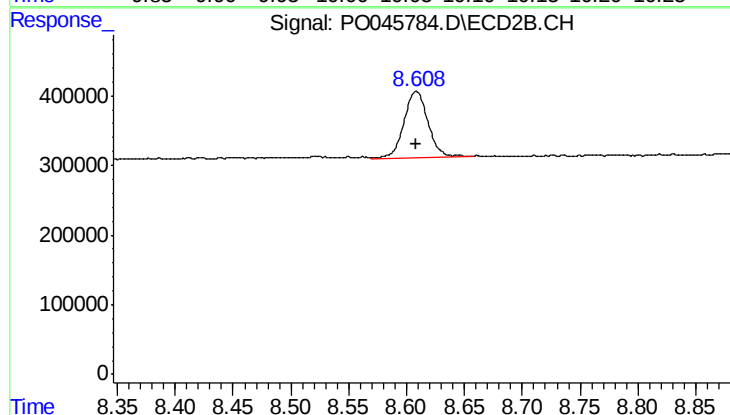

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: 0.000 min
Response: 1375461
Conc: 17.41 ng/ml