

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
 Data File : P0045789.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2018 21:16
 Operator : SM/UA
 Sample : J3241-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-05-061318-A

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 08:42:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 15 08:20:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	ugo

System Monitoring Compounds							
1) SA Tetrachlo...	4.390	3.624	4175460	2417692	21.282m	25.797	
2) SA Decachlor...	10.054	8.605	3256272	1134573	16.156	14.363	6/15/2018 6:56:35 PM

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045789.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2018 21:16
Operator : SM/UA
Sample : J3241-07
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
HR-05-061318-A

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 08:42:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

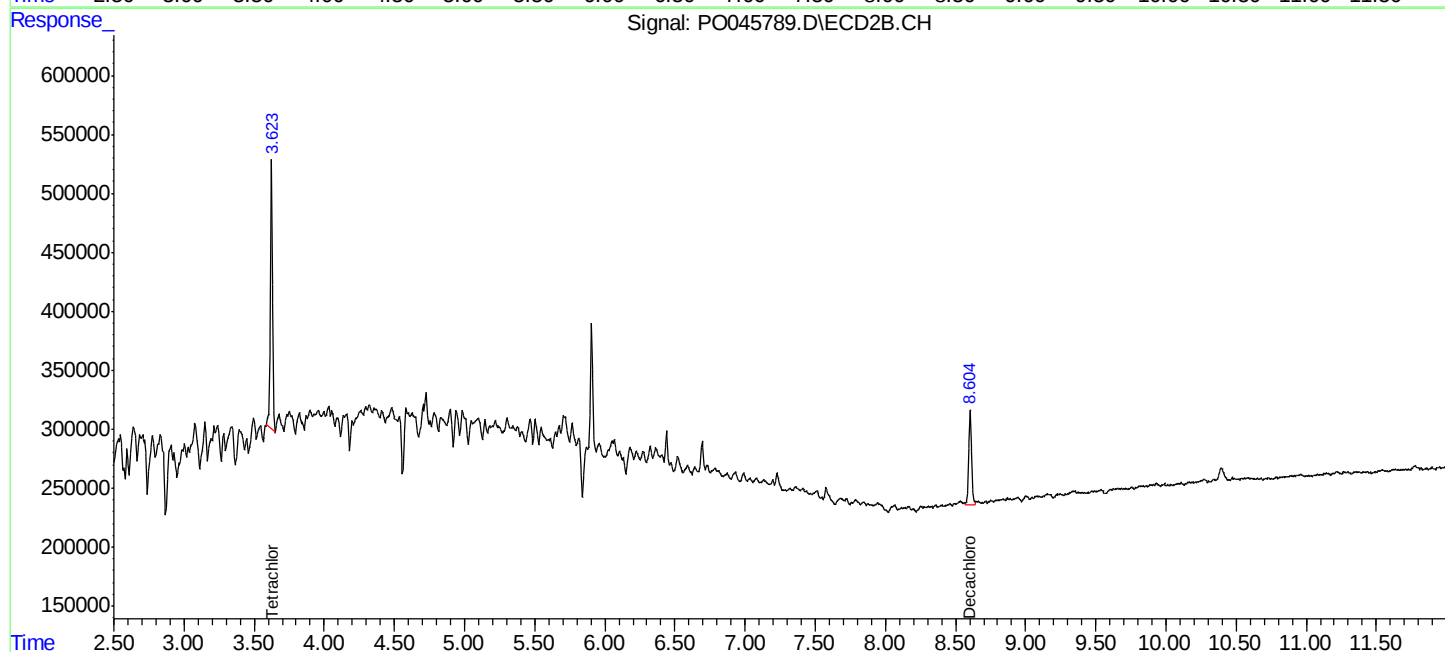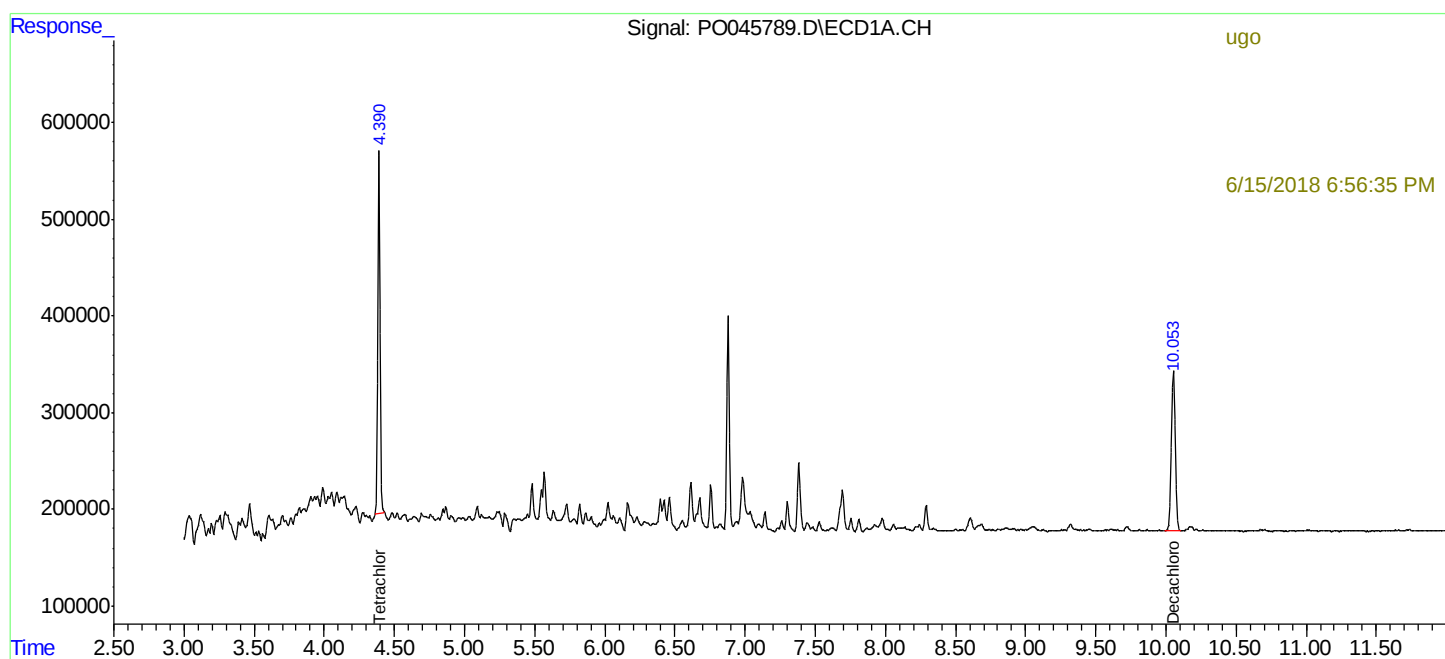

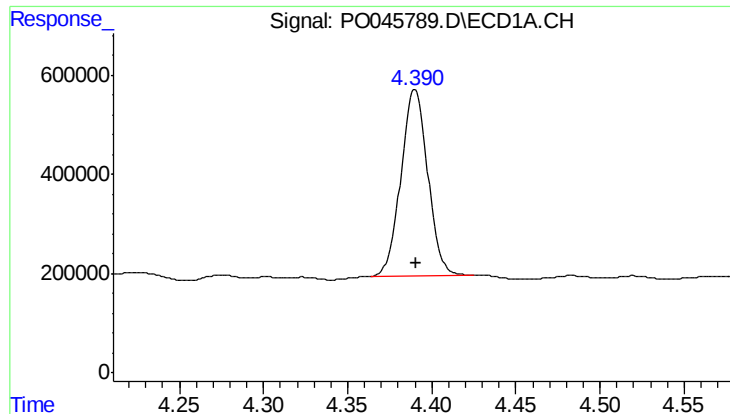


#1 Tetrachloro-m-xylene

R.T.: 4.390 min
Delta R.T.: -0.001 min
Response: 4175460
Conc: 21.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-05-061318-A


Manual Integrations
APPROVED

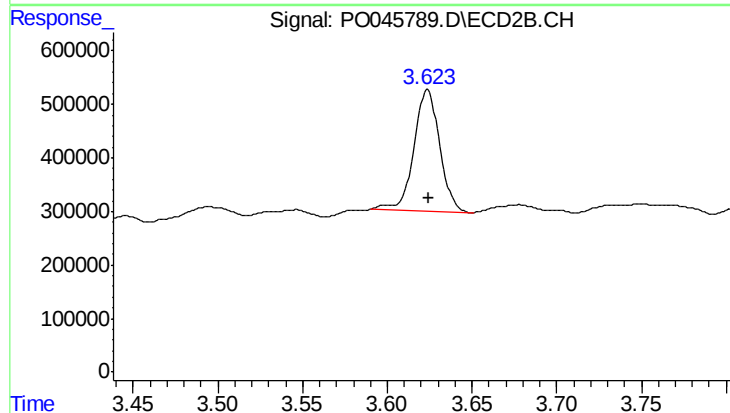

#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 2417692
Conc: 25.80 ng/ml


ugo

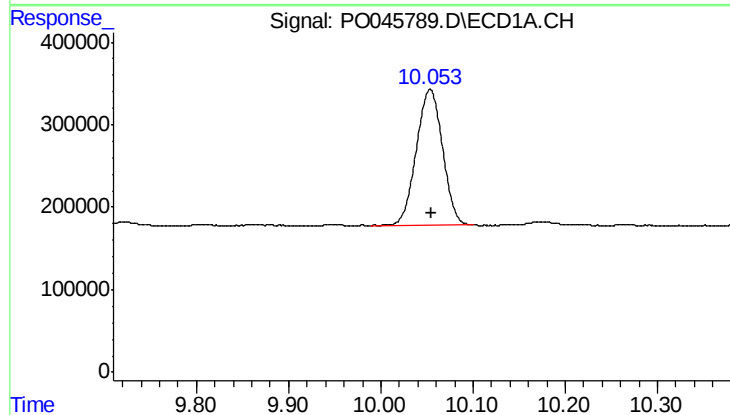

#2 Decachlorobiphenyl

6/15/2018 6:56:35 PM

R.T.: 10.054 min
Delta R.T.: -0.001 min
Response: 3256272
Conc: 16.16 ng/ml

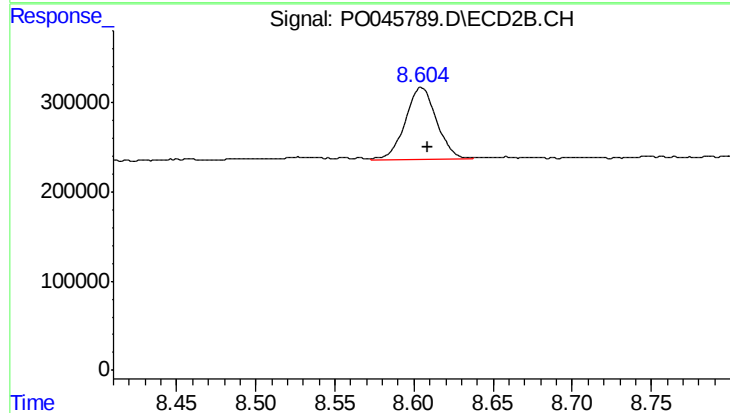

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: -0.004 min
Response: 1134573
Conc: 14.36 ng/ml