

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
 Data File : P0045790.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2018 21:32
 Operator : SM/UA
 Sample : J3241-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-05-061318-B

Manual Integrations
 APPROVED

ugo
 6/15/2018 6:56:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 08:45:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 15 08:20:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.390	3.624	6357735	3729620	32.405m	39.796
2) SA Decachlor...	10.054	8.606	4930398	1654600	24.462	20.947

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045790.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2018 21:32
Operator : SM/UA
Sample : J3241-09
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HR-05-061318-B


Manual Integrations
APPROVED

ugo
6/15/2018 6:56:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 08:45:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

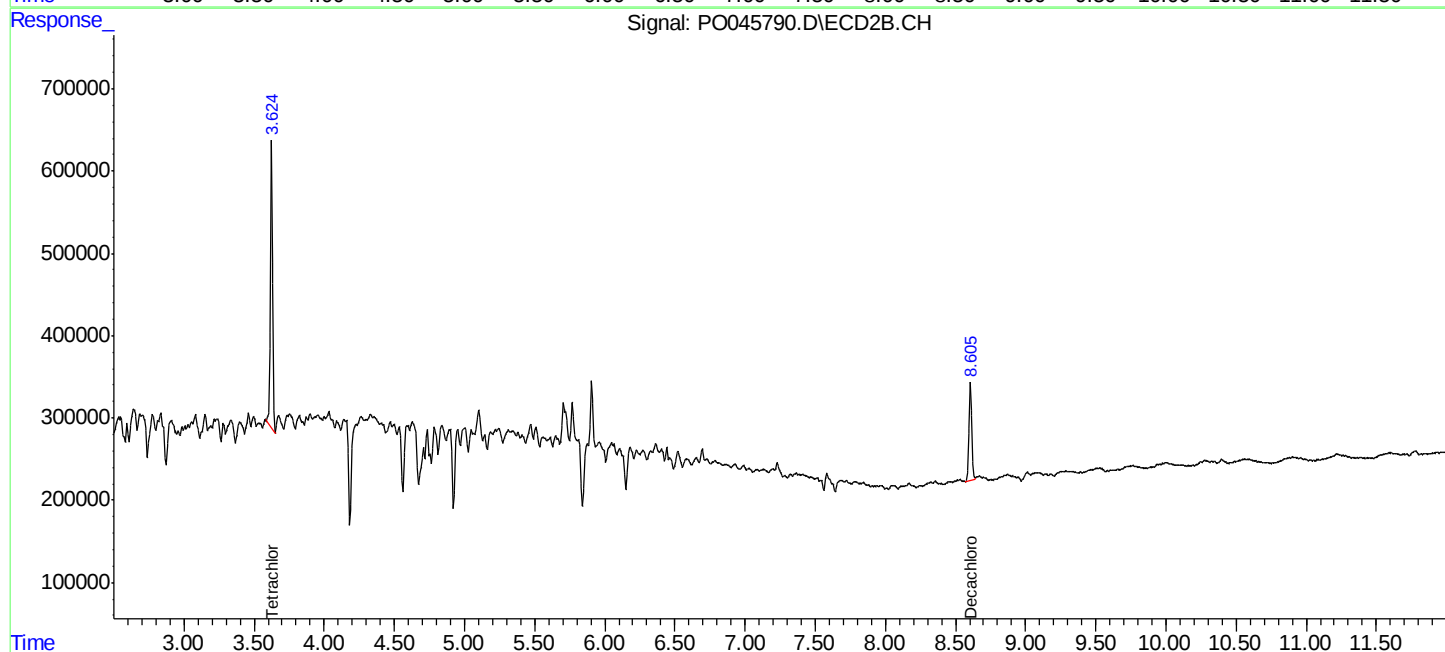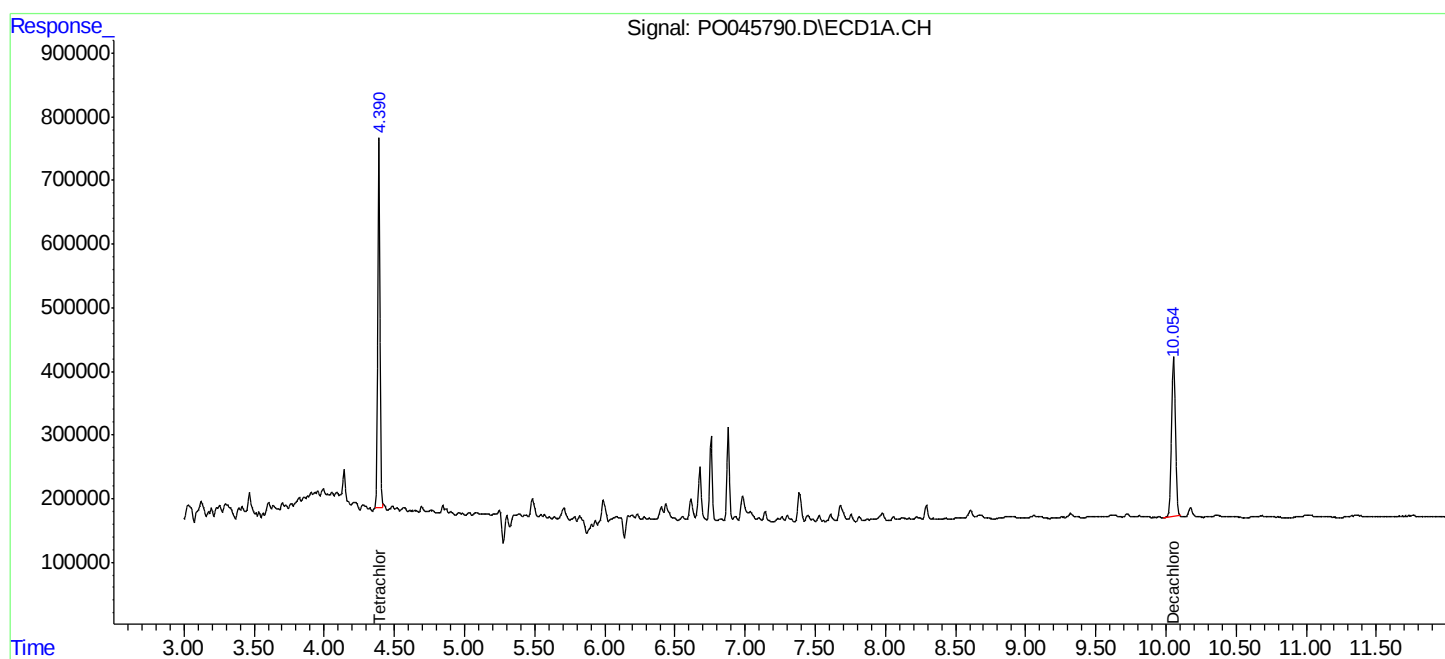

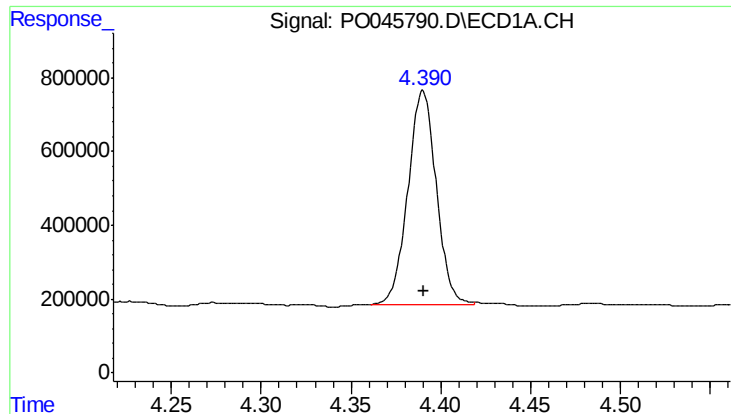


#1 Tetrachloro-m-xylene

R.T.: 4.390 min
Delta R.T.: -0.001 min
Response: 6357735
Conc: 32.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-05-061318-B


Manual Integrations
APPROVED

ugo
6/15/2018 6:56:32 PM

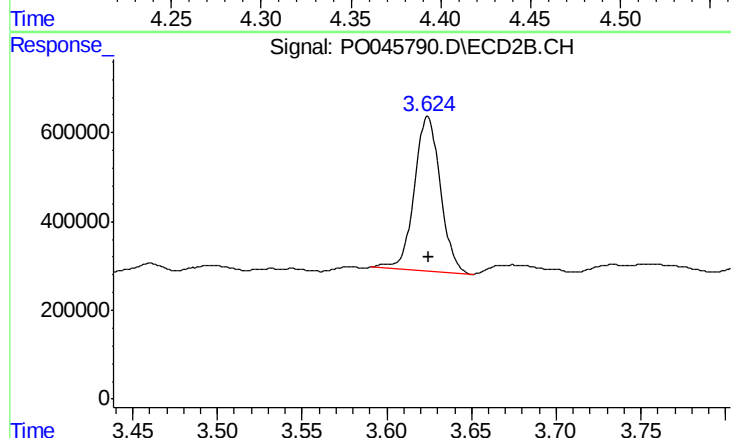


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 3729620
Conc: 39.80 ng/ml

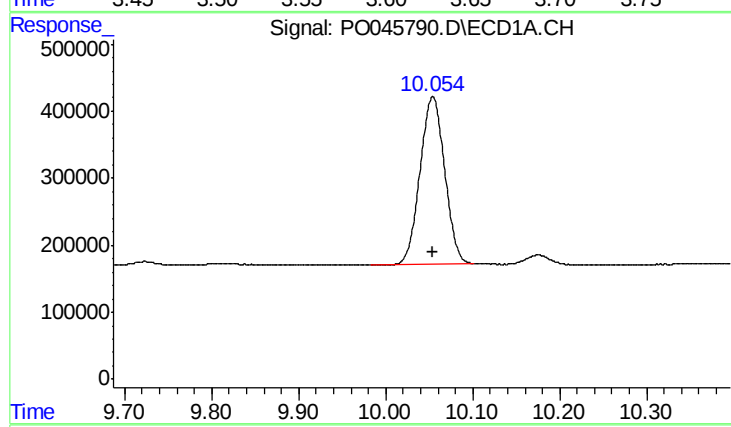

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: 0.000 min
Response: 4930398
Conc: 24.46 ng/ml

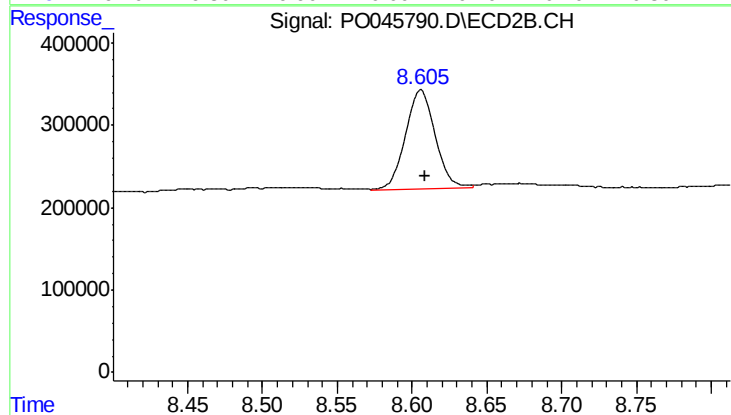

#2 Decachlorobiphenyl

R.T.: 8.606 min
Delta R.T.: -0.003 min
Response: 1654600
Conc: 20.95 ng/ml