

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
 Data File : P0045804.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jun 2018 1:15
 Operator : SM/UA
 Sample : PB110231BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB110231BL

Manual Integrations
 APPROVED

ugo
 6/15/2018 6:55:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 08:52:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 15 08:20:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.390	3.623	5215699	2472032	26.584	26.377
2) SA Decachlor...	10.054	8.604	3432872	1439030	17.032	18.218

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045804.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2018 1:15
Operator : SM/UA
Sample : PB110231BL
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB110231BL


Manual Integrations
APPROVED

ugo
6/15/2018 6:55:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 08:52:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

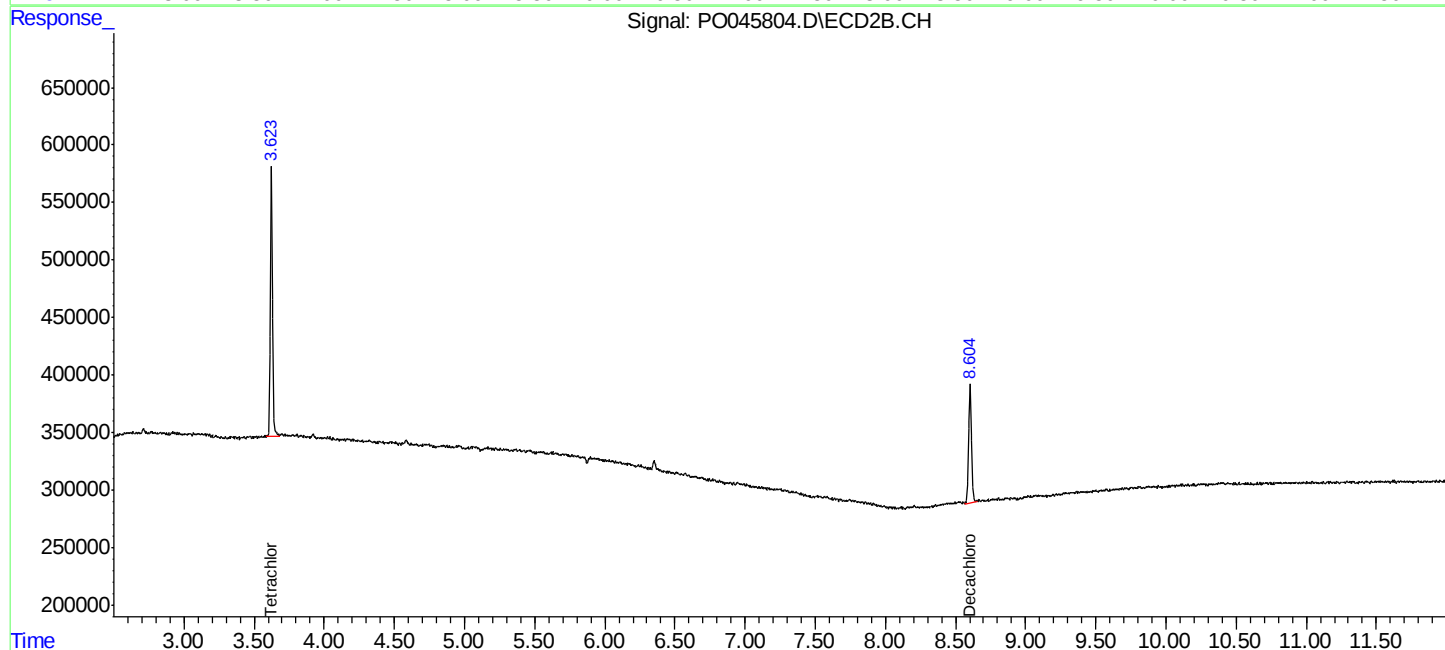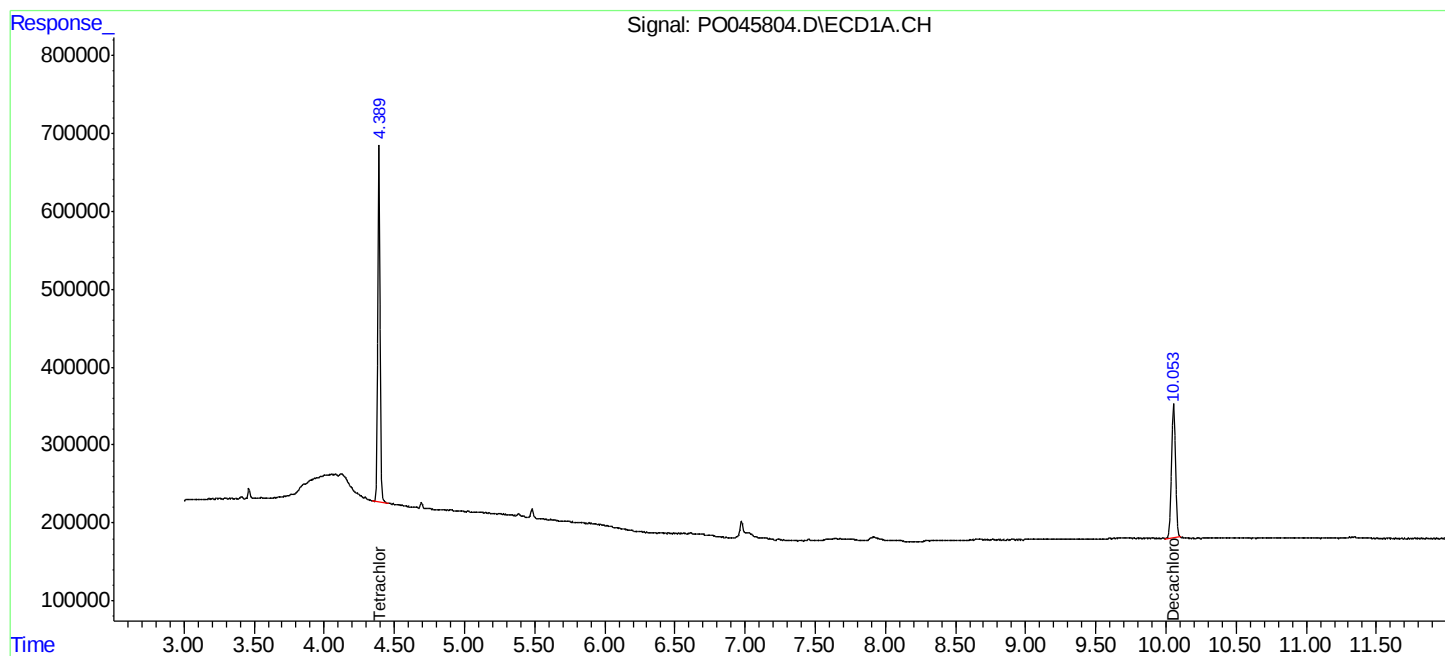

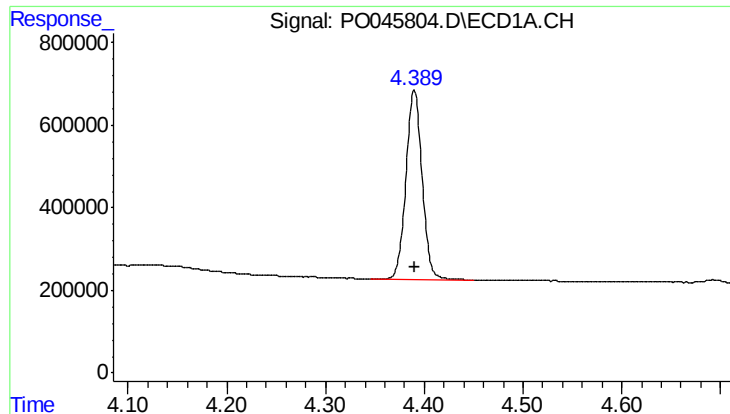


#1 Tetrachloro-m-xylene

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 5215699
Conc: 26.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB110231BL


Manual Integrations
APPROVED

ugo
6/15/2018 6:55:54 PM

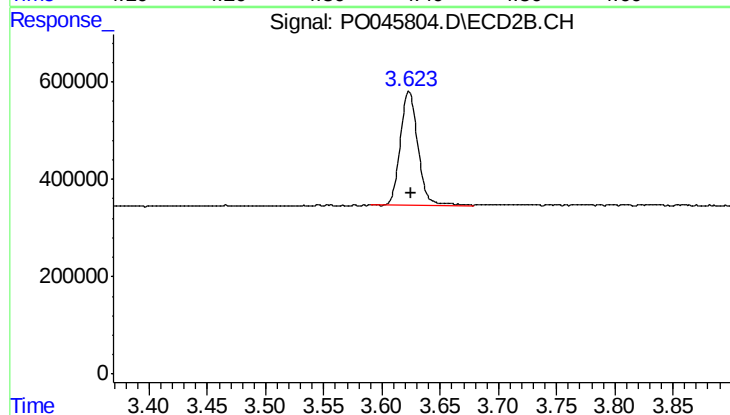


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.001 min
Response: 2472032
Conc: 26.38 ng/ml

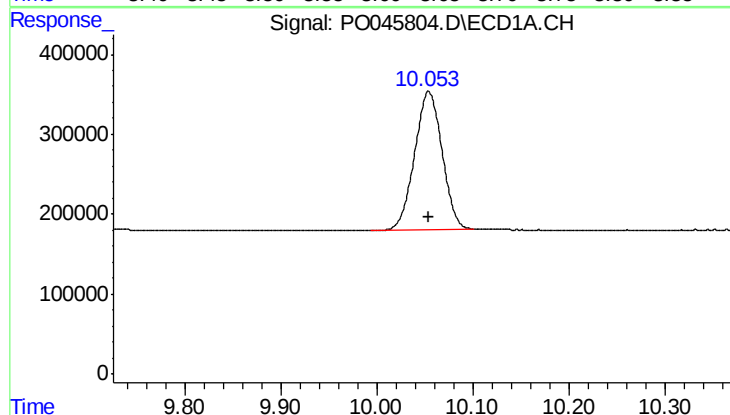

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: -0.001 min
Response: 3432872
Conc: 17.03 ng/ml

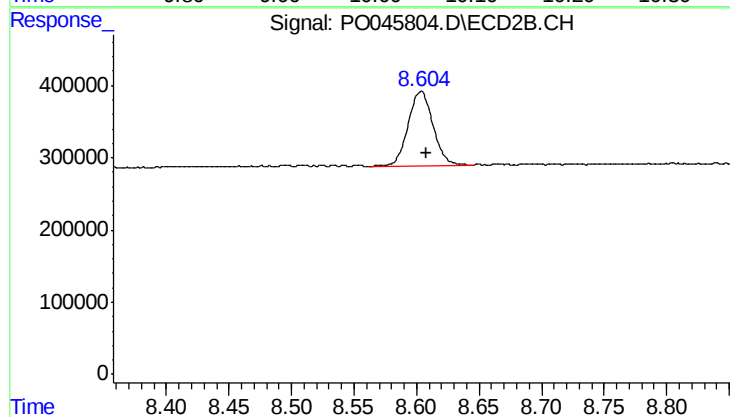

#2 Decachlorobiphenyl

R.T.: 8.604 min
Delta R.T.: -0.005 min
Response: 1439030
Conc: 18.22 ng/ml