

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
 Data File : P0045809.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jun 2018 2:35
 Operator : SM/UA
 Sample : J3502-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20180367-SITE-WATER

Manual Integrations
 APPROVED

ugo
 6/15/2018 6:55:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 08:59:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 15 08:20:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.390	3.625	5007796	2609583	25.524	27.845
2) SA Decachlor...	10.053	8.603	2911316	1291800	14.444	16.354
Target Compounds						
3) L1 AR-1016-1	0.000	4.494	0	25807	N.D. d	9.615 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045809.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2018 2:35
Operator : SM/UA
Sample : J3502-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20180367-SITE-WATER


Manual Integrations
APPROVED

ugo
6/15/2018 6:55:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 08:59:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

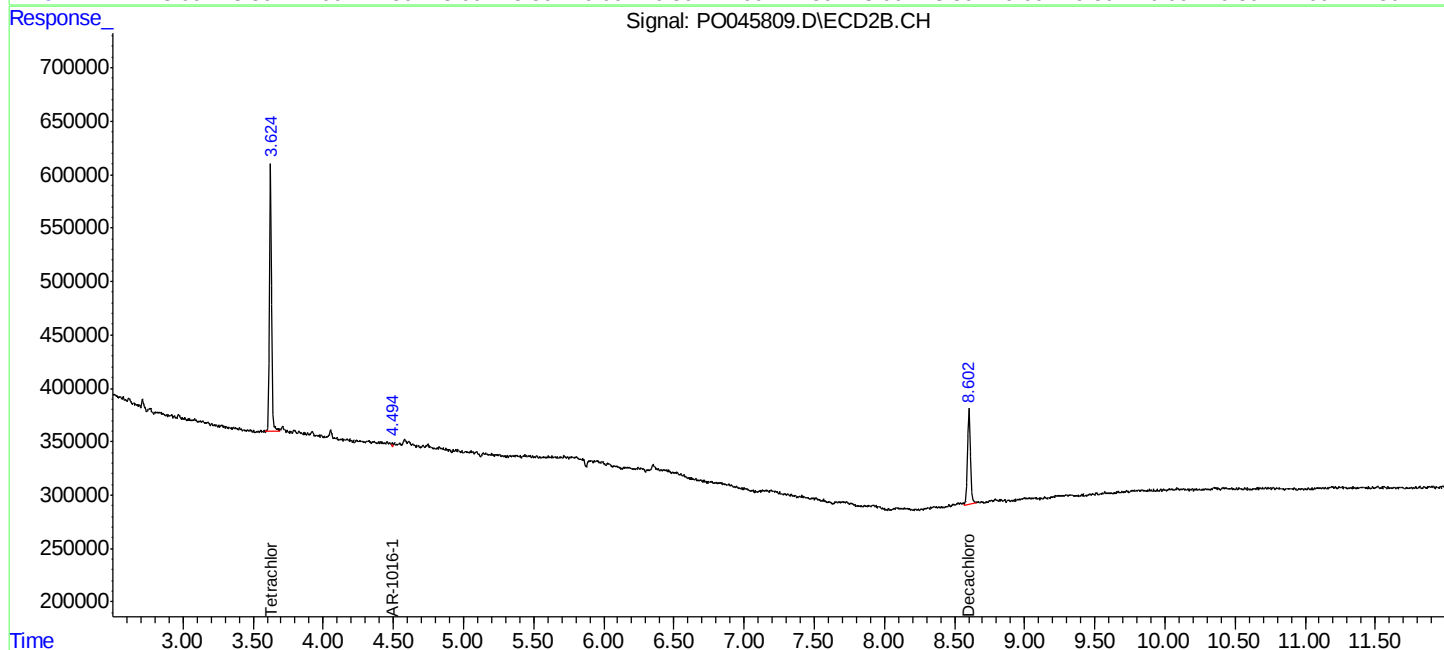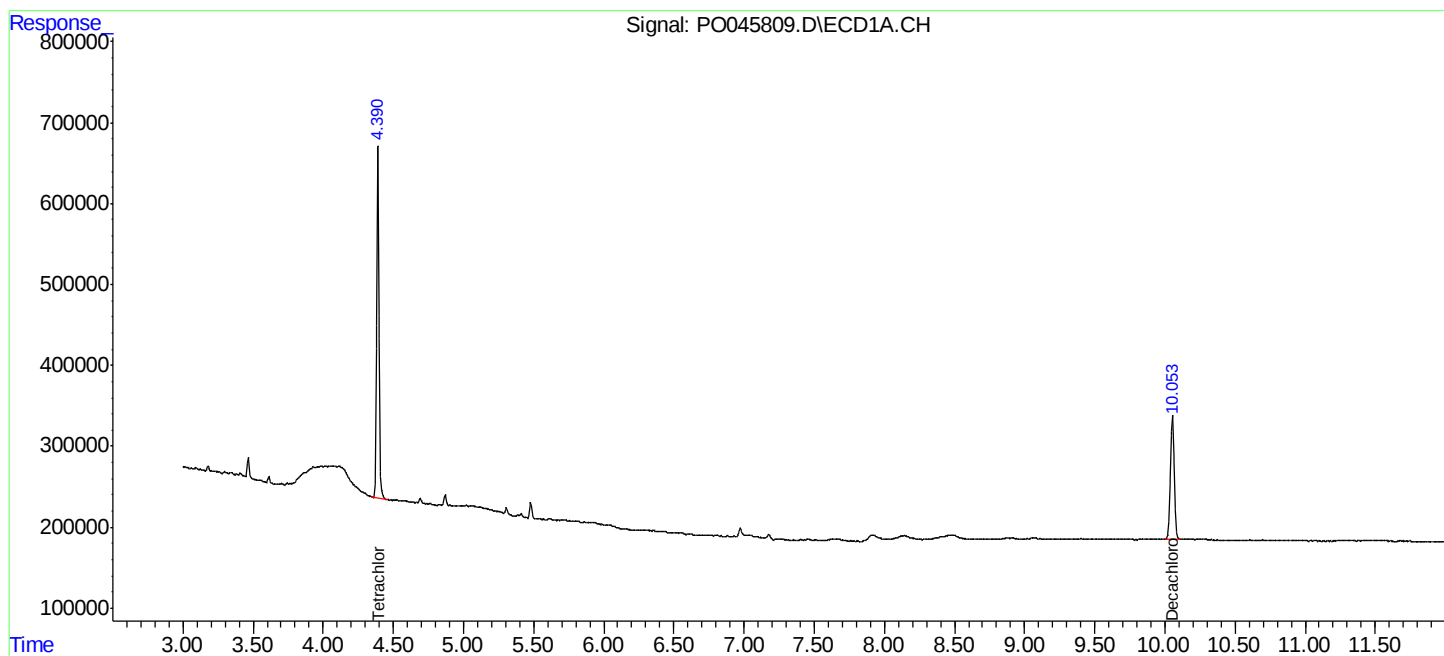

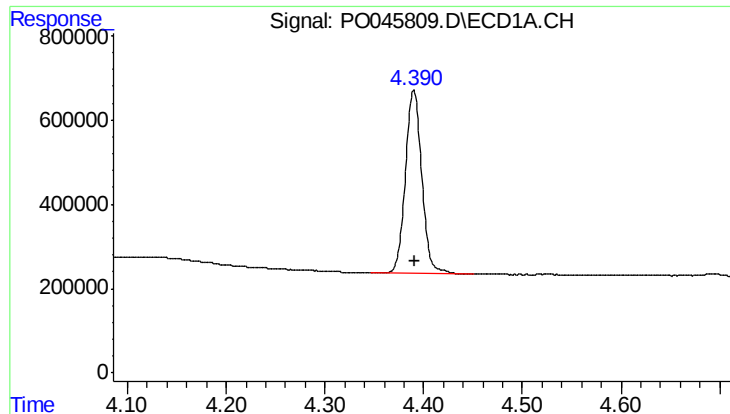


#1 Tetrachloro-m-xylene

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 5007796
Conc: 25.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
20180367-SITE-WATER


Manual Integrations
APPROVED

ugo
6/15/2018 6:55:44 PM

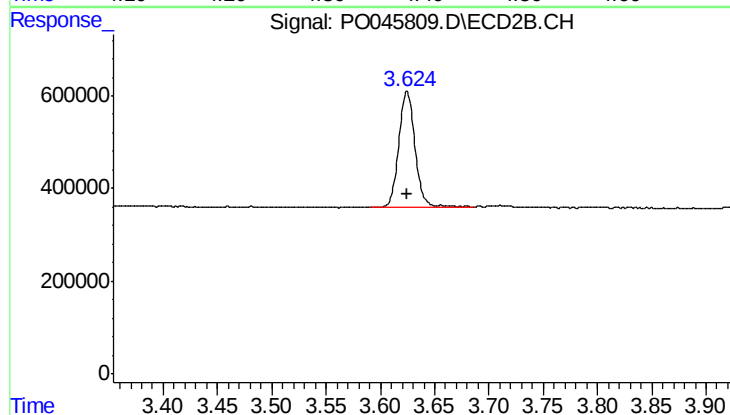


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: 0.000 min
Response: 2609583
Conc: 27.84 ng/ml

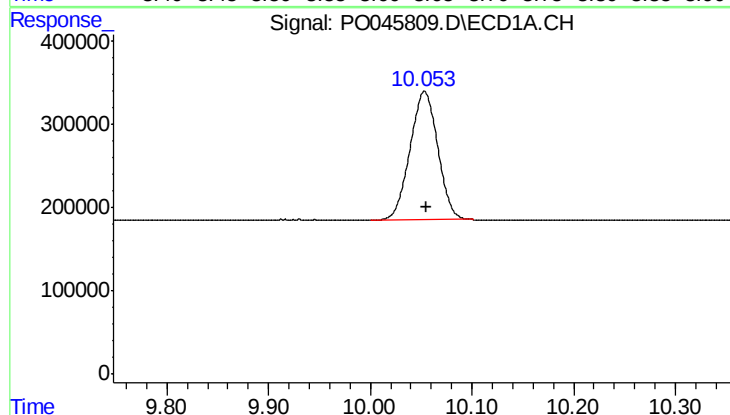


#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: -0.001 min
Response: 2911316
Conc: 14.44 ng/ml

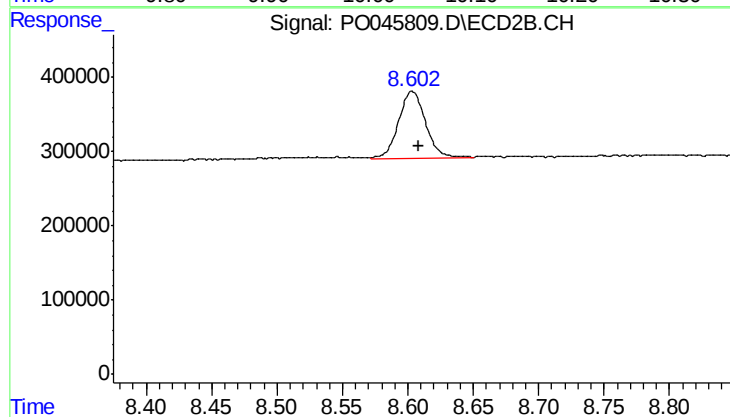

#2 Decachlorobiphenyl

R.T.: 8.603 min
Delta R.T.: -0.005 min
Response: 1291800
Conc: 16.35 ng/ml

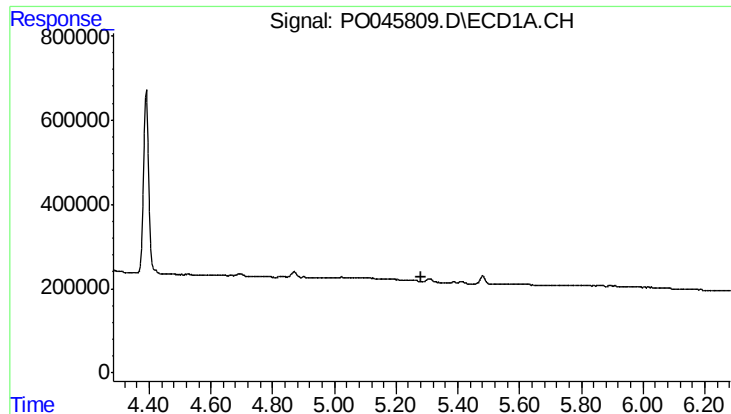


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20180367-SITE-WATER

Manual Integrations
APPROVED

ugo
6/15/2018 6:55:44 PM

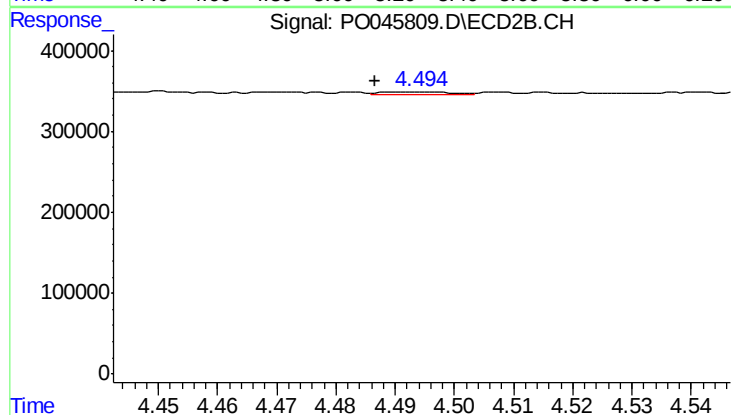

#3 AR-1016-1

R.T.: 4.494 min
Delta R.T.: 0.007 min
Response: 25807
Conc: 9.62 ng/ml