

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2018 4:59
Operator : SM/UA
Sample : J3415-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-37COMP

Manual Integrations
APPROVED

ugo
6/15/2018 6:55:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 09:05:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.389	3.622	4918992	2289473	25.072	24.429
2)	SA Decachlor...	10.053	8.602	2500040	986184	12.404	12.485m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061418\
Data File : P0045818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2018 4:59
Operator : SM/UA
Sample : J3415-06
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-37COMP


Manual Integrations
APPROVED

ugo
6/15/2018 6:55:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 09:05:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

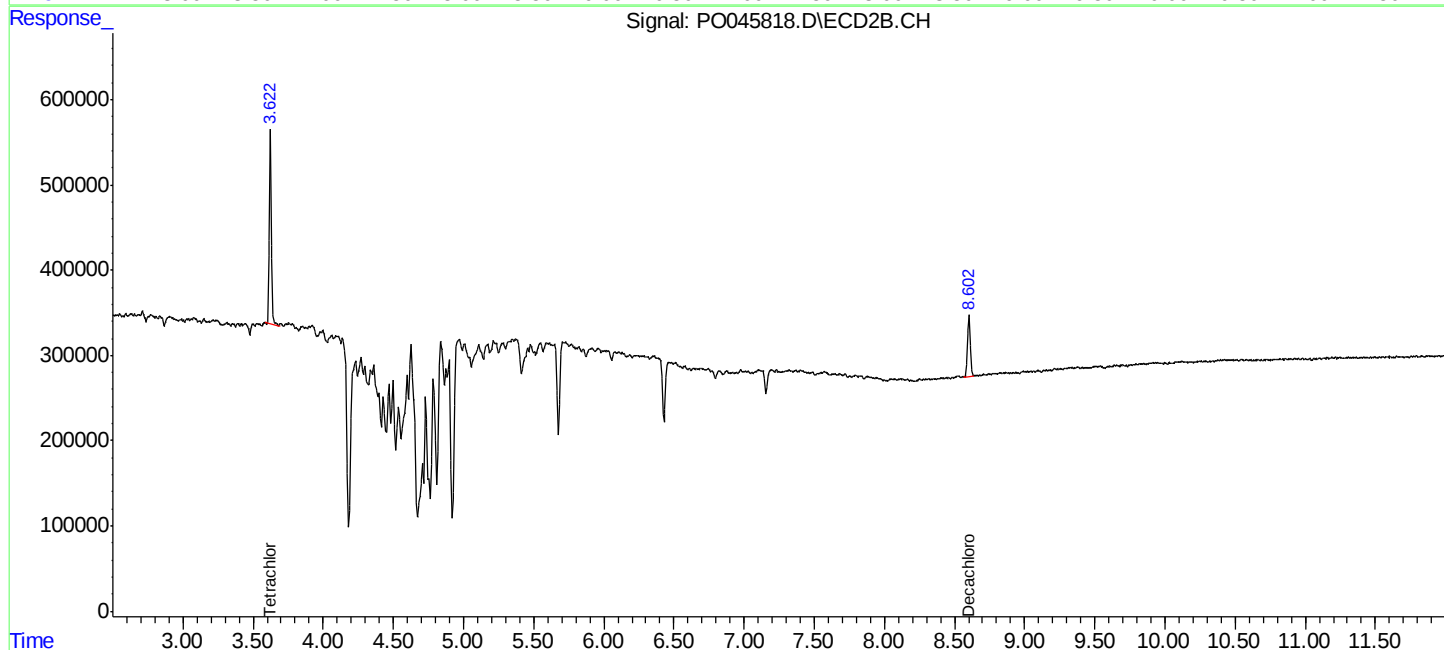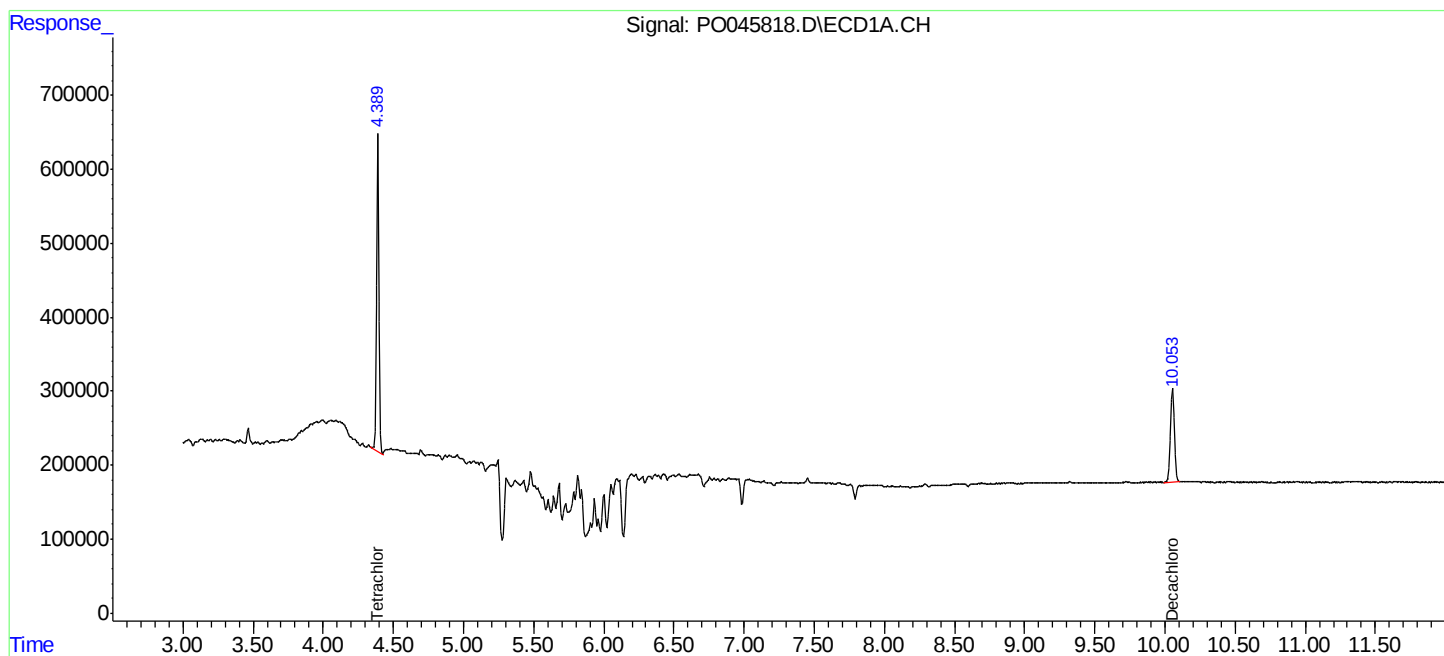

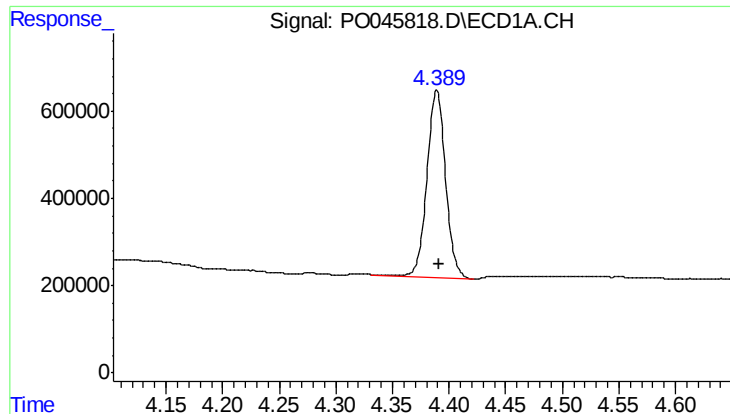


#1 Tetrachloro-m-xylene

R.T.: 4.389 min
Delta R.T.: -0.002 min
Response: 4918992
Conc: 25.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-37COMP


Manual Integrations
APPROVED

ugo
6/15/2018 6:55:37 PM

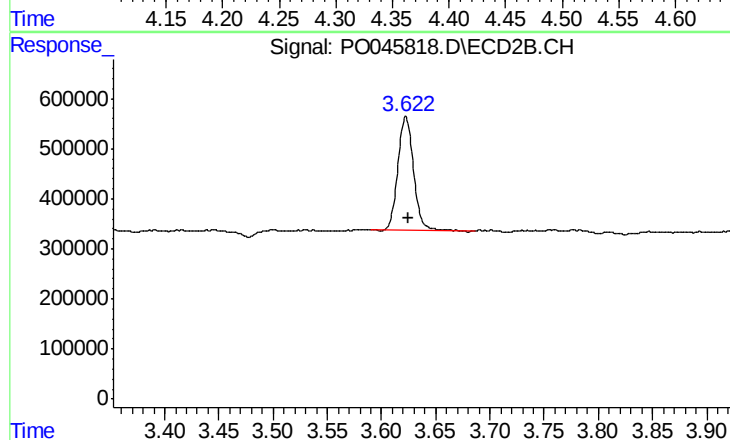


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.002 min
Response: 2289473
Conc: 24.43 ng/ml

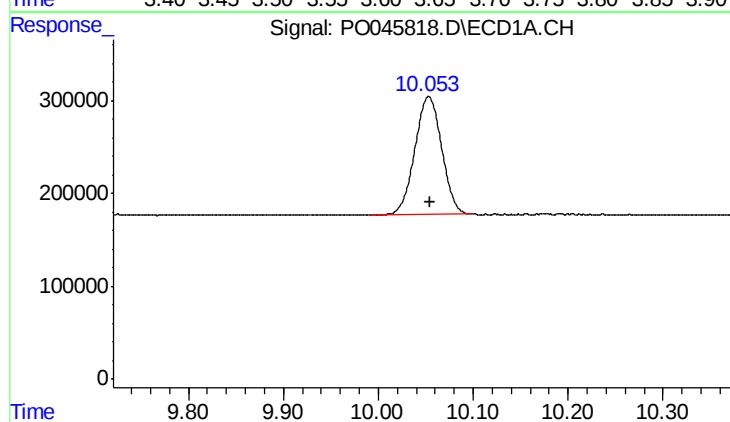

#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: -0.002 min
Response: 2500040
Conc: 12.40 ng/ml

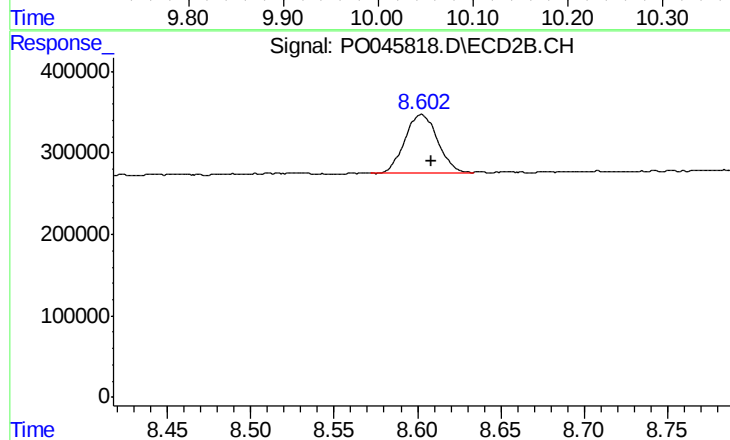

#2 Decachlorobiphenyl

R.T.: 8.602 min
Delta R.T.: -0.006 min
Response: 986184
Conc: 12.48 ng/ml m