

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061421\
 Data File : P0078780.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 19:36
 Operator : DD\AJ
 Sample : PB137008BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 01:45:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.330	3.606	1782283	730118	21.051	21.091
2)	SA Decachlor...	9.938	8.789	1363334	727032	23.232	23.383
Target Compounds							
8)	L2 AR-1221-1	4.576	0.000	30871	0	34.306	N.D. #
9)	L2 AR-1221-2	4.671	0.000	18867	0	28.436	N.D. #
24)	L5 AR-1248-4	6.535f	0.000	973	0	0.371	N.D. #
26)	L6 AR-1254-1	6.527	0.000	5439	0	1.984	N.D. #
28)	L6 AR-1254-3	7.141f	0.000	68989	0	15.846	N.D. #
32)	L7 AR-1260-2	7.543	0.000	29923	0	8.094	N.D. #
45)	L9 AR-1268-5	9.678	0.000	8553	0	0.434	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061421\
Data File : P0078780.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 19:36
Operator : DD\AJ
Sample : PB137008BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 01:45:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

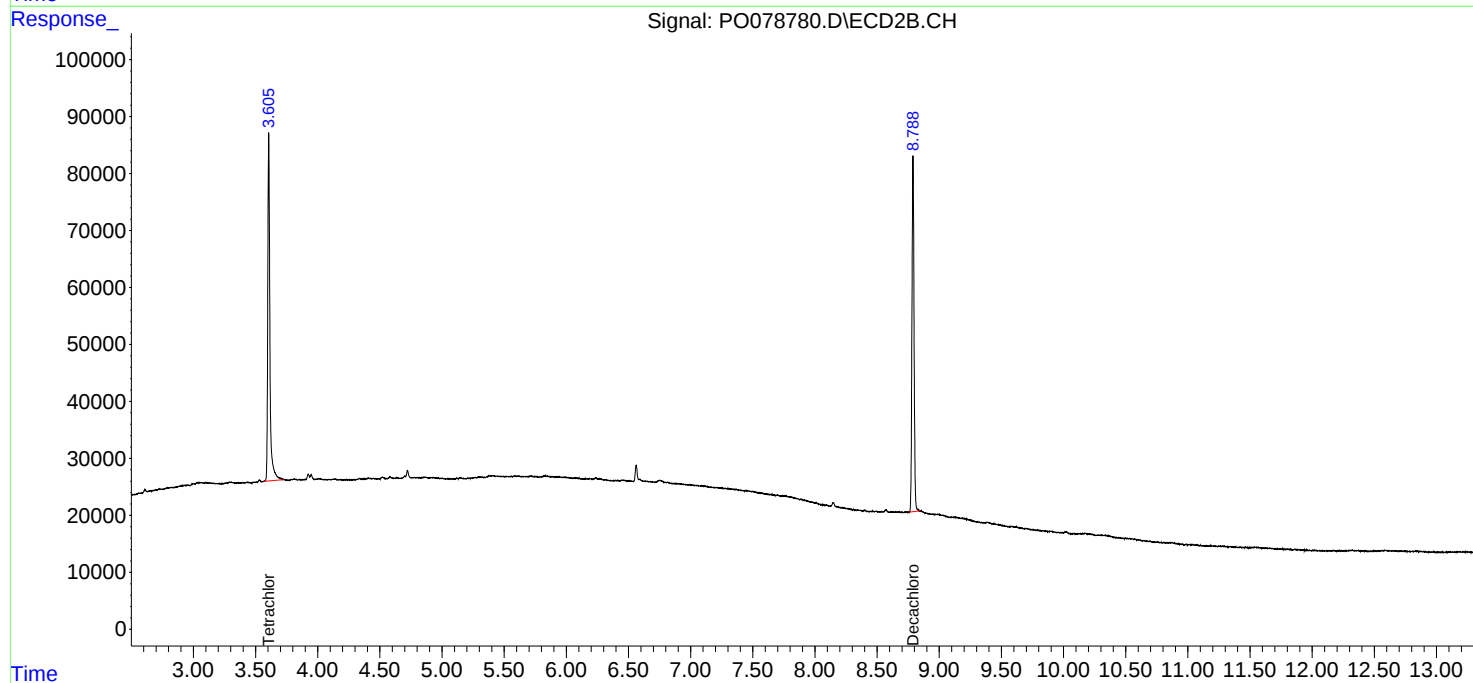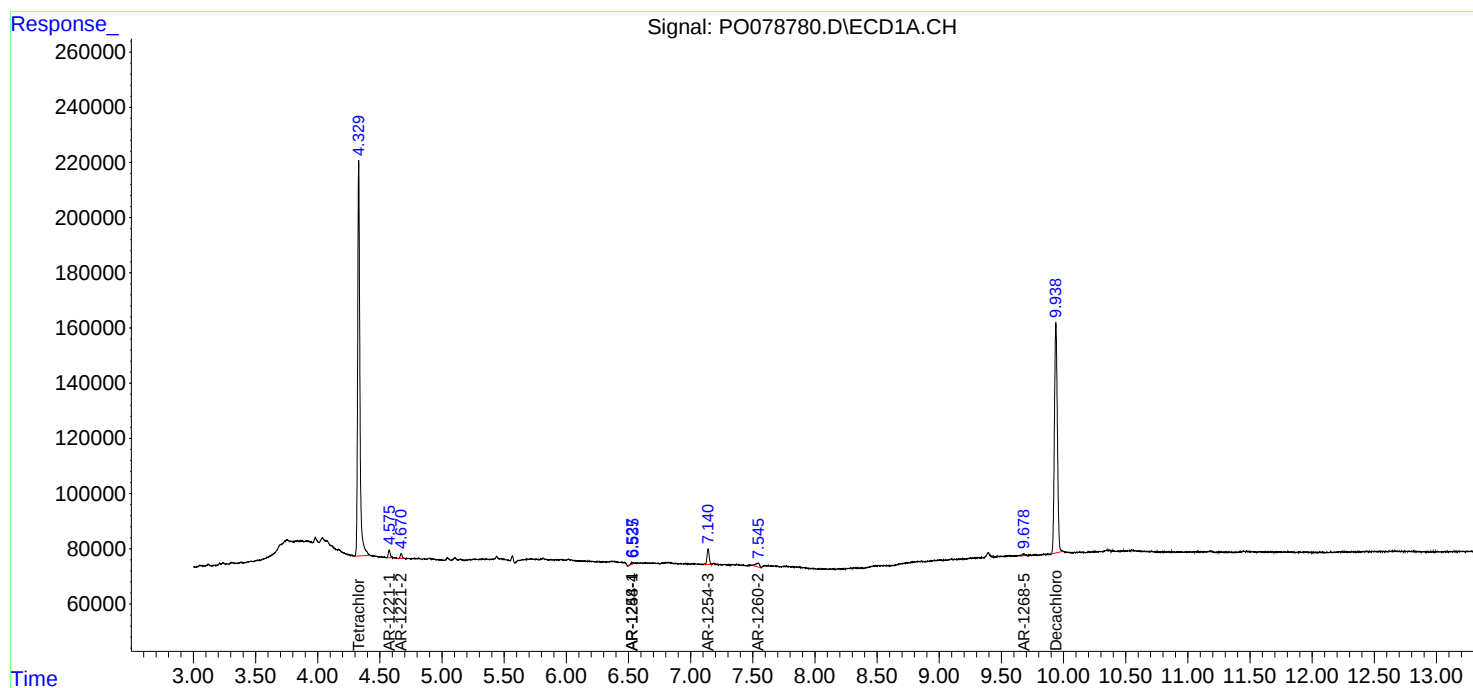


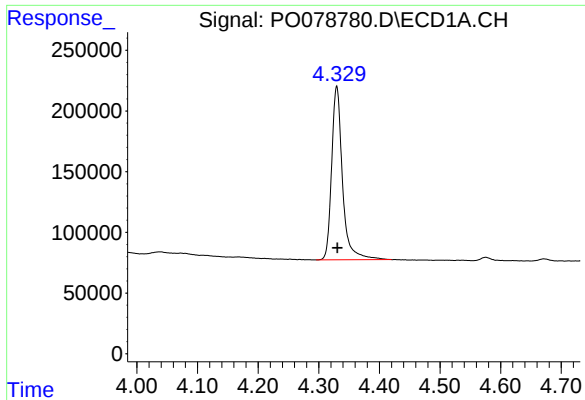

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: -0.001 min
Response: 1782283
Conc: 21.05 ng/ml

Instrument :
ECD_O
ClientSampleId :

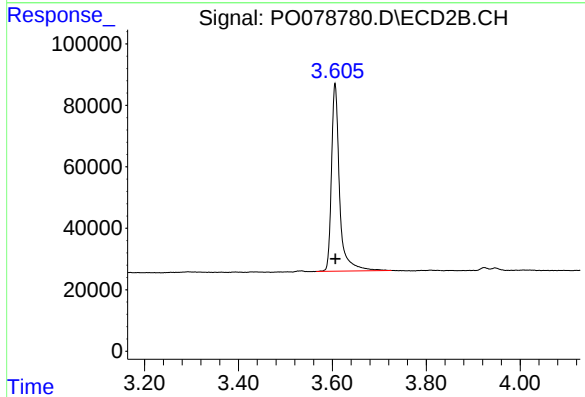


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 730118
Conc: 21.09 ng/ml

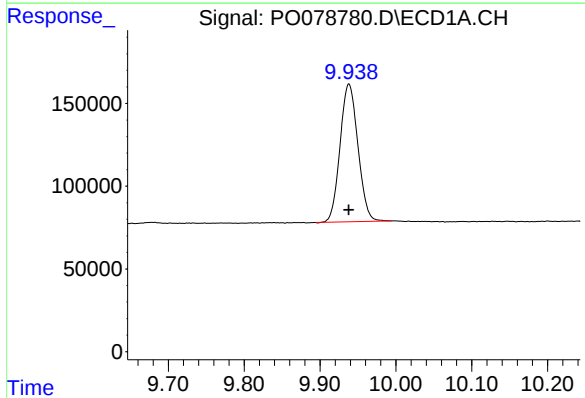


#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.000 min
Response: 1363334
Conc: 23.23 ng/ml

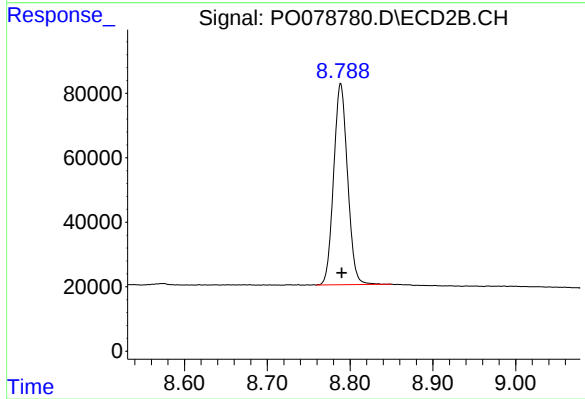

#2 Decachlorobiphenyl


R.T.: 8.789 min
Delta R.T.: -0.001 min
Response: 727032
Conc: 23.38 ng/ml

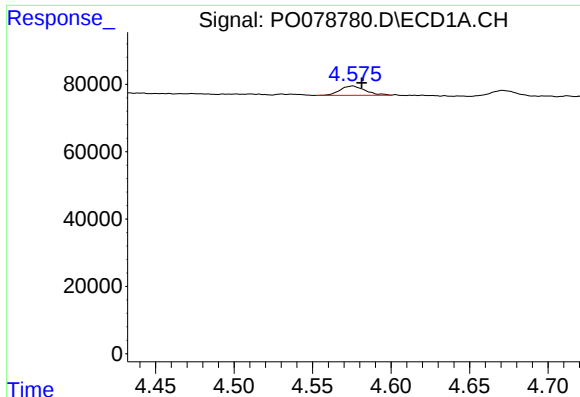

#8 AR-1221-1


R.T.: 4.576 min
Delta R.T.: -0.006 min
Response: 30871
Conc: 34.31 ng/ml

Instrument :
ECD_O
ClientSampleId :

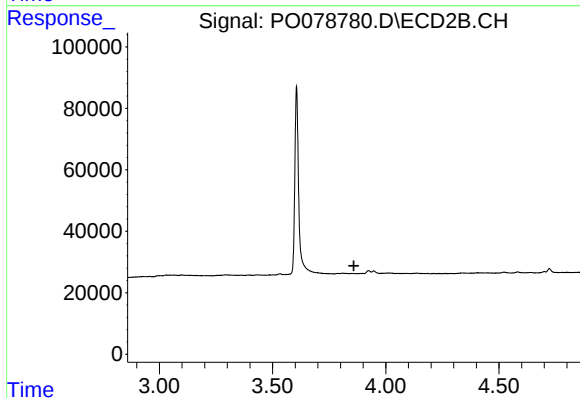


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.859 min
Response: 0
Conc: N.D.

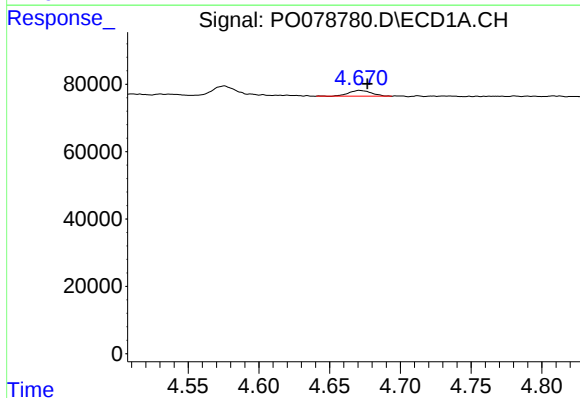


#9 AR-1221-2

R.T.: 4.671 min
Delta R.T.: -0.006 min
Response: 18867
Conc: 28.44 ng/ml

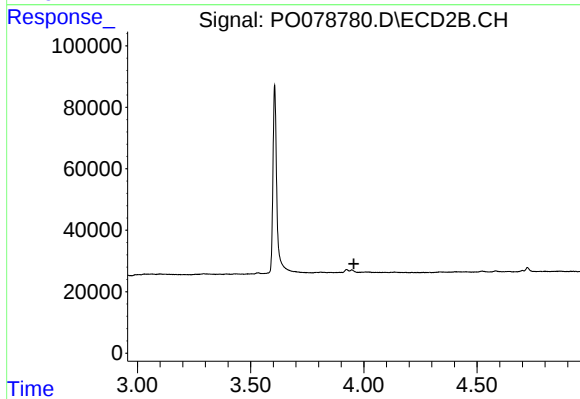

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.956 min
Response: 0
Conc: N.D.

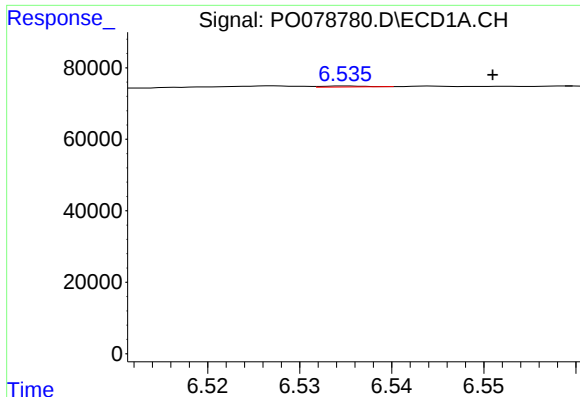

#24 AR-1248-4


R.T.: 6.535 min
Delta R.T.: -0.016 min
Response: 973
Conc: 0.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

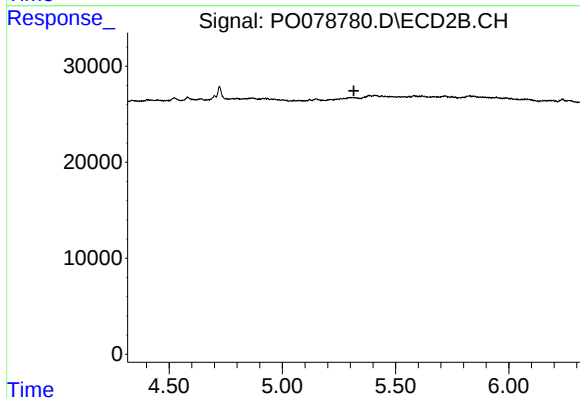


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.316 min
Response: 0
Conc: N.D.

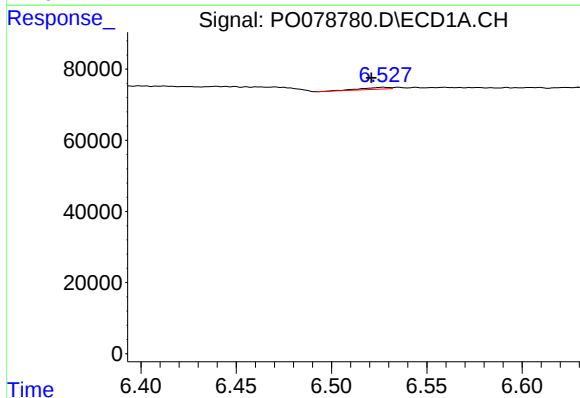


#26 AR-1254-1

R.T.: 6.527 min
Delta R.T.: 0.006 min
Response: 5439
Conc: 1.98 ng/ml

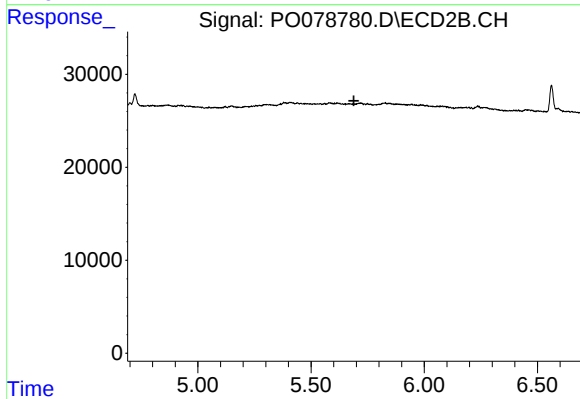

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.689 min
Response: 0
Conc: N.D.

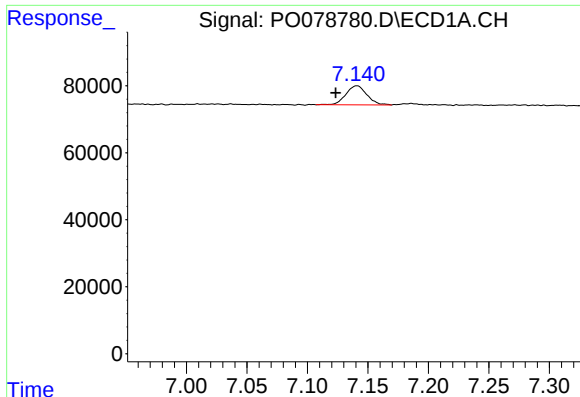

#28 AR-1254-3


R.T.: 7.141 min
Delta R.T.: 0.017 min
Response: 68989
Conc: 15.85 ng/ml

Instrument :
ECD_O
ClientSampleId :

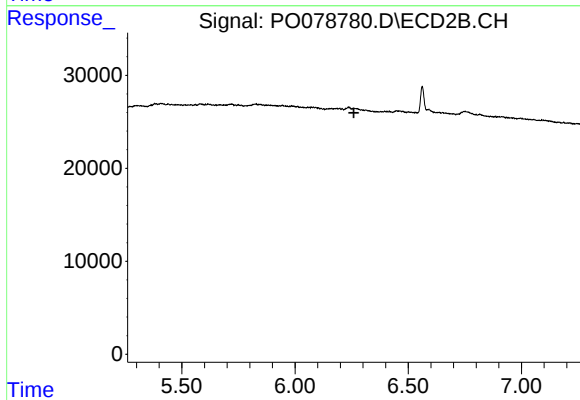


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.260 min
Response: 0
Conc: N.D.

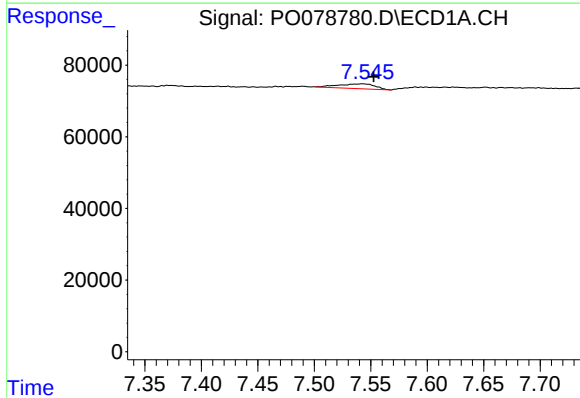


#32 AR-1260-2

R.T.: 7.543 min
Delta R.T.: -0.010 min
Response: 29923
Conc: 8.09 ng/ml

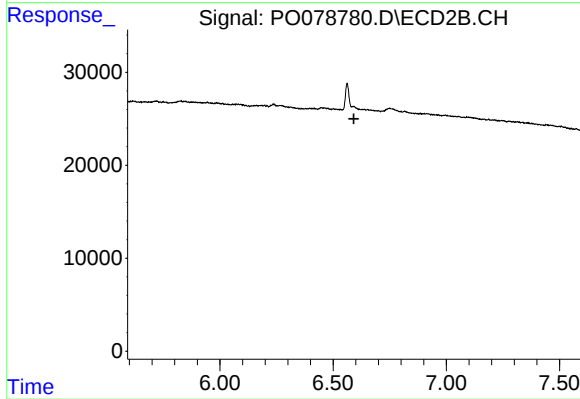

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.592 min
Response: 0
Conc: N.D.

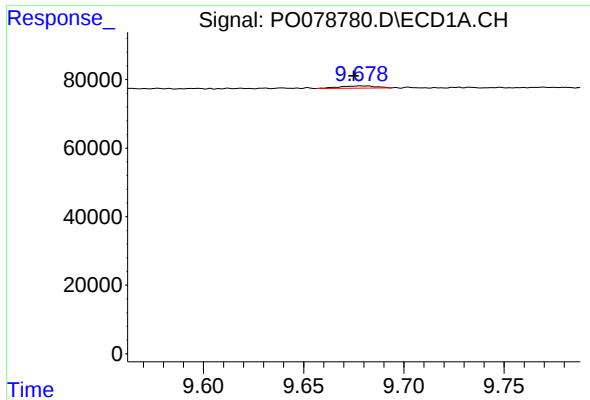

#45 AR-1268-5

R.T.: 9.678 min
Delta R.T.: 0.003 min
Response: 8553
Conc: 0.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

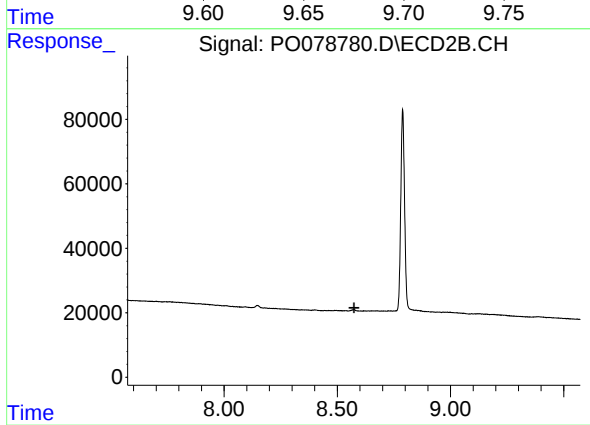

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.574 min
Response: 0
Conc: N.D.