

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0061421\
 Data File : P0078748.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 10:24
 Operator : DD\AJ
 Sample : M2678-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 0205-COMP-F(DISCRETE-CL-05)

Manual Integrations
 APPROVED

Ankita
 6/15/2021 2:38:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 01:28:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.332	3.608	1626943	662717	19.216	19.144
2) SA Decachlor...	9.940	8.791	983114	519975	16.753	16.724
Target Compounds						
26) L6 AR-1254-1	6.522	5.690	96999	24624	35.386	13.937 #
27) L6 AR-1254-2	6.749	5.848	96131	22872	22.728m	14.117 #
28) L6 AR-1254-3	7.125	6.261	62528	25834	14.362m	10.627 #
29) L6 AR-1254-4	7.416	6.499	39683	23285	12.891	15.551
30) L6 AR-1254-5	7.840	6.921	45697	27483	13.257	11.972

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061421\
Data File : PO078748.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 10:24
Operator : DD\AJ
Sample : M2678-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 2:38:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 01:28:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

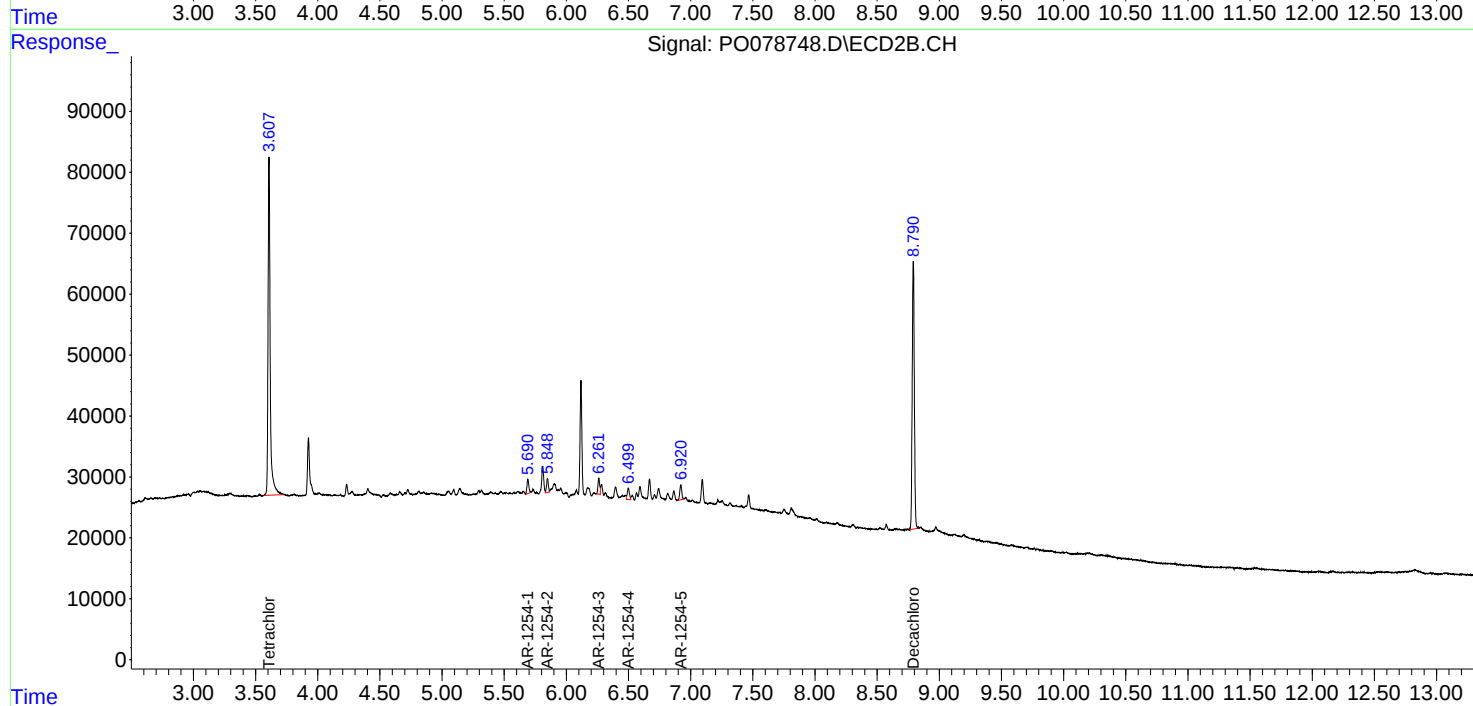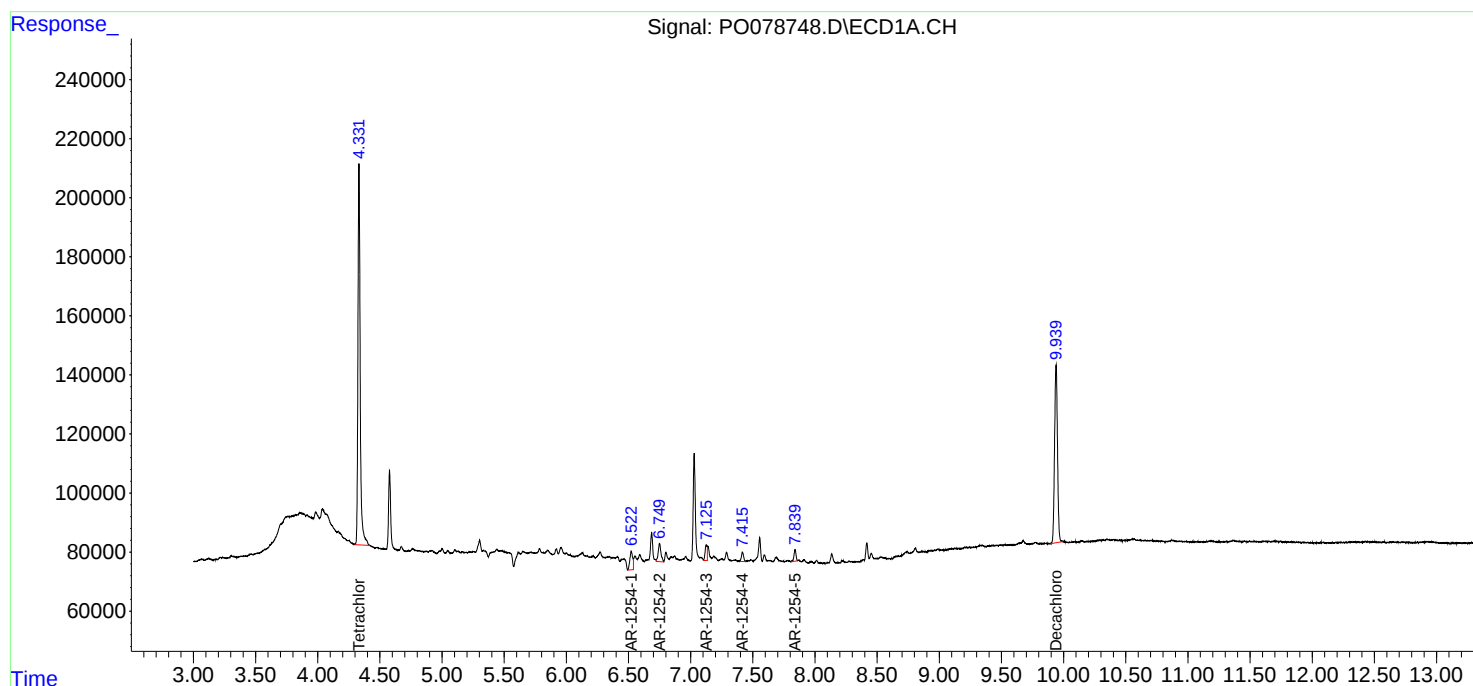

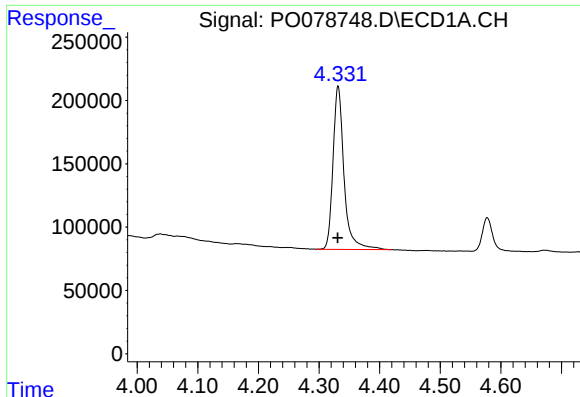


#1 Tetrachloro-m-xylene

R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 1626943
Conc: 19.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 2:38:29 PM

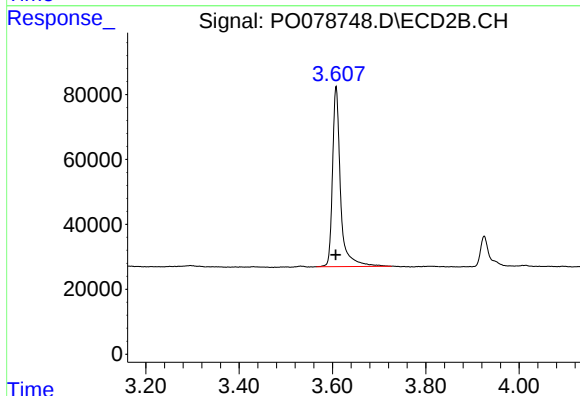


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: 0.000 min
Response: 662717
Conc: 19.14 ng/ml

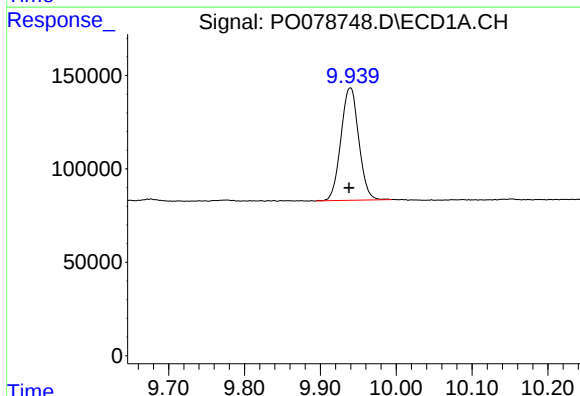


#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.002 min
Response: 983114
Conc: 16.75 ng/ml

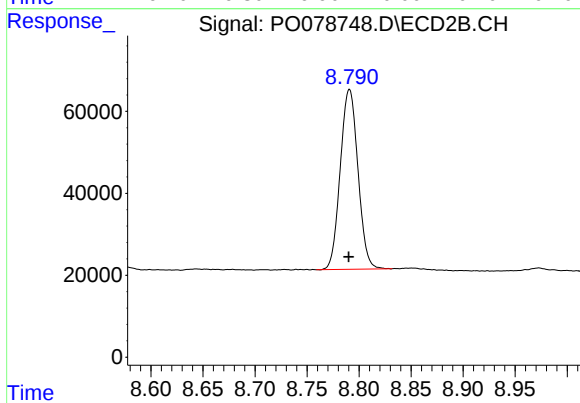

#2 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 519975
Conc: 16.72 ng/ml

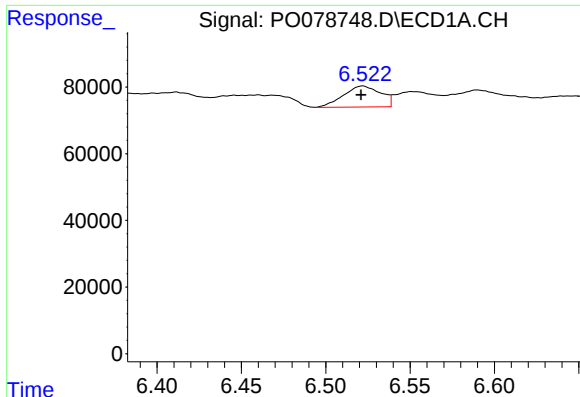


#26 AR-1254-1

R.T.: 6.522 min
Delta R.T.: 0.001 min
Response: 96999
Conc: 35.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 2:38:29 PM

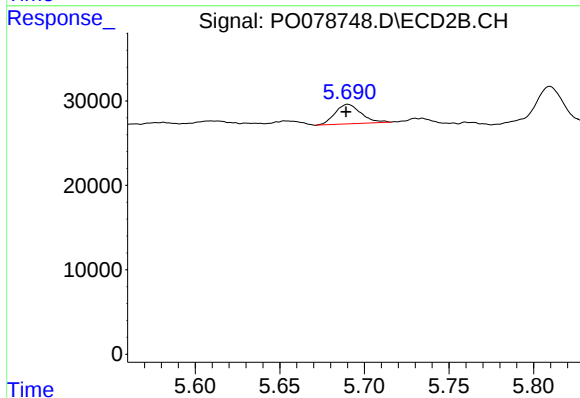


#26 AR-1254-1

R.T.: 5.690 min
Delta R.T.: 0.001 min
Response: 24624
Conc: 13.94 ng/ml

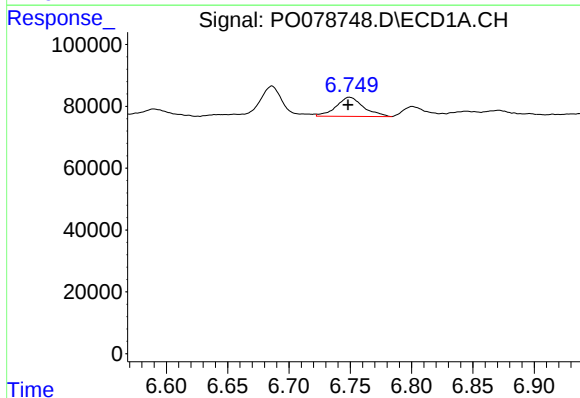


#27 AR-1254-2

R.T.: 6.749 min
Delta R.T.: 0.000 min
Response: 96131
Conc: 22.73 ng/ml m

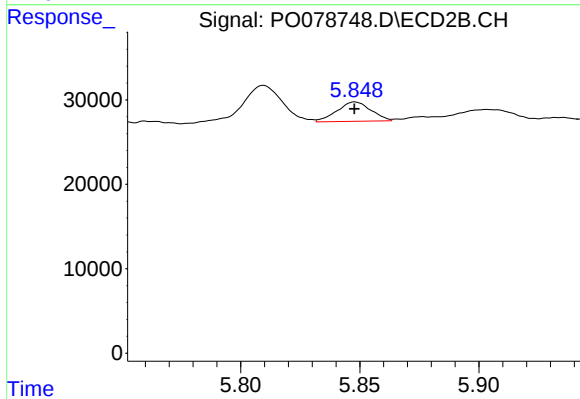

#27 AR-1254-2

R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 22872
Conc: 14.12 ng/ml

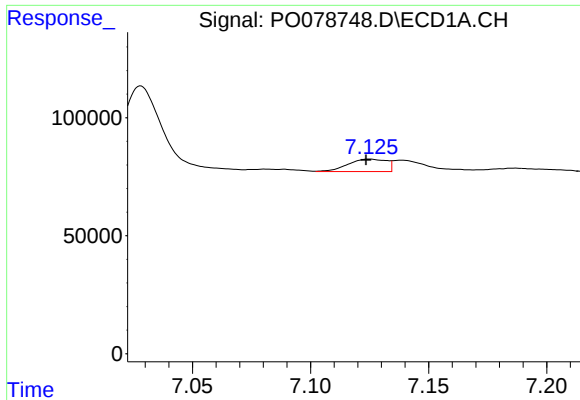


#28 AR-1254-3

R.T.: 7.125 min
Delta R.T.: 0.001 min
Response: 62528
Conc: 14.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 2:38:29 PM

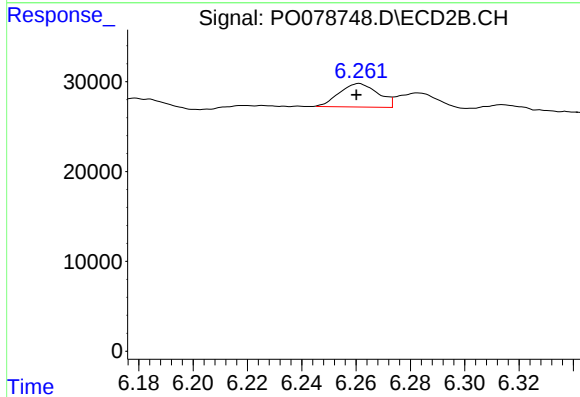


#28 AR-1254-3

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 25834
Conc: 10.63 ng/ml

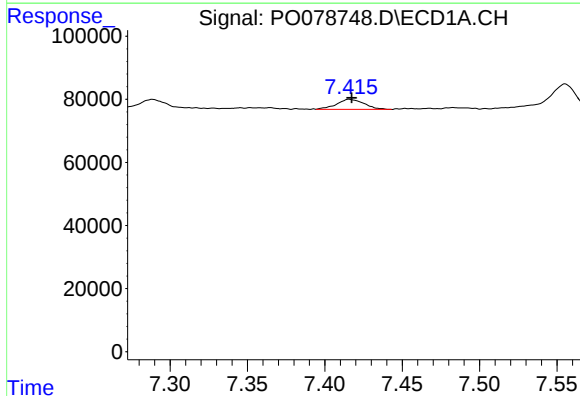


#29 AR-1254-4

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 39683
Conc: 12.89 ng/ml

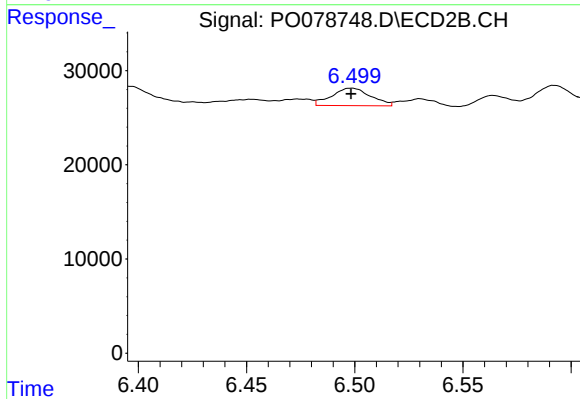

#29 AR-1254-4

R.T.: 6.499 min
Delta R.T.: 0.000 min
Response: 23285
Conc: 15.55 ng/ml

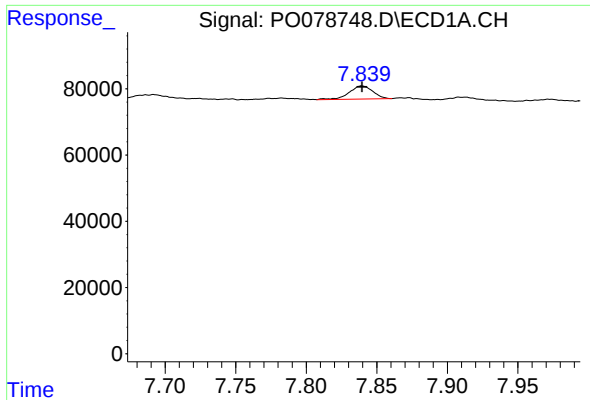


#30 AR-1254-5

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 45697
Conc: 13.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)

Manual Integrations
APPROVED

Ankita
6/15/2021 2:38:29 PM

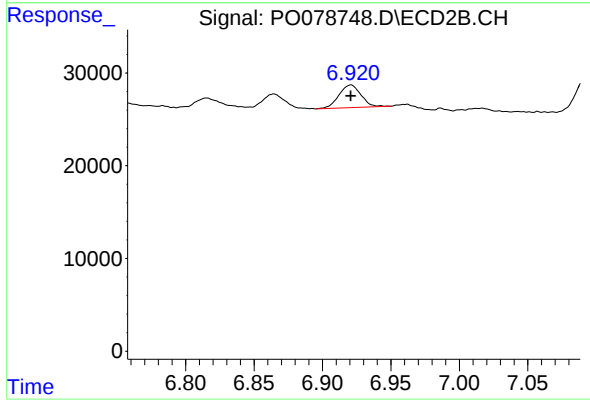

#30 AR-1254-5

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 27483
Conc: 11.97 ng/ml