

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061421\
 Data File : P0078751.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 11:16
 Operator : DD\AJ
 Sample : M2678-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0231-COMPOSITE-H

Manual Integrations
 APPROVED

Ankita
 6/15/2021 2:38:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 01:29:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.331	3.607	1538239	650210	18.168	18.782
2) SA Decachlor...	9.943	8.791	1084098	578649	18.473	18.611m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061421\
Data File : P0078751.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 11:16
Operator : DD\AJ
Sample : M2678-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
0231-COMPOSITE-H


Manual Integrations
APPROVED

Ankita
6/15/2021 2:38:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 01:29:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

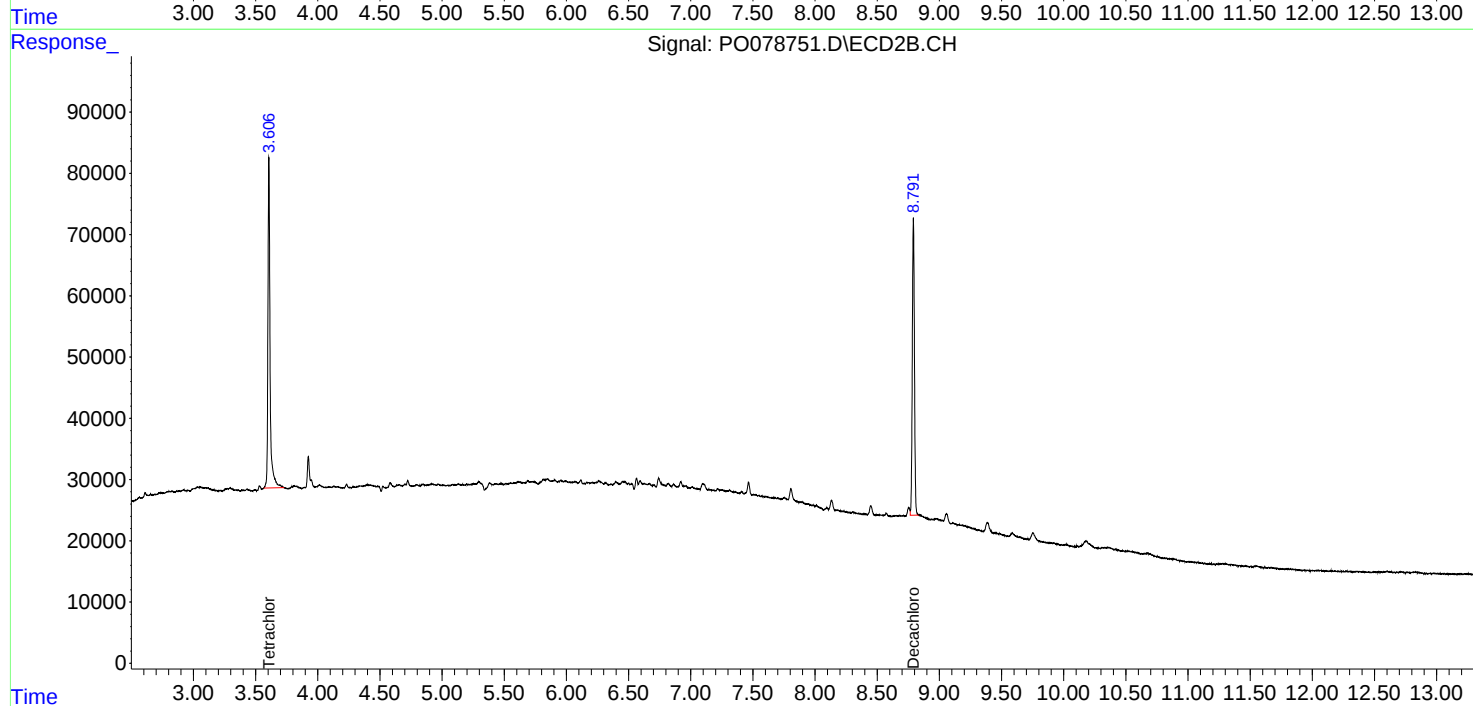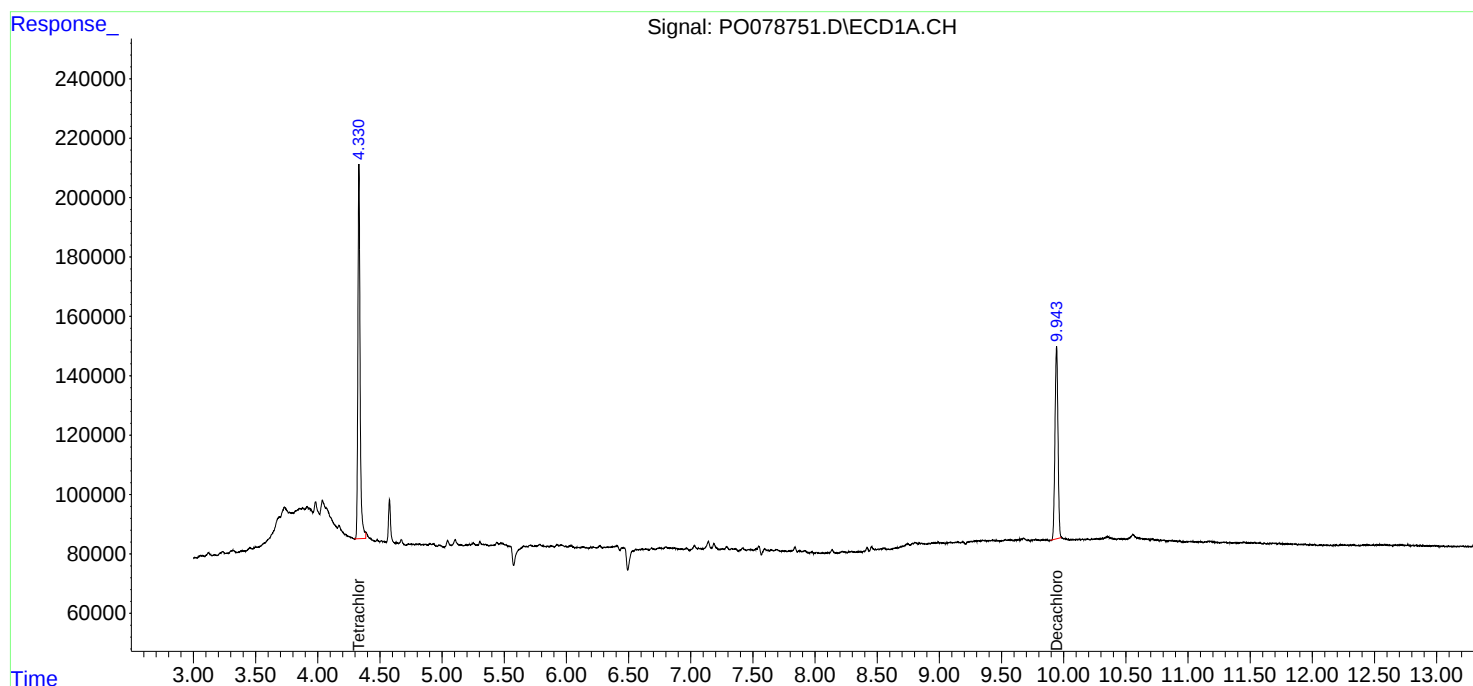

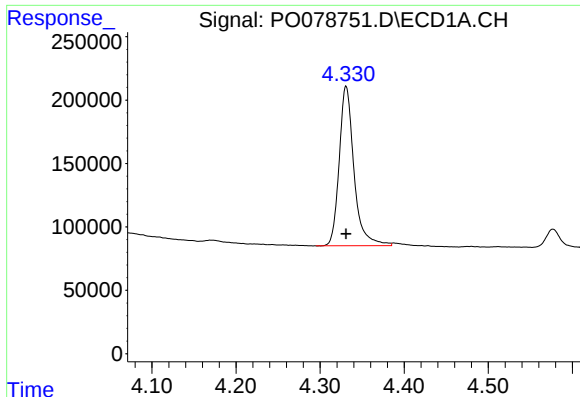


#1 Tetrachloro-m-xylene

R.T.: 4.331 min
Delta R.T.: 0.000 min
Response: 1538239
Conc: 18.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
0231-COMPOSITE-H


Manual Integrations
APPROVED

Ankita
6/15/2021 2:38:30 PM

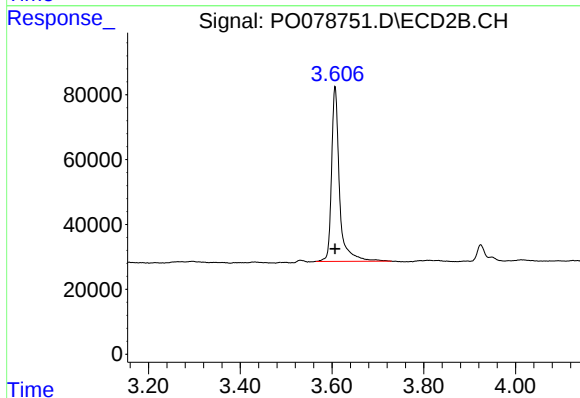


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 650210
Conc: 18.78 ng/ml

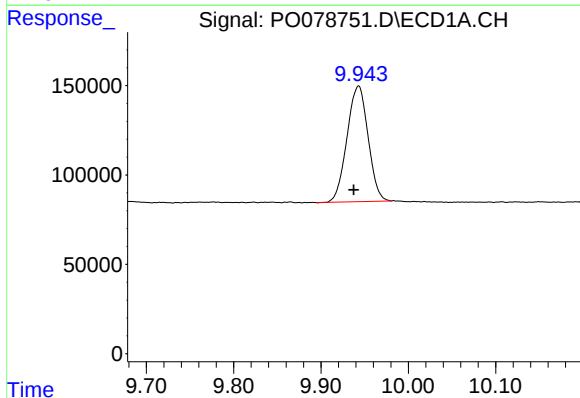

#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: 0.006 min
Response: 1084098
Conc: 18.47 ng/ml

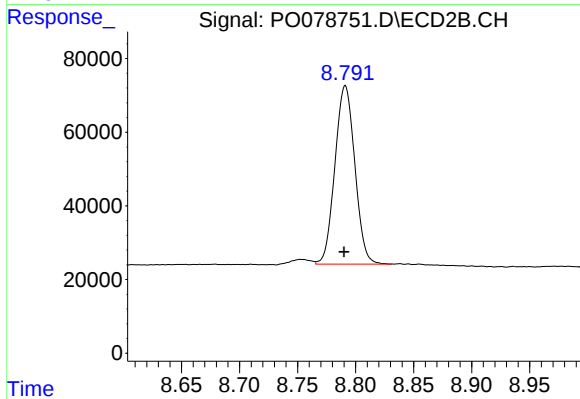

#2 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 578649
Conc: 18.61 ng/ml m