

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061421\
 Data File : P0078753.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 11:50
 Operator : DD\AJ
 Sample : M2678-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0241-AMND-COMP-F(CL-05)

Manual Integrations
 APPROVED

Ankita
 6/15/2021 4:23:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 01:30:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.331	3.606	1724399	699261	20.367	20.199
2)	SA Decachlor...	9.941	8.791	1185510	603497	20.202	19.410
Target Compounds							
26)	L6 AR-1254-1	6.522	5.689	175479	88293	64.017	49.974m
27)	L6 AR-1254-2	6.749	5.847	435482	90299	102.960	55.733m#
28)	L6 AR-1254-3	7.125	6.259	356958	118303	81.987m	48.662m#
29)	L6 AR-1254-4	7.416	6.498	160278	82115	52.065m	54.841
30)	L6 AR-1254-5	7.839	6.920	321172	166795	93.176m	72.661
31)	L7 AR-1260-1	7.288	6.394	207323	179513	65.947m	106.836 #
32)	L7 AR-1260-2	7.555	6.591	426735	137209	115.428m	68.085 #
33)	L7 AR-1260-3	7.914	6.741	171382	105137	60.429	53.896
34)	L7 AR-1260-4	8.135	7.219	219820	71699	69.588m	44.870 #
35)	L7 AR-1260-5	8.452	7.466	319227	155471	52.309	42.259

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061421\
Data File : PO078753.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 11:50
Operator : DD\AJ
Sample : M2678-07
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
0241-AMND-COMP-F(CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 4:23:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 01:30:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

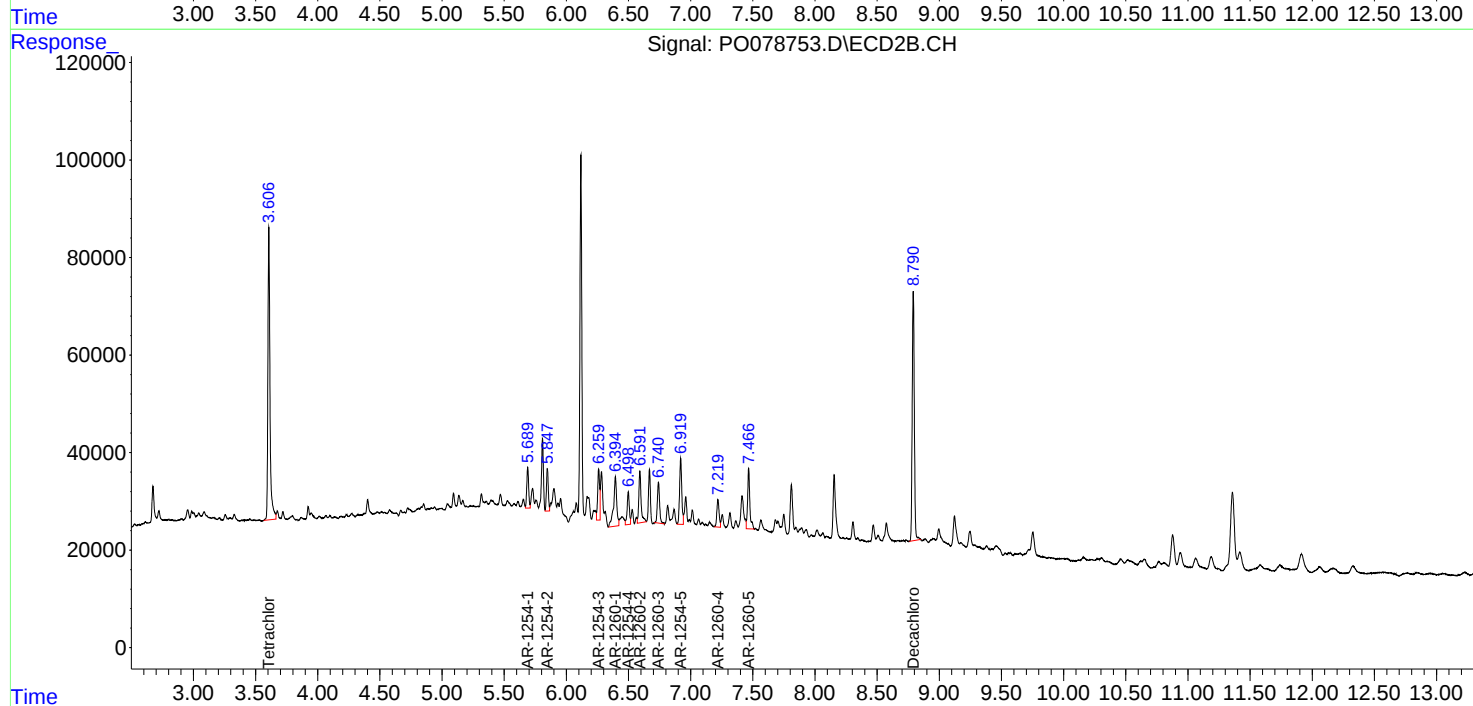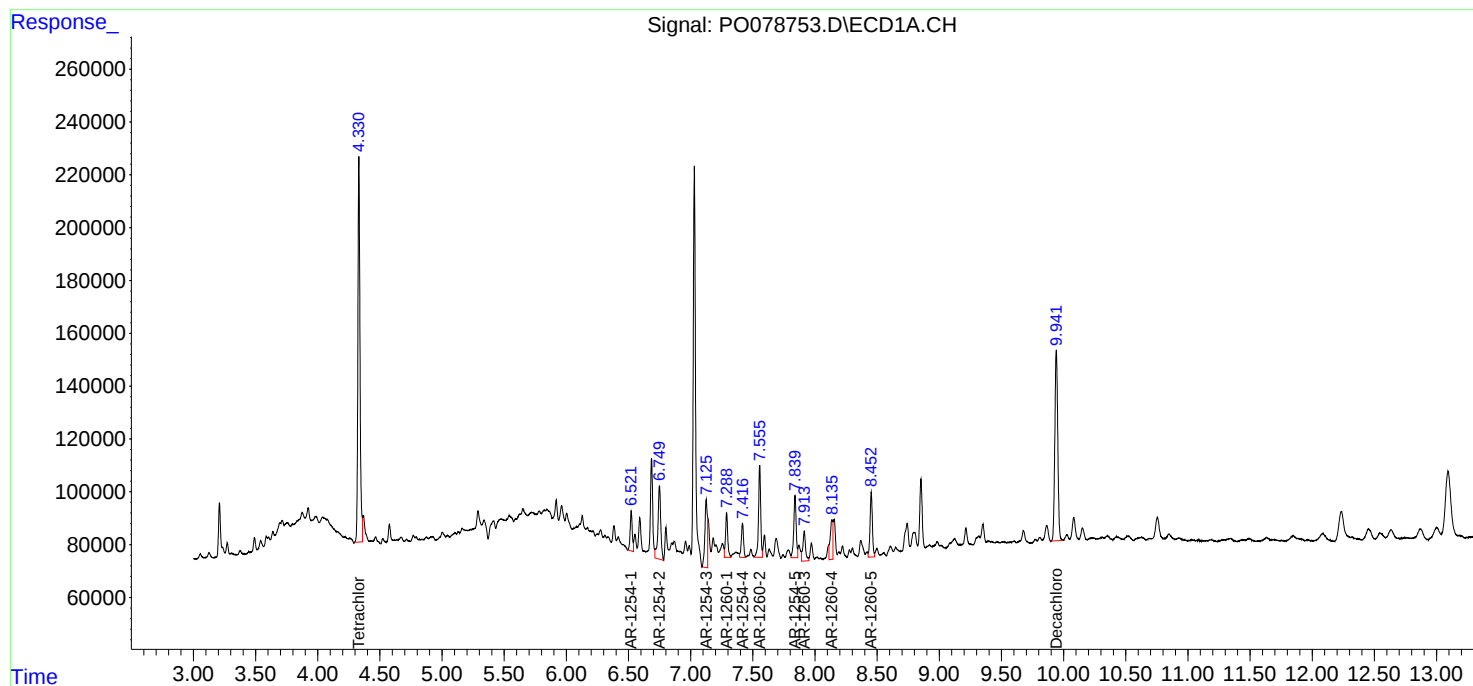

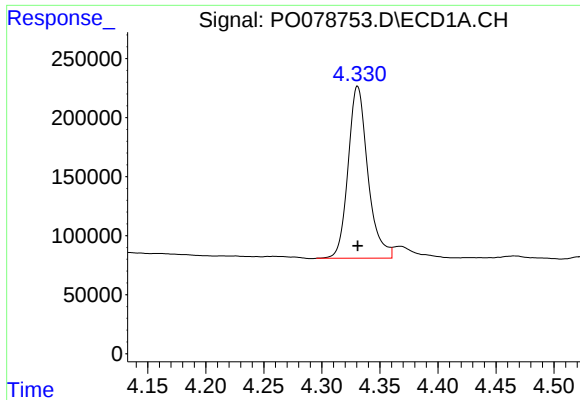


#1 Tetrachloro-m-xylene

R.T.: 4.331 min
Delta R.T.: 0.000 min
Response: 1724399
Conc: 20.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
0241-AMND-COMP-F(CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 4:23:30 PM

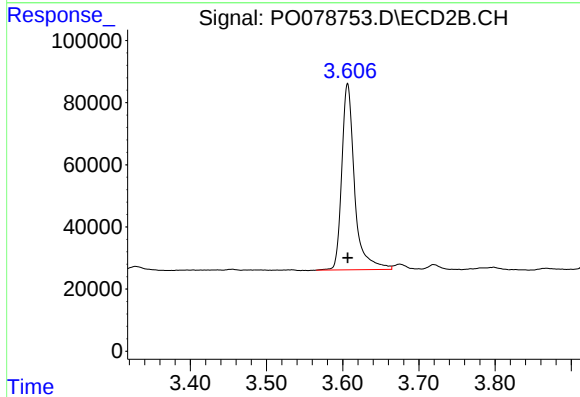


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 699261
Conc: 20.20 ng/ml

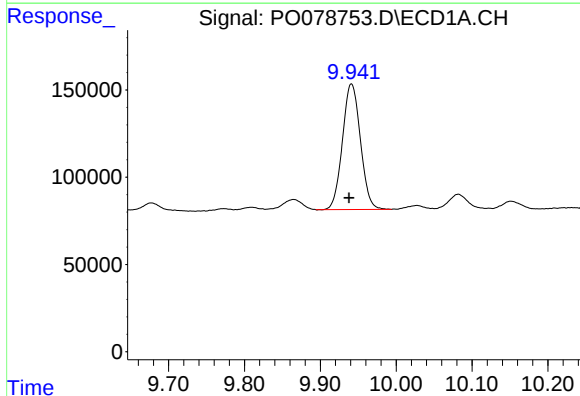


#2 Decachlorobiphenyl

R.T.: 9.941 min
Delta R.T.: 0.003 min
Response: 1185510
Conc: 20.20 ng/ml

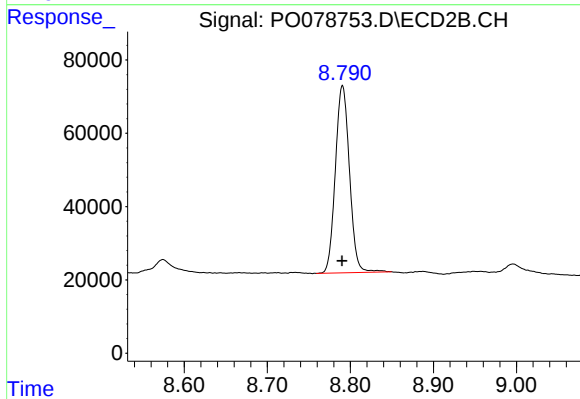

#2 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 603497
Conc: 19.41 ng/ml

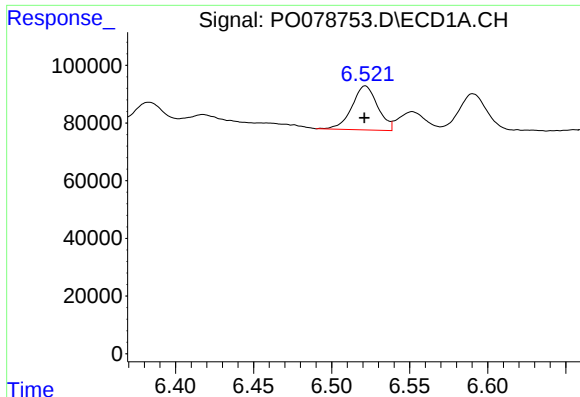


#26 AR-1254-1

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 175479
Conc: 64.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
0241-AMND-COMP-F(CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 4:23:30 PM

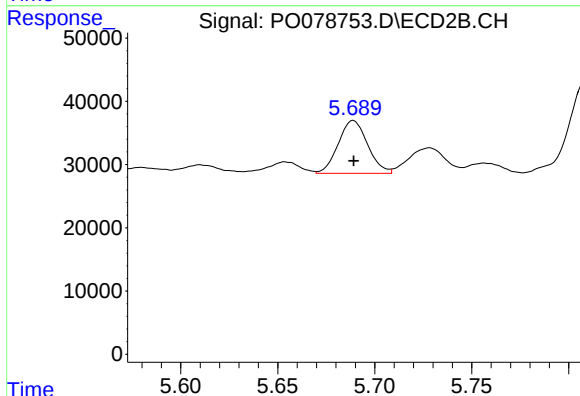


#26 AR-1254-1

R.T.: 5.689 min
Delta R.T.: 0.000 min
Response: 88293
Conc: 49.97 ng/ml m

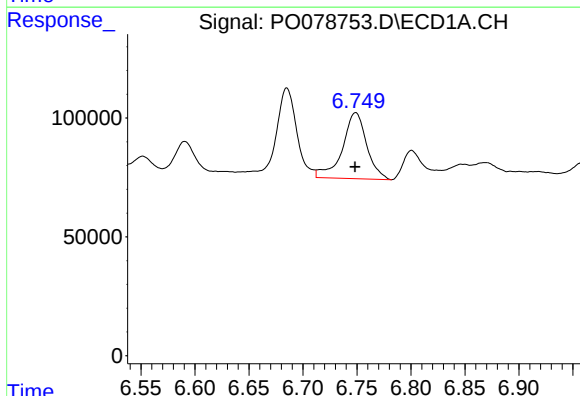


#27 AR-1254-2

R.T.: 6.749 min
Delta R.T.: 0.000 min
Response: 435482
Conc: 102.96 ng/ml

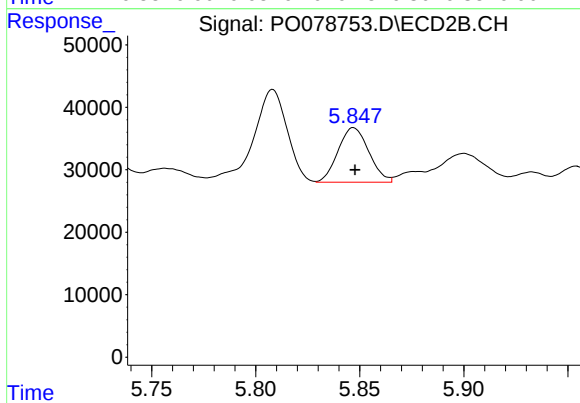

#27 AR-1254-2

R.T.: 5.847 min
Delta R.T.: -0.001 min
Response: 90299
Conc: 55.73 ng/ml m

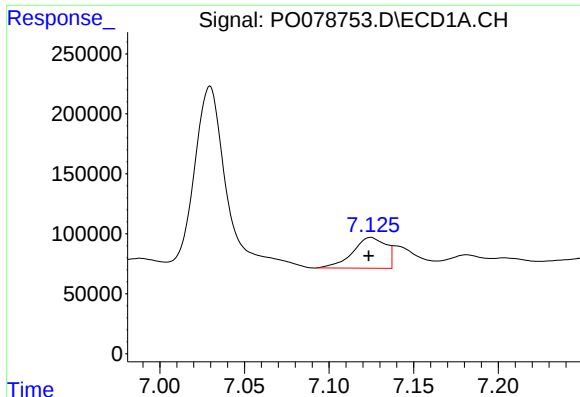


#28 AR-1254-3

R.T.: 7.125 min
Delta R.T.: 0.001 min
Response: 356958
Conc: 81.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0241-AMND-COMP-F(CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 4:23:30 PM

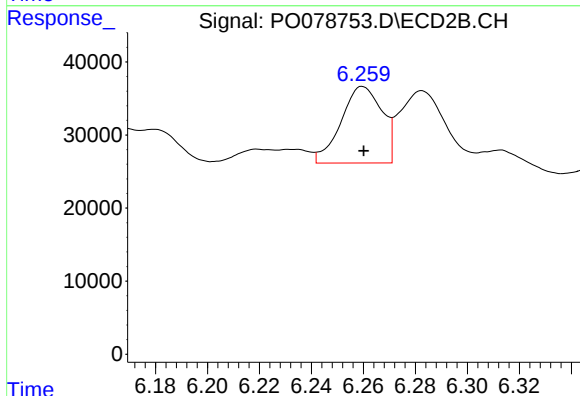


#28 AR-1254-3

R.T.: 6.259 min
Delta R.T.: -0.001 min
Response: 118303
Conc: 48.66 ng/ml m

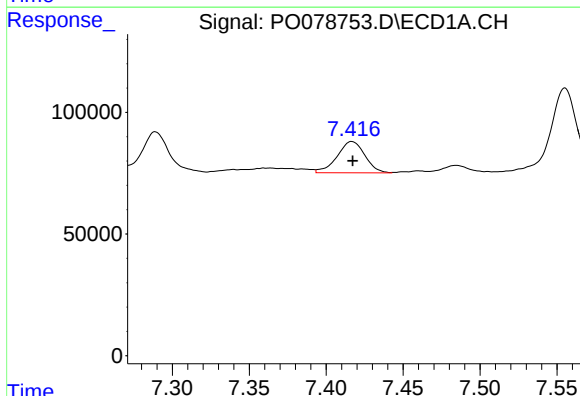


#29 AR-1254-4

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 160278
Conc: 52.07 ng/ml m

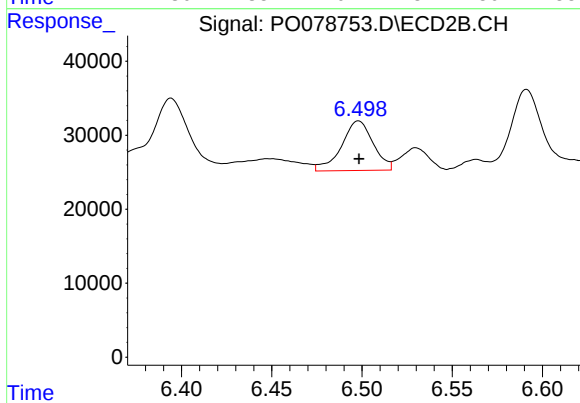

#29 AR-1254-4

R.T.: 6.498 min
Delta R.T.: 0.000 min
Response: 82115
Conc: 54.84 ng/ml

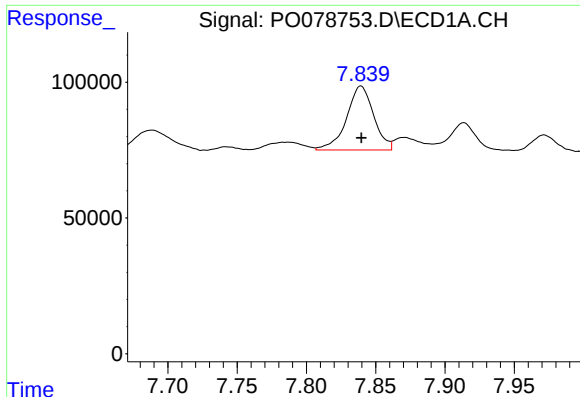


#30 AR-1254-5

R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 321172
Conc: 93.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0241-AMND-COMP-F(CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 4:23:30 PM

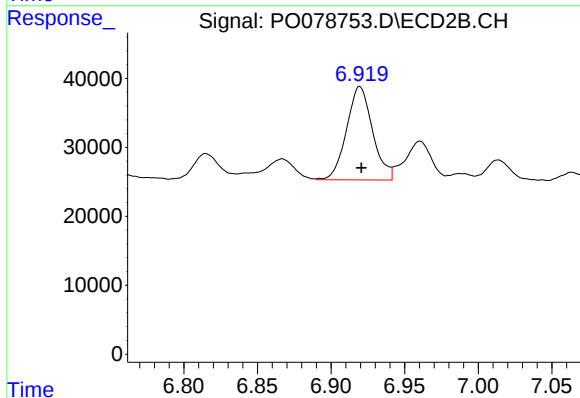


#30 AR-1254-5

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 166795
Conc: 72.66 ng/ml

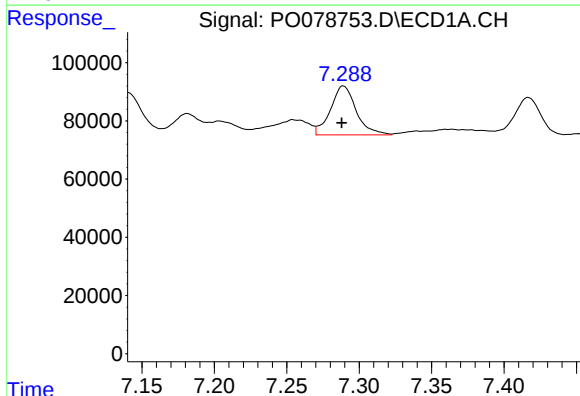


#31 AR-1260-1

R.T.: 7.288 min
Delta R.T.: 0.000 min
Response: 207323
Conc: 65.95 ng/ml m

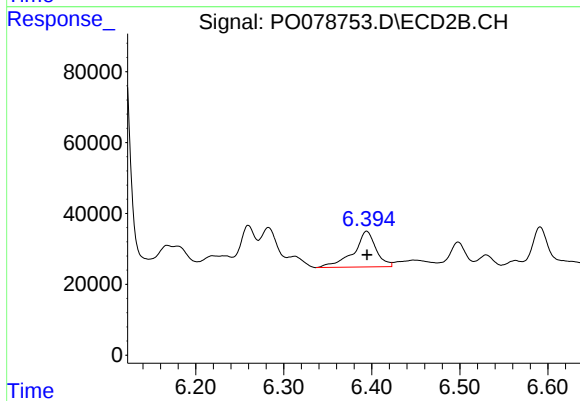

#31 AR-1260-1

R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 179513
Conc: 106.84 ng/ml

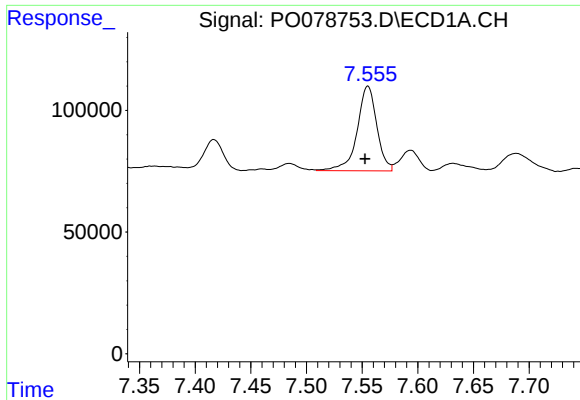


#32 AR-1260-2

R.T.: 7.555 min
Delta R.T.: 0.002 min
Response: 426735
Conc: 115.43 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0241-AMND-COMP-F(CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 4:23:30 PM

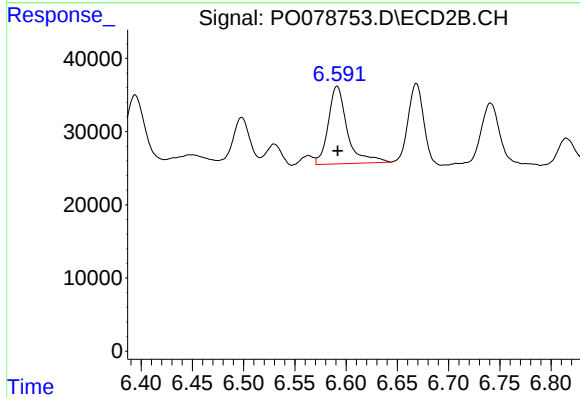


#32 AR-1260-2

R.T.: 6.591 min
Delta R.T.: 0.000 min
Response: 137209
Conc: 68.09 ng/ml

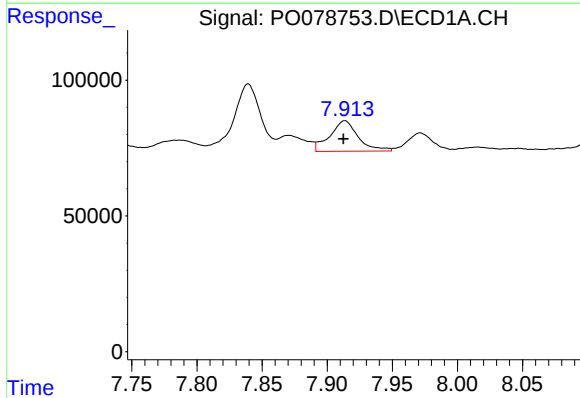


#33 AR-1260-3

R.T.: 7.914 min
Delta R.T.: 0.001 min
Response: 171382
Conc: 60.43 ng/ml

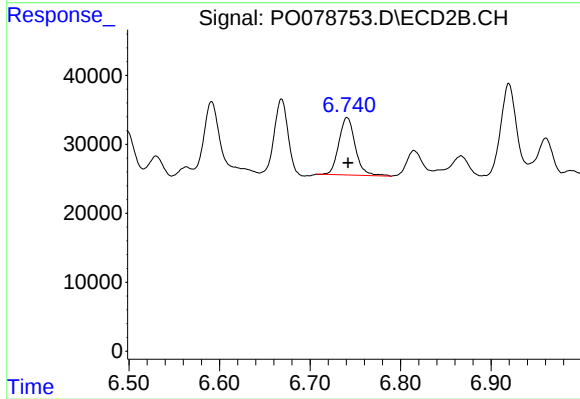

#33 AR-1260-3

R.T.: 6.741 min
Delta R.T.: -0.001 min
Response: 105137
Conc: 53.90 ng/ml

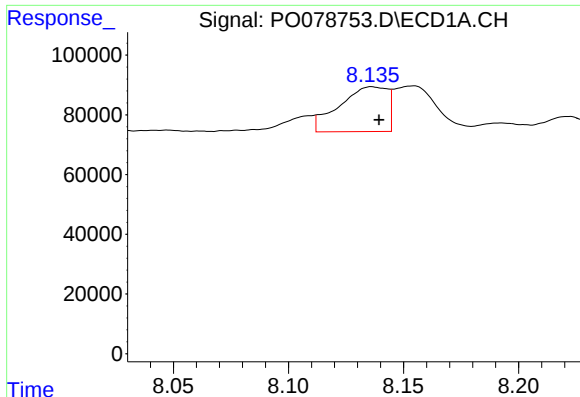


#34 AR-1260-4

R.T.: 8.135 min
Delta R.T.: -0.004 min
Response: 219820
Conc: 69.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0241-AMND-COMP-F(CL-05)


Manual Integrations
APPROVED

Ankita
6/15/2021 4:23:30 PM

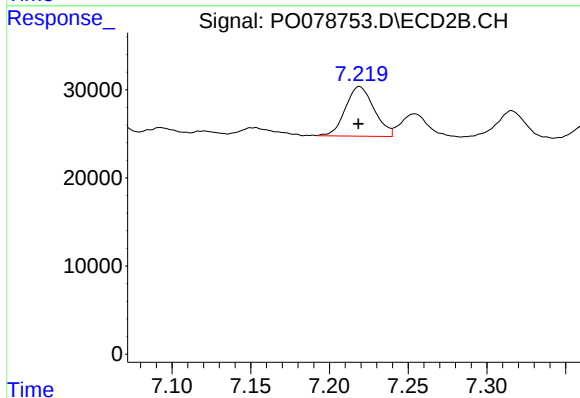


#34 AR-1260-4

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 71699
Conc: 44.87 ng/ml

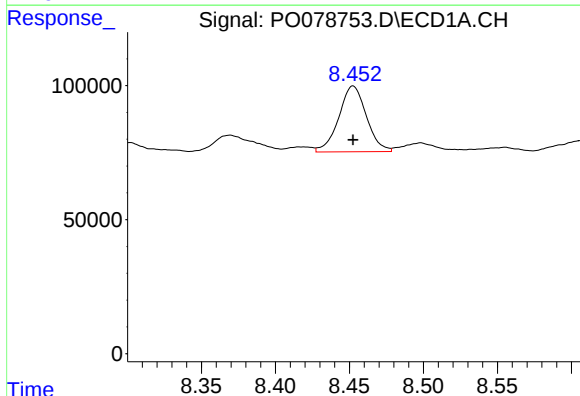

#35 AR-1260-5

R.T.: 8.452 min
Delta R.T.: 0.000 min
Response: 319227
Conc: 52.31 ng/ml

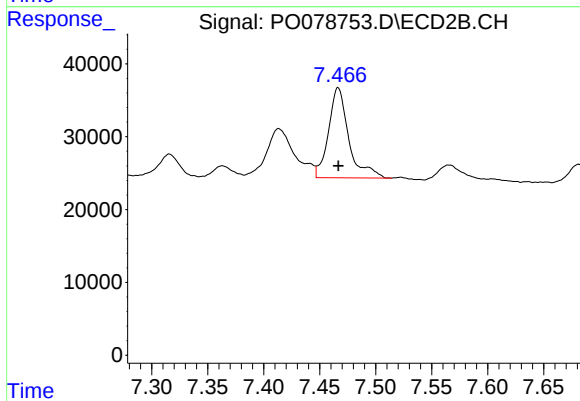

#35 AR-1260-5

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 155471
Conc: 42.26 ng/ml