

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061423\
 Data File : P0095696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2023 16:08
 Operator : YP/AJ
 Sample : 03171-01DL 100X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40236DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :Ankita Jodhani 06/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 17:12:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 10 06:51:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
26)	L6	AR-1254-1	6.448	5.521	52325152 30228390	423.070 435.309
27)	L6	AR-1254-2	6.669	5.670	59691692 21203684	333.828 332.407
28)	L6	AR-1254-3	7.038	6.076	28956651 16955868	167.008 184.959
29)	L6	AR-1254-4	7.326	6.306	18804262 4978290	163.980m 116.713 #
30)	L6	AR-1254-5	7.750	6.727	11648708 6864619	84.465 88.296

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO061423\
Data File : PO095696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2023 16:08
Operator : YP/AJ
Sample : 03171-01DL 100X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
40236DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :Ankita Jodhani 06/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 17:12:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 10 06:51:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

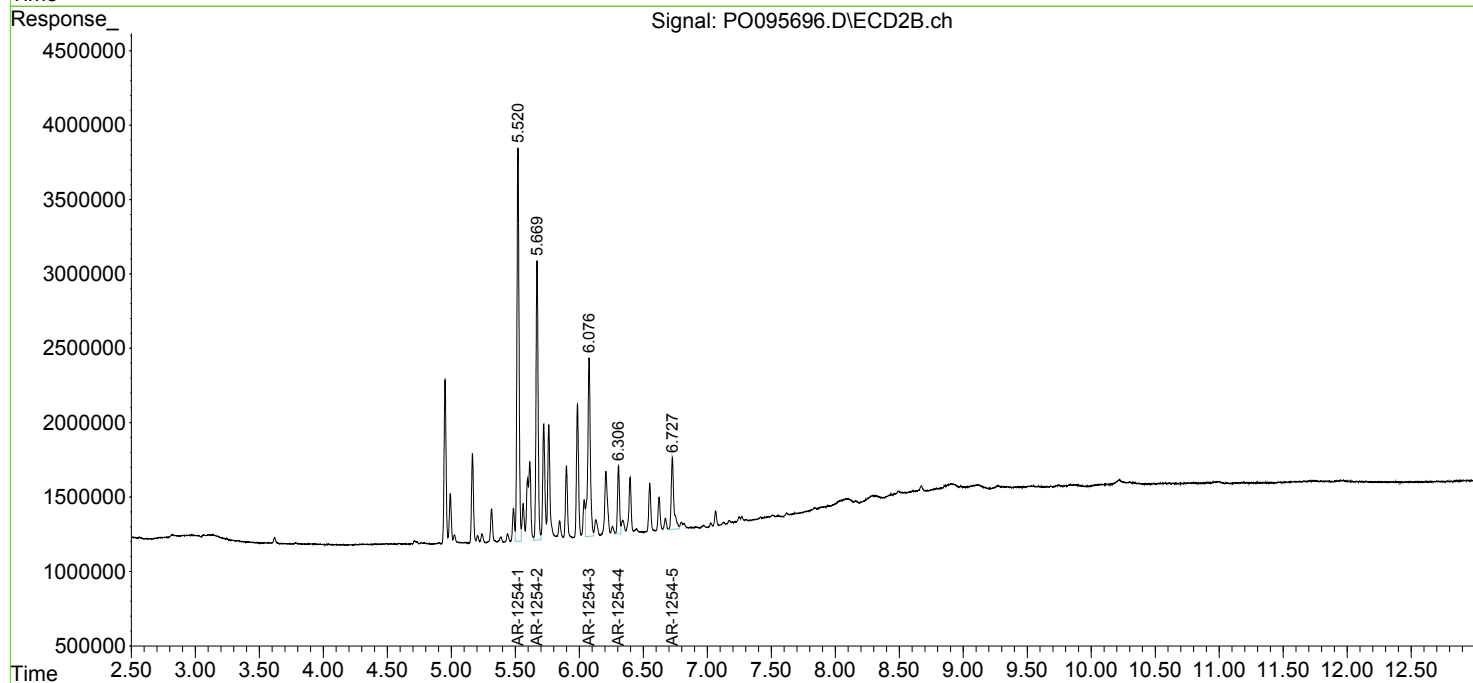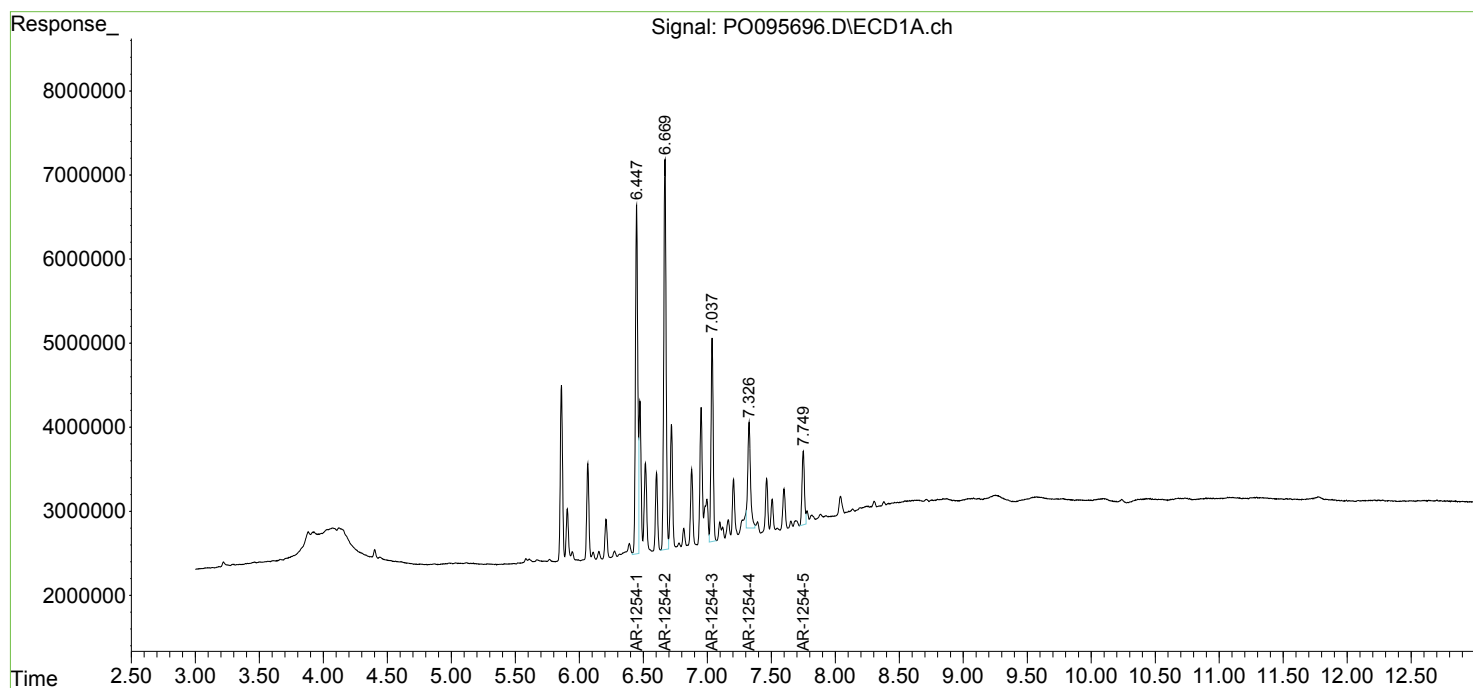

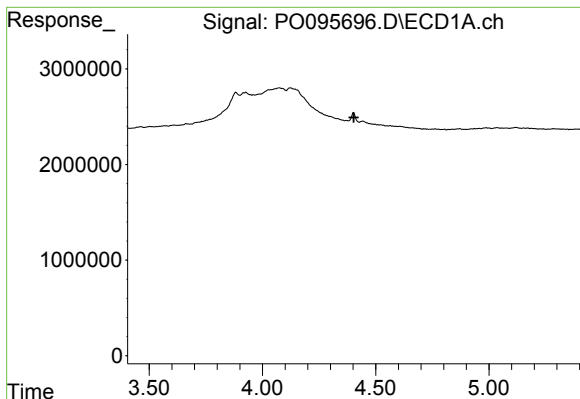


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.403 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
40236DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :Ankita Jodhani 06/15/2023

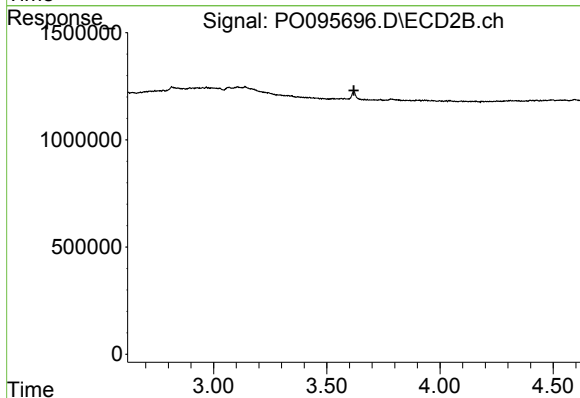


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.619 min
Response: 0
Conc: N.D.

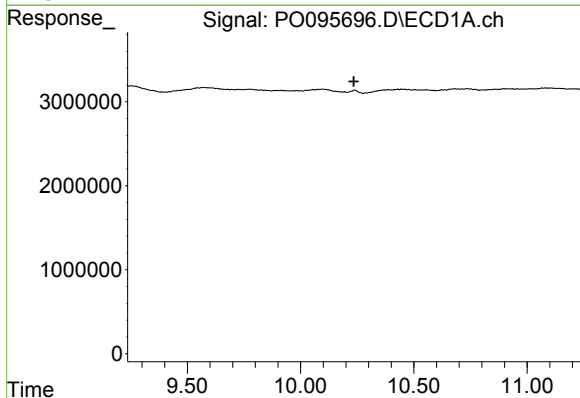


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.236 min
Response: 0
Conc: N.D.

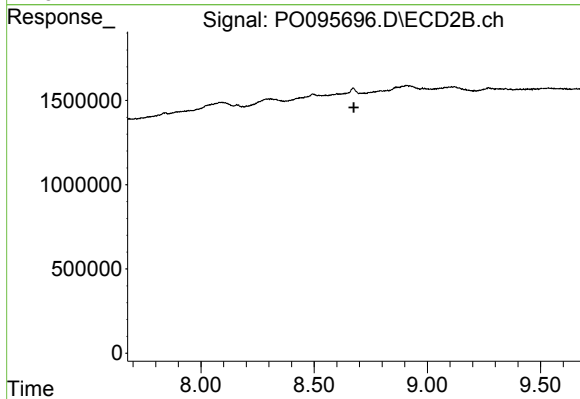

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.675 min
Response: 0
Conc: N.D.

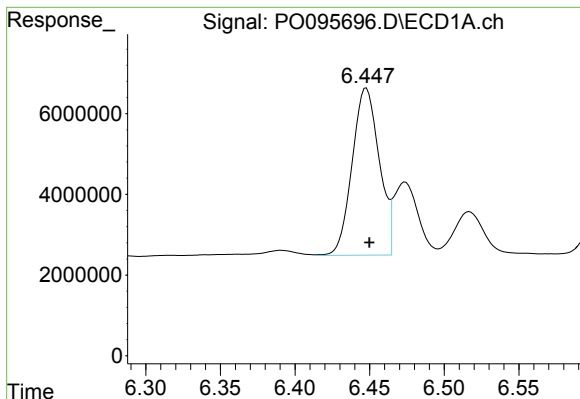


#26 AR-1254-1

R.T.: 6.448 min
Delta R.T.: -0.002 min
Response: 52325152
Conc: 423.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
40236DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :Ankita Jodhani 06/15/2023

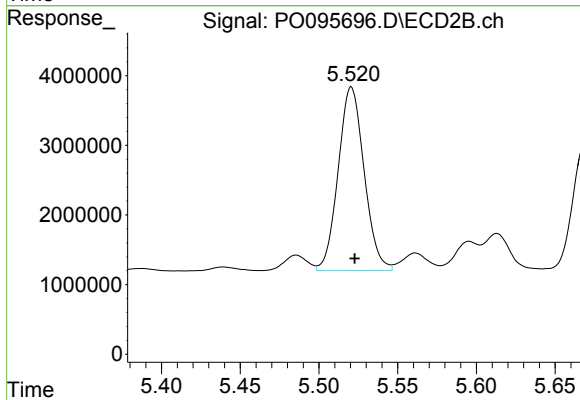


#26 AR-1254-1

R.T.: 5.521 min
Delta R.T.: -0.002 min
Response: 30228390
Conc: 435.31 ng/ml

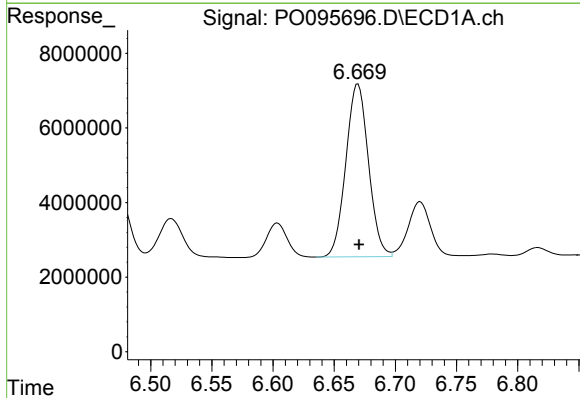


#27 AR-1254-2

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 59691692
Conc: 333.83 ng/ml

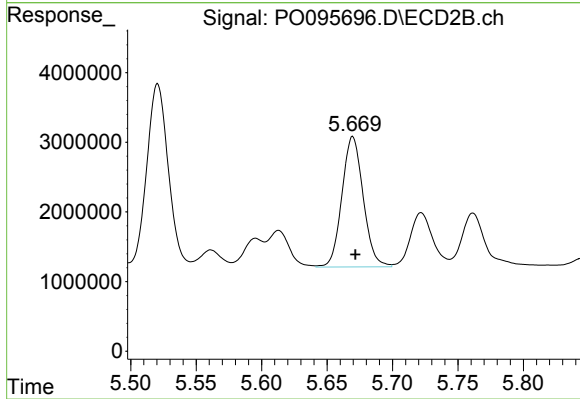

#27 AR-1254-2

R.T.: 5.670 min
Delta R.T.: -0.002 min
Response: 21203684
Conc: 332.41 ng/ml

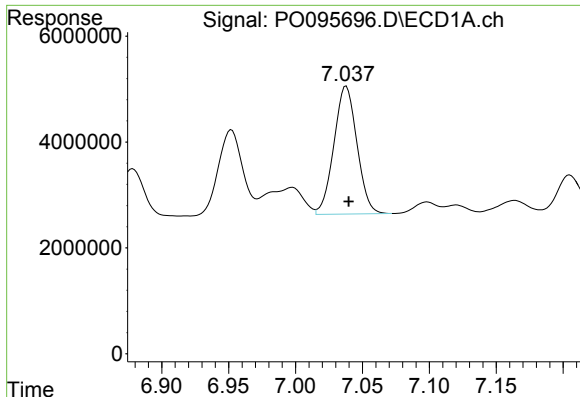


#28 AR-1254-3

R.T.: 7.038 min
Delta R.T.: -0.002 min
Response: 28956651
Conc: 167.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
40236DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :Ankita Jodhani 06/15/2023

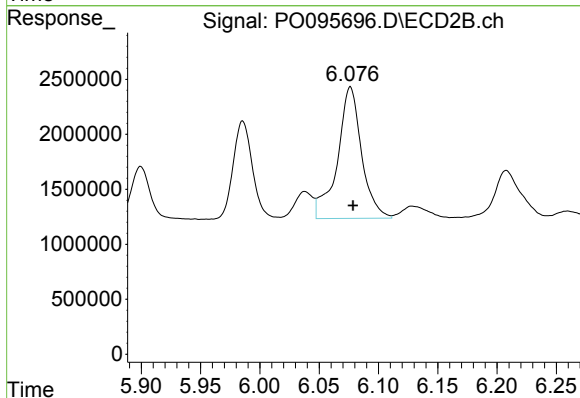


#28 AR-1254-3

R.T.: 6.076 min
Delta R.T.: -0.002 min
Response: 16955868
Conc: 184.96 ng/ml

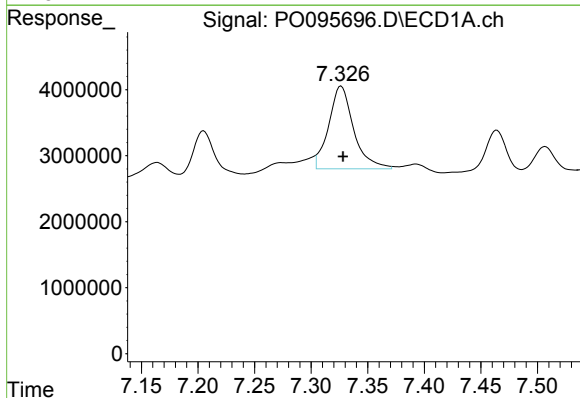


#29 AR-1254-4

R.T.: 7.326 min
Delta R.T.: -0.002 min
Response: 18804262
Conc: 163.98 ng/ml m

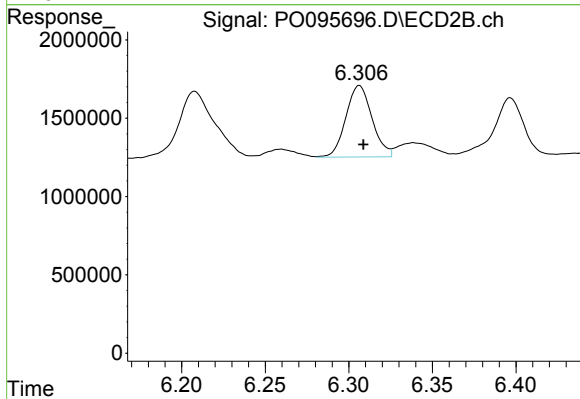

#29 AR-1254-4

R.T.: 6.306 min
Delta R.T.: -0.002 min
Response: 4978290
Conc: 116.71 ng/ml

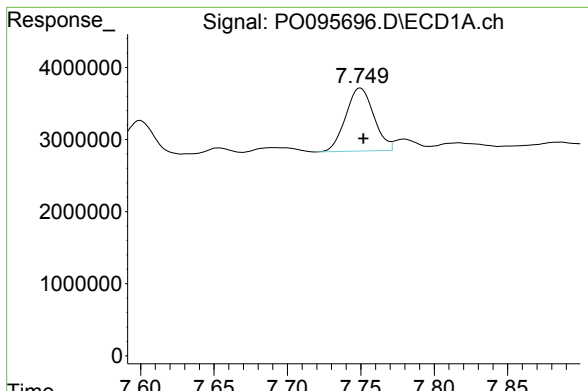

#30 AR-1254-5

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 11648708
Conc: 84.47 ng/ml

Instrument :

ECD_O

ClientSampleId :


40236DL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/15/2023

Supervised By :Ankita Jodhani 06/15/2023

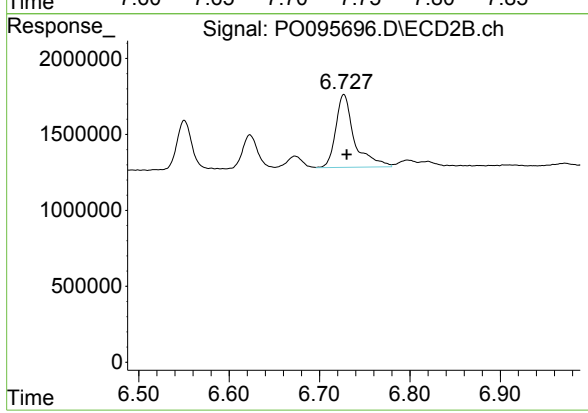

#30 AR-1254-5

R.T.: 6.727 min
Delta R.T.: -0.003 min
Response: 6864619
Conc: 88.30 ng/ml