

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061423\
 Data File : P0095708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2023 20:47
 Operator : YP/AJ
 Sample : 03168-01 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH238R-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/15/2023
 Supervised By :Ankita Jodhani 06/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 01:18:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 10 06:51:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.618	9086802	3612048	2.120	1.987
2) SA Decachlor...	10.238	8.671	6370816	2748259	2.556	2.468m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061423\
Data File : PO095708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2023 20:47
Operator : YP/AJ
Sample : 03168-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH238R-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :Ankita Jodhani 06/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 01:18:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 10 06:51:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

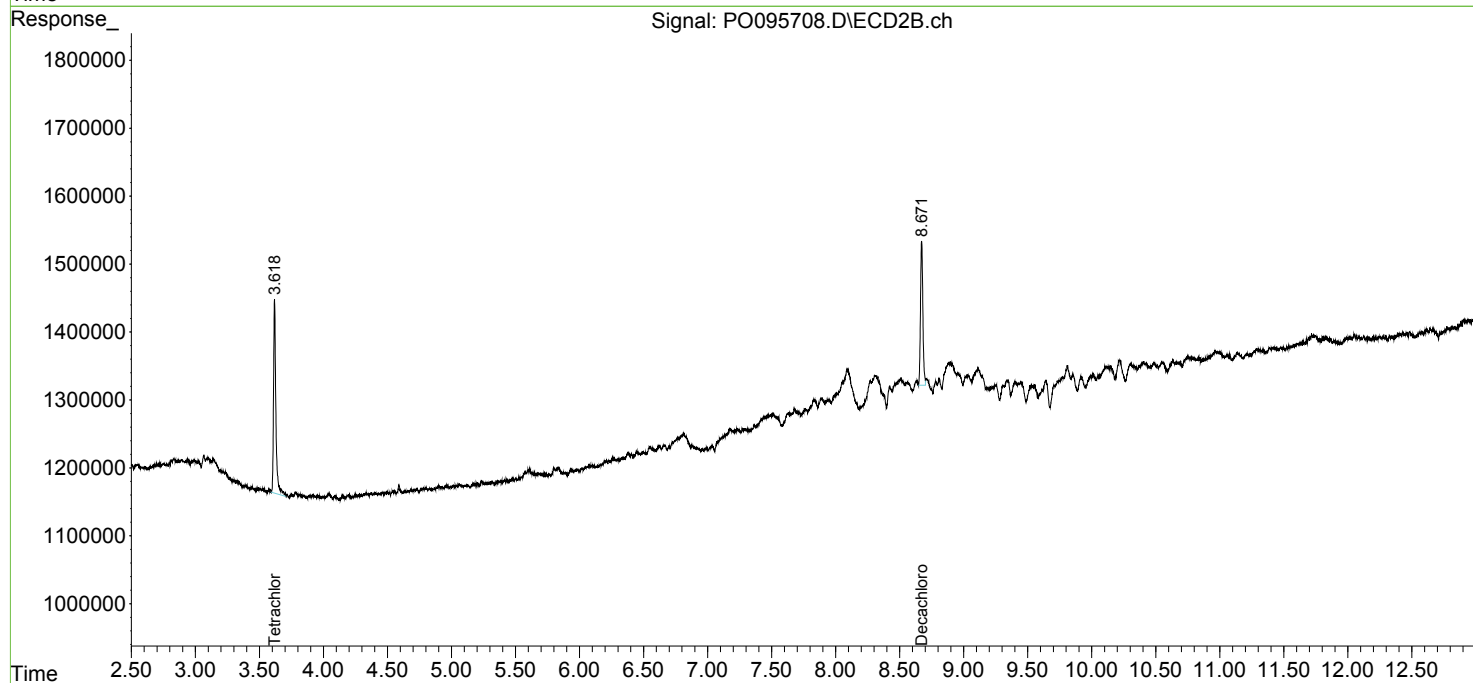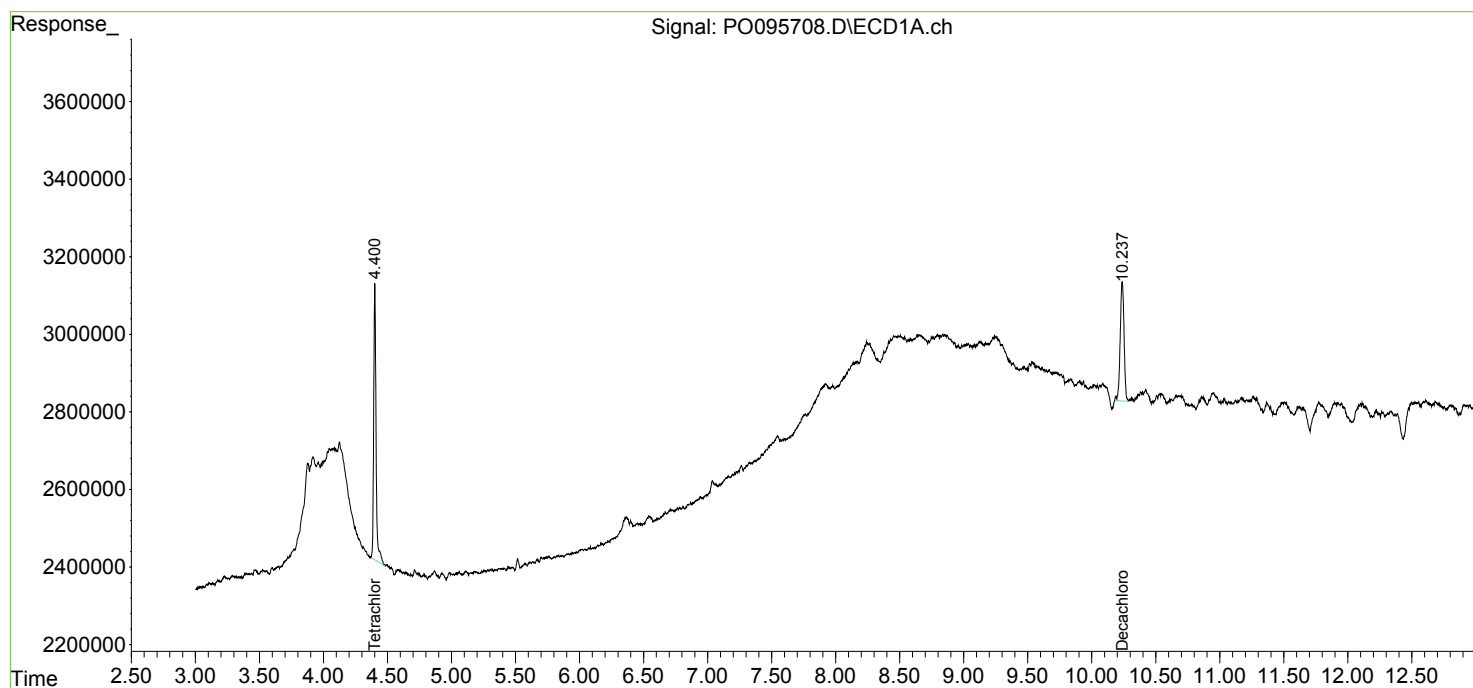

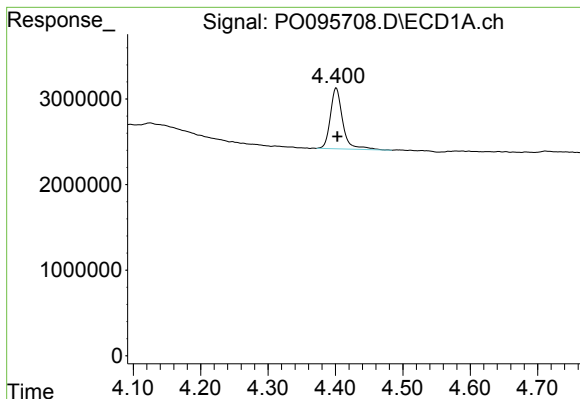

#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.002 min
Response: 9086802
Conc: 2.12 ng/ml

Instrument :

ECD_O


ClientSampleId :

KMH238R-1-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/15/2023
Supervised By :Ankita Jodhani 06/15/2023

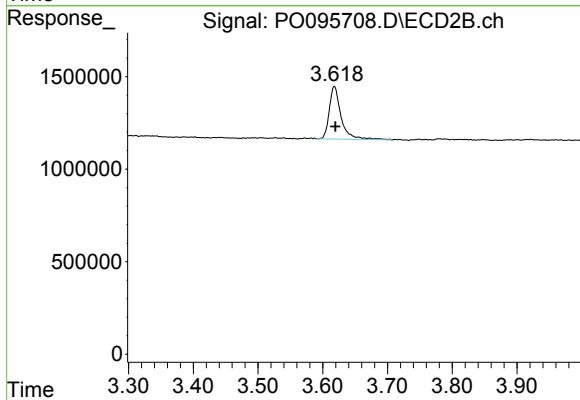


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.001 min
Response: 3612048
Conc: 1.99 ng/ml

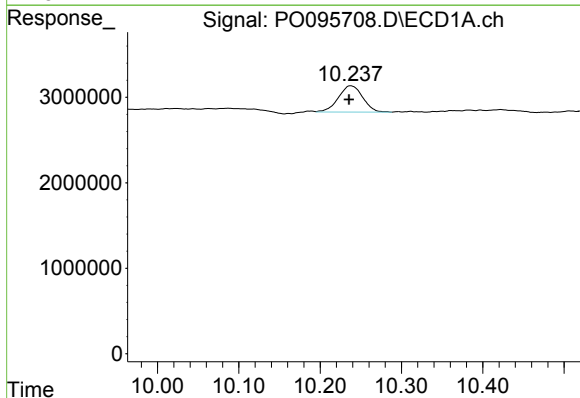

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: 0.002 min
Response: 6370816
Conc: 2.56 ng/ml

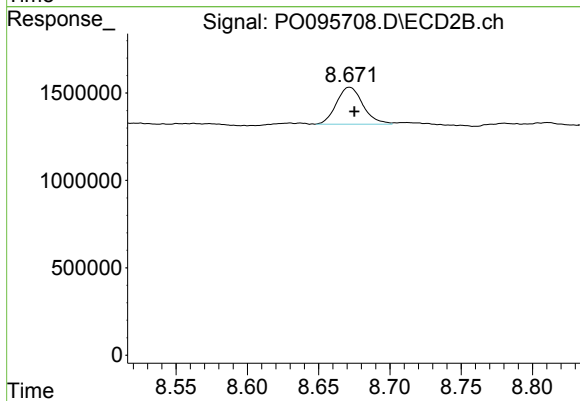

#2 Decachlorobiphenyl

R.T.: 8.671 min
Delta R.T.: -0.004 min
Response: 2748259
Conc: 2.47 ng/ml m