

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061423\
 Data File : P0095717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 00:34
 Operator : YP/AJ
 Sample : 03163-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 149TH-ST-DRUM-15-POLY

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 01:21:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 10 06:51:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.618	111.0E6	46633528	25.892	25.652
2) SA Decachlor...	10.240	8.672	71483492	35173224	28.682	31.582

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061423\
Data File : P0095717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 00:34
Operator : YP/AJ
Sample : 03163-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
149TH-ST-DRUM-15-POLY

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 01:21:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 10 06:51:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

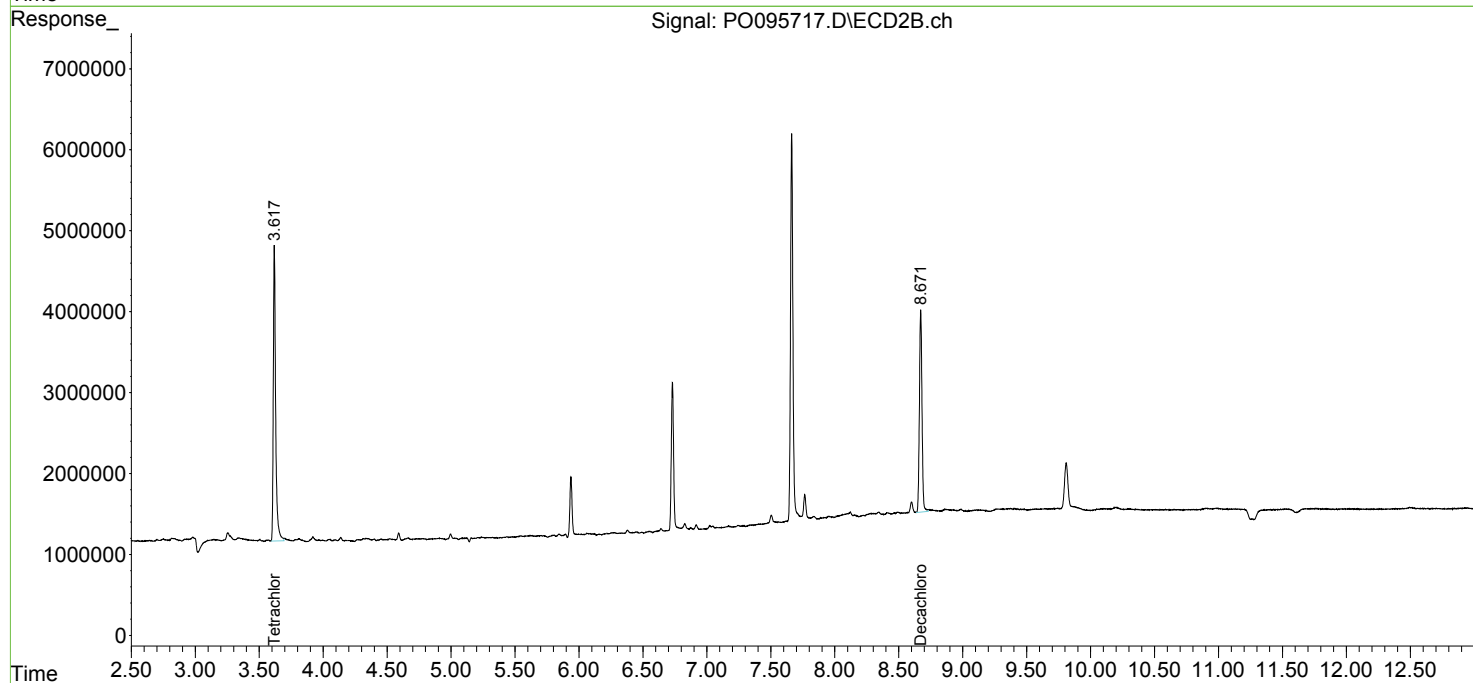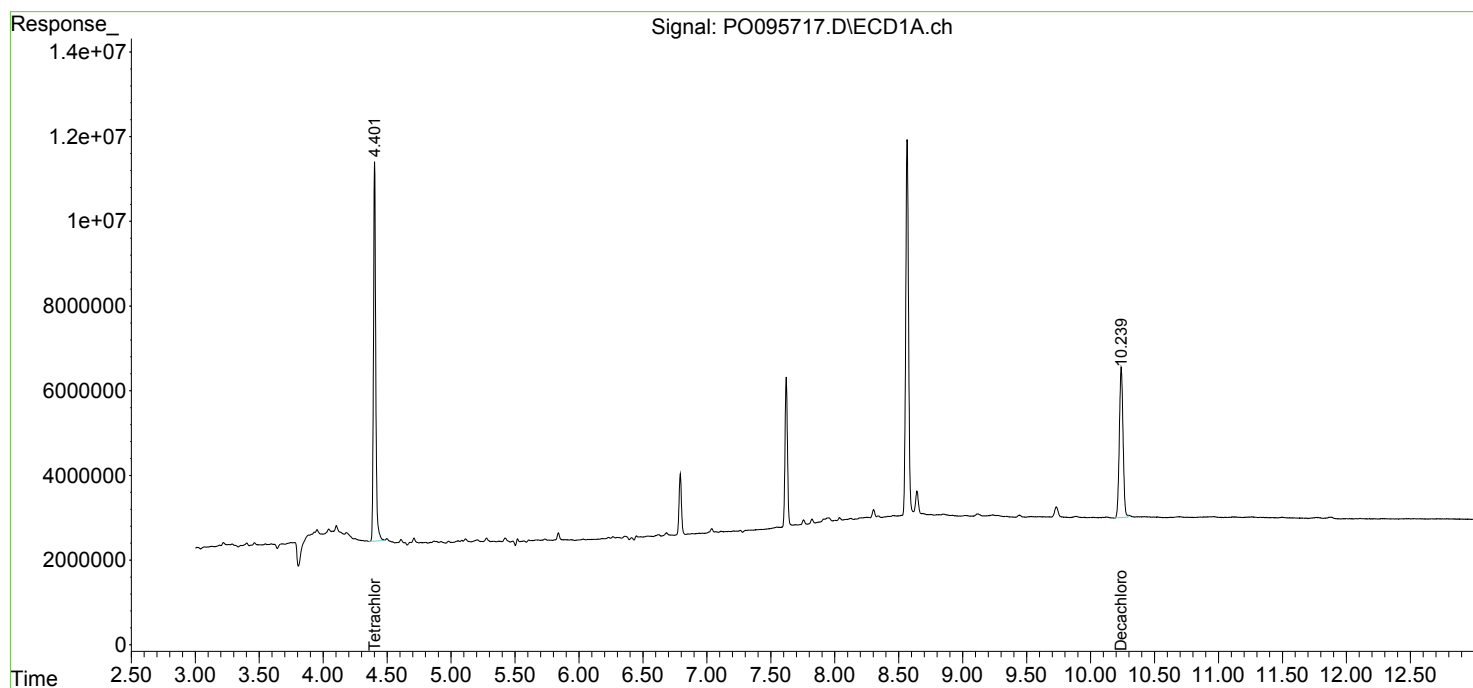


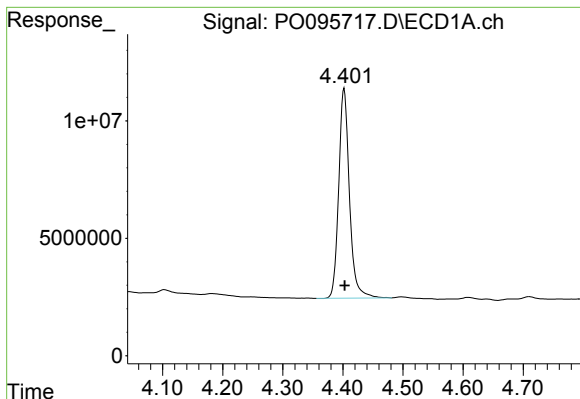

#1 Tetrachloro-m-xylene


R.T.: 4.402 min
Delta R.T.: 0.000 min
Response: 110979885
Conc: 25.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
149TH-ST-DRUM-15-POLY

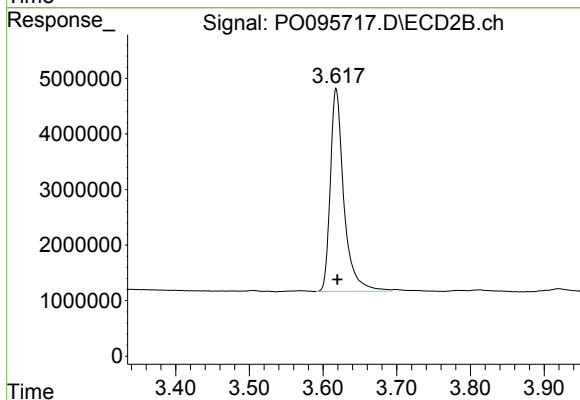


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.002 min
Response: 46633528
Conc: 25.65 ng/ml

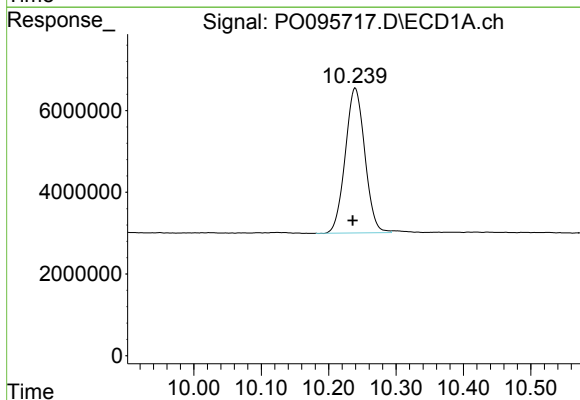

#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: 0.004 min
Response: 71483492
Conc: 28.68 ng/ml

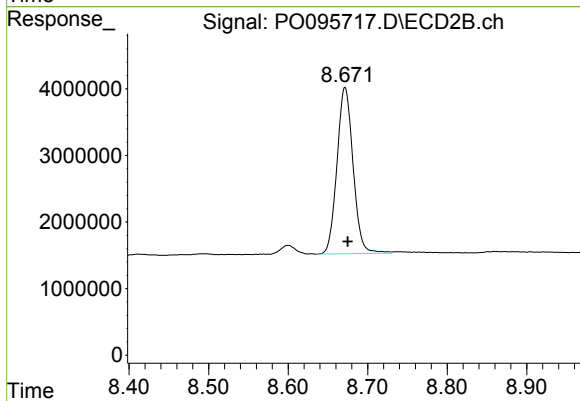

#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: -0.004 min
Response: 35173224
Conc: 31.58 ng/ml