

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061424\
 Data File : P0104336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2024 11:22
 Operator : YP/AJ
 Sample : P2853-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/17/2024
 Supervised By :Ankita Jodhani 06/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 23:22:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 12 05:42:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.546	156.5E6	42189833	18.756m	19.569m
2) SA Decachlor...	10.104	8.458	96738508	49842508	16.514	15.571

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061424\
Data File : PO104336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2024 11:22
Operator : YP/AJ
Sample : P2853-10
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/17/2024
Supervised By :Ankita Jodhani 06/17/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 23:22:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061124.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 12 05:42:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

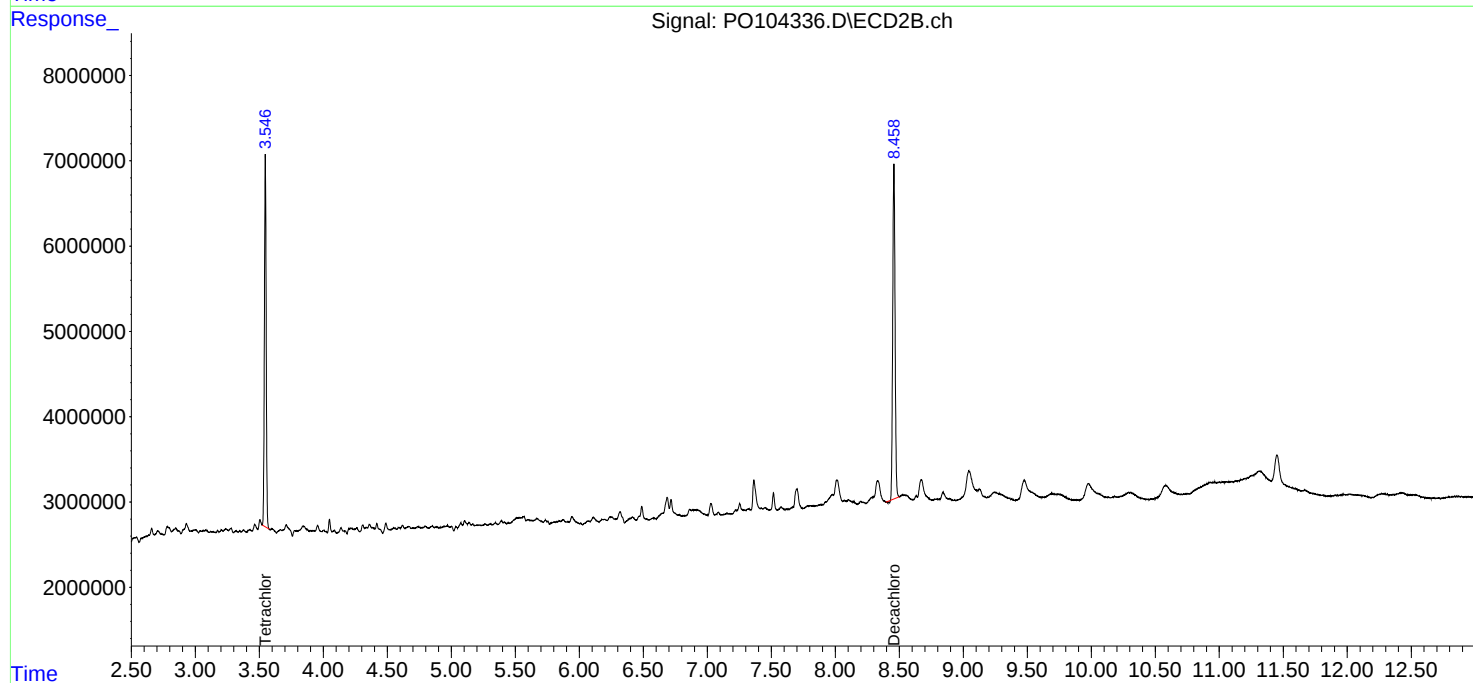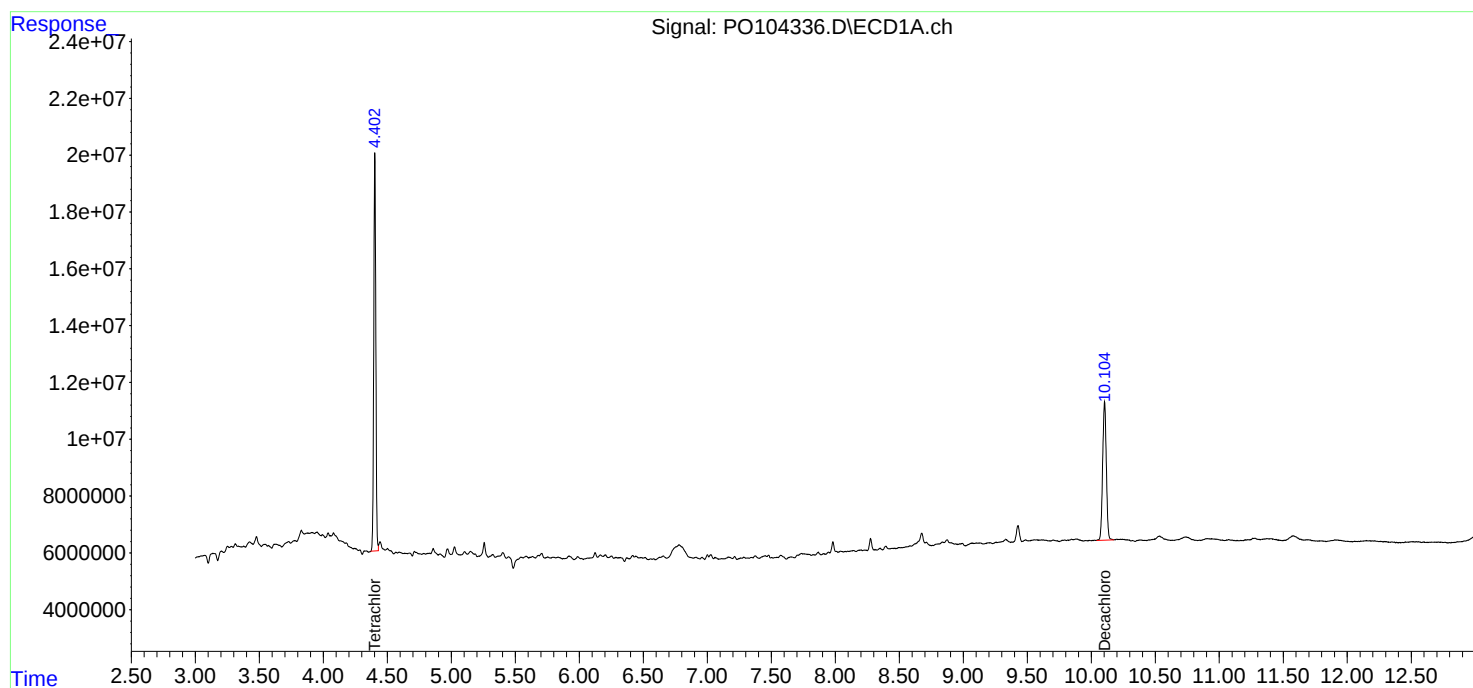

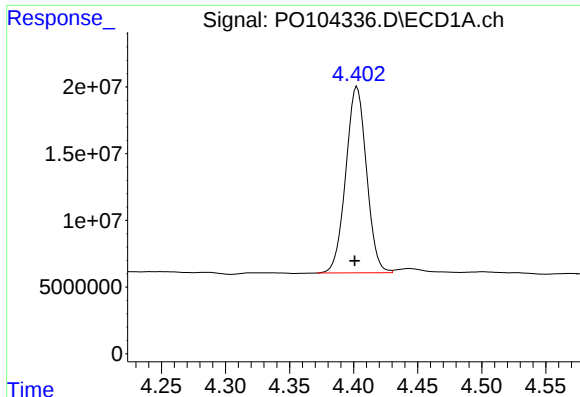


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: 0.000 min
Response: 156528658
Conc: 18.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/17/2024
Supervised By :Ankita Jodhani 06/17/2024

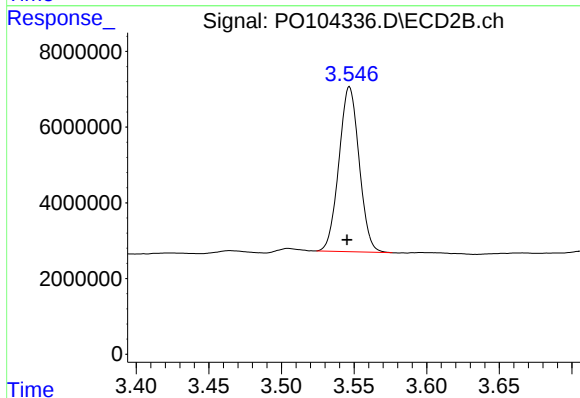


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.001 min
Response: 42189833
Conc: 19.57 ng/ml m

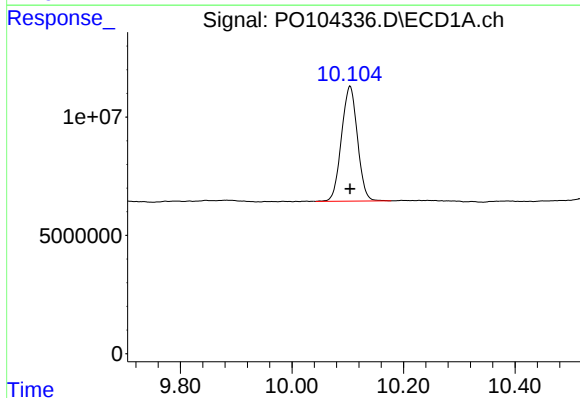

#2 Decachlorobiphenyl

R.T.: 10.104 min
Delta R.T.: 0.000 min
Response: 96738508
Conc: 16.51 ng/ml

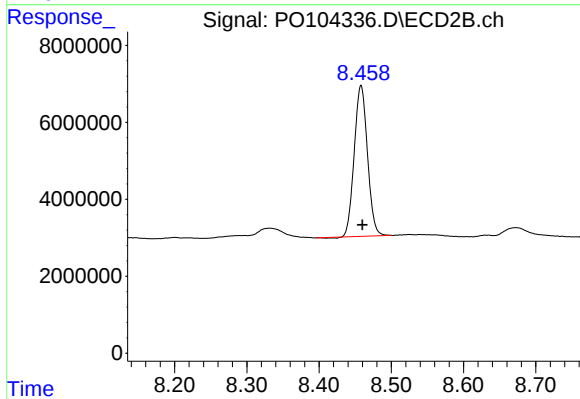

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 49842508
Conc: 15.57 ng/ml