

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061521\
 Data File : P0078805.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jun 2021 17:42
 Operator : DD\AJ
 Sample : M2372-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 02:21:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.330	3.606	1759422	717763	20.781	20.734
2)	SA Decachlor...	9.938	8.789	1206321	644493	20.556	20.729
Target Compounds							
8)	L2 AR-1221-1	4.575	0.000	37679	0	41.871	N.D. #
9)	L2 AR-1221-2	4.673	0.000	17428	0	26.266	N.D. #
20)	L4 AR-1242-5	6.563f	0.000	697	0	0.463	N.D. #
24)	L5 AR-1248-4	6.556	0.000	1943	0	0.742	N.D. #
25)	L5 AR-1248-5	6.563f	0.000	697	0	0.276	N.D. #
28)	L6 AR-1254-3	7.141f	0.000	25068	0	5.758	N.D. #
32)	L7 AR-1260-2	0.000	6.563f	0	4546	N.D.	2.256 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061521\
Data File : P0078805.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2021 17:42
Operator : DD\AJ
Sample : M2372-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 02:21:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

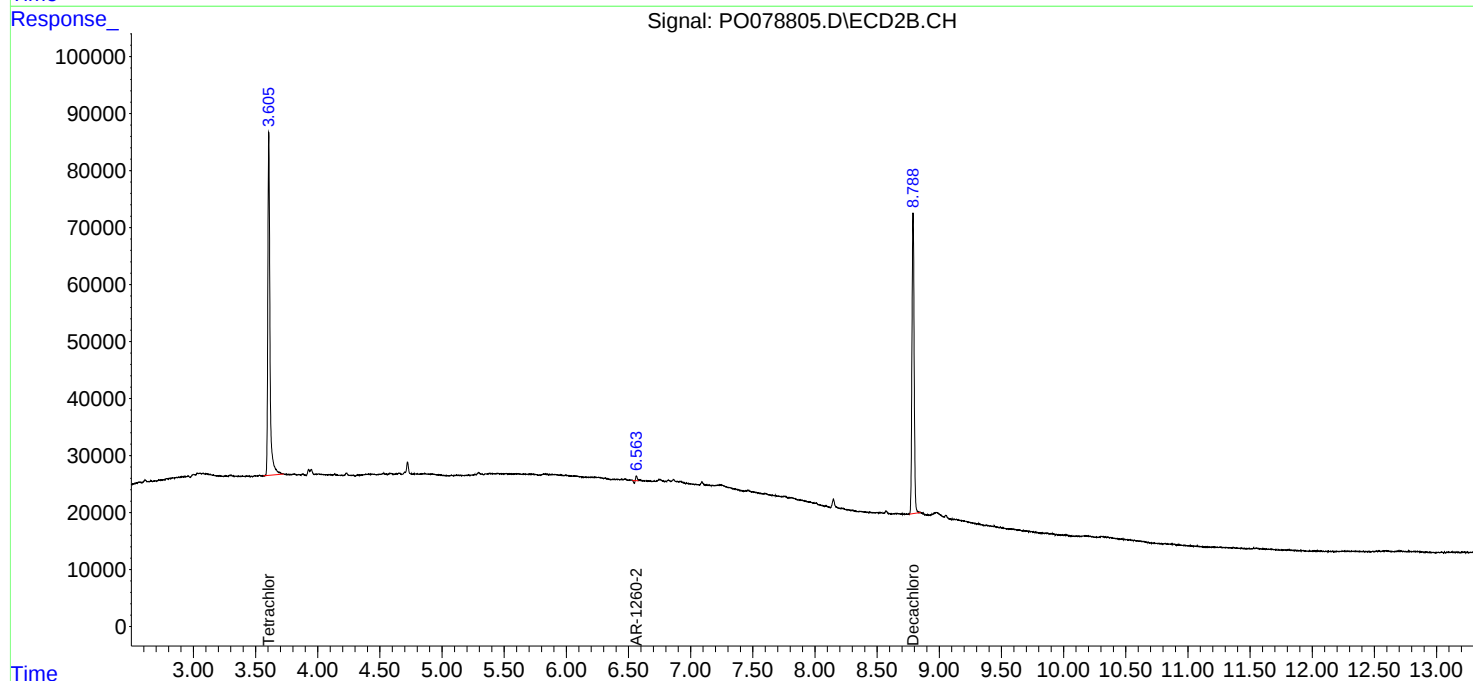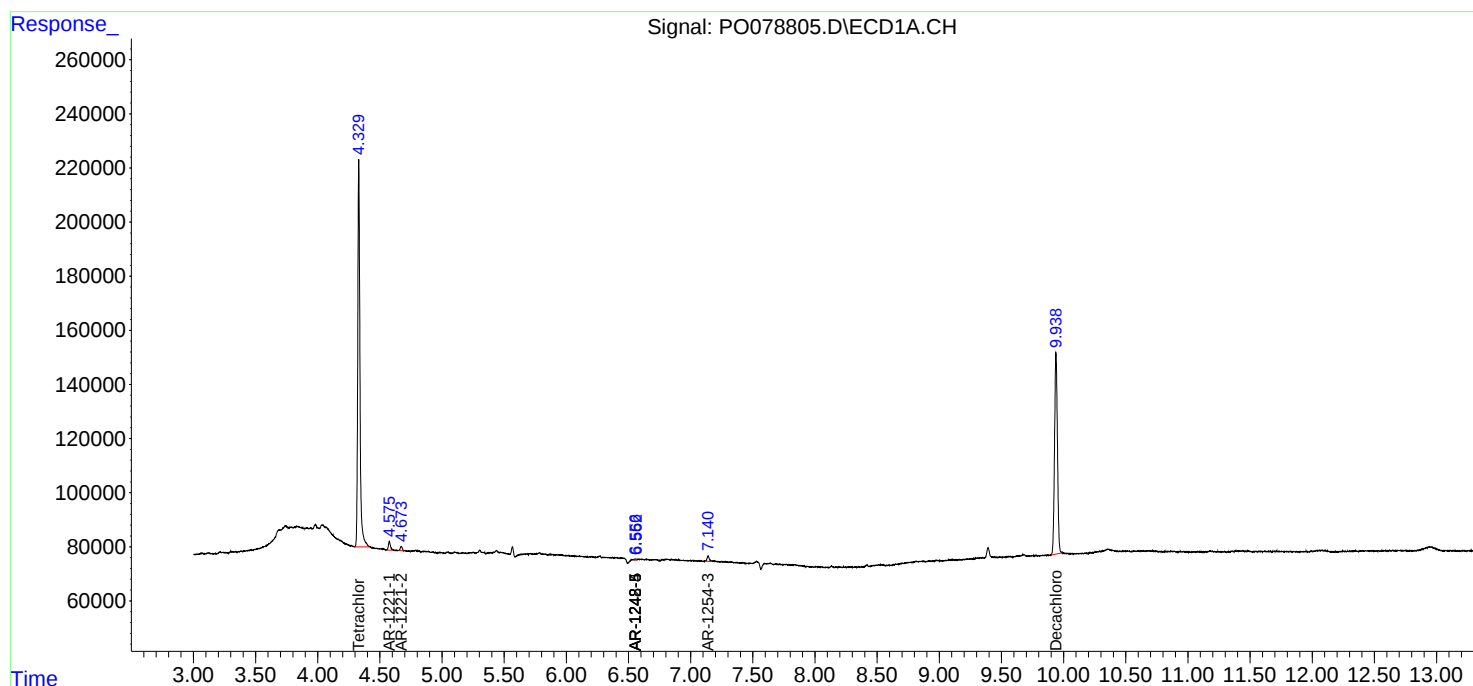


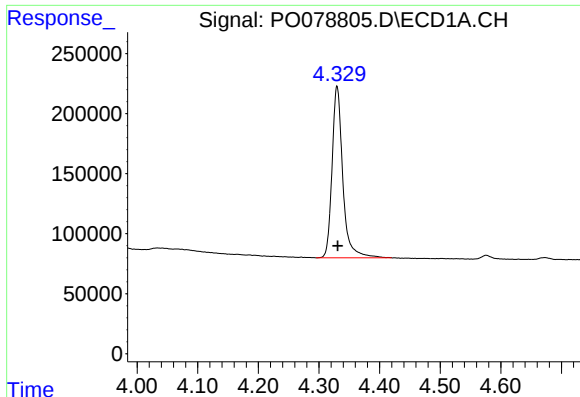

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: -0.001 min
Response: 1759422
Conc: 20.78 ng/ml

Instrument :
ECD_O
ClientSampleId :

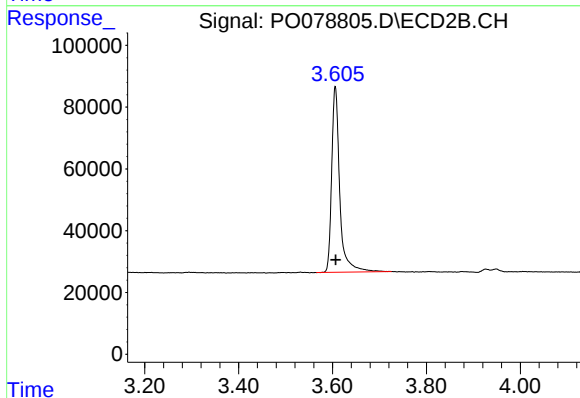


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 717763
Conc: 20.73 ng/ml

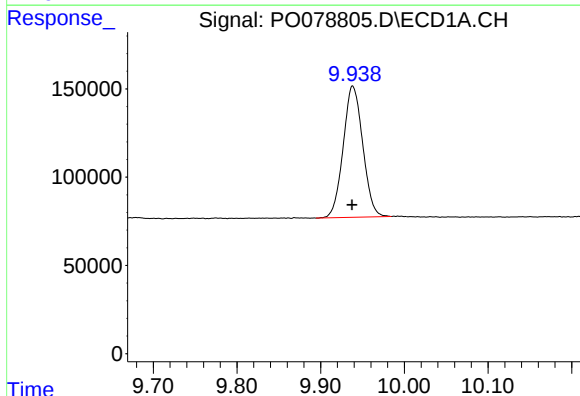


#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.000 min
Response: 1206321
Conc: 20.56 ng/ml

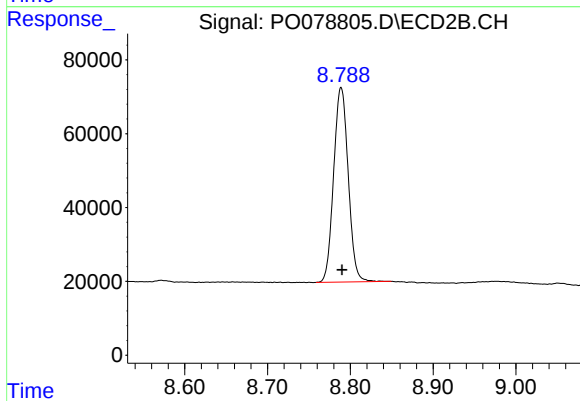

#2 Decachlorobiphenyl


R.T.: 8.789 min
Delta R.T.: -0.001 min
Response: 644493
Conc: 20.73 ng/ml

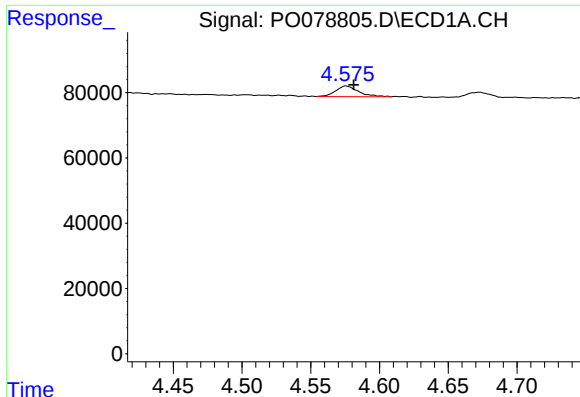

#8 AR-1221-1


R.T.: 4.575 min
Delta R.T.: -0.006 min
Response: 37679
Conc: 41.87 ng/ml

Instrument :
ECD_O
ClientSampleId :

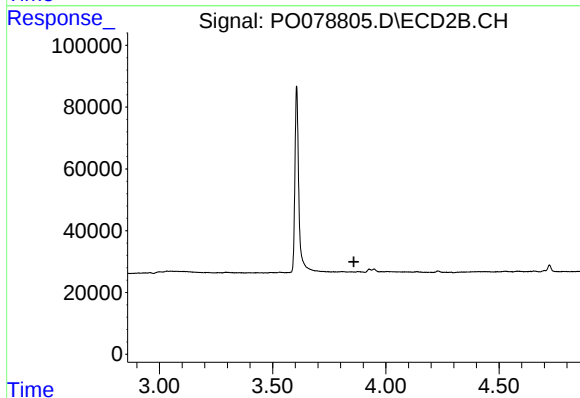


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.859 min
Response: 0
Conc: N.D.

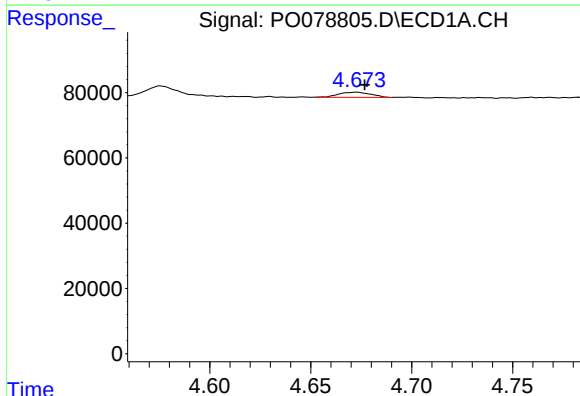


#9 AR-1221-2

R.T.: 4.673 min
Delta R.T.: -0.004 min
Response: 17428
Conc: 26.27 ng/ml

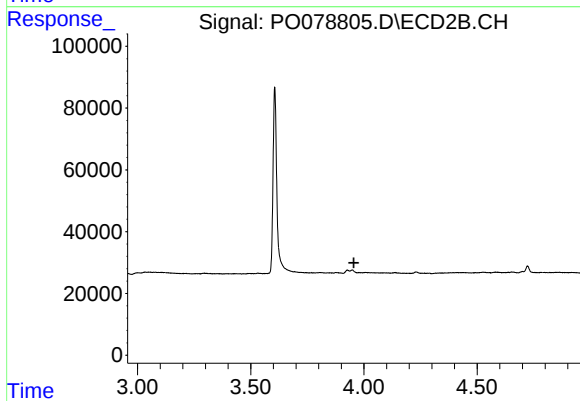

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.956 min
Response: 0
Conc: N.D.

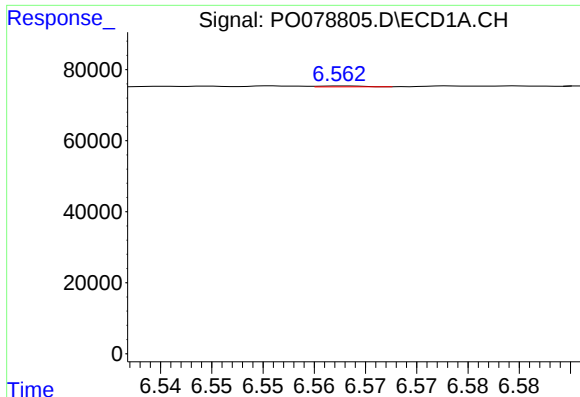

#20 AR-1242-5


R.T.: 6.563 min
Delta R.T.: -0.026 min
Response: 697
Conc: 0.46 ng/ml

Instrument :
ECD_O
ClientSampleId :

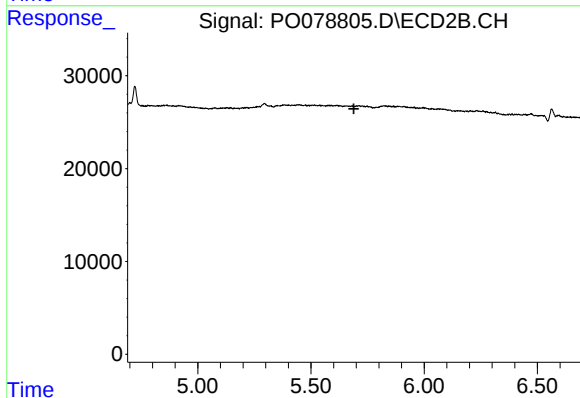


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.690 min
Response: 0
Conc: N.D.

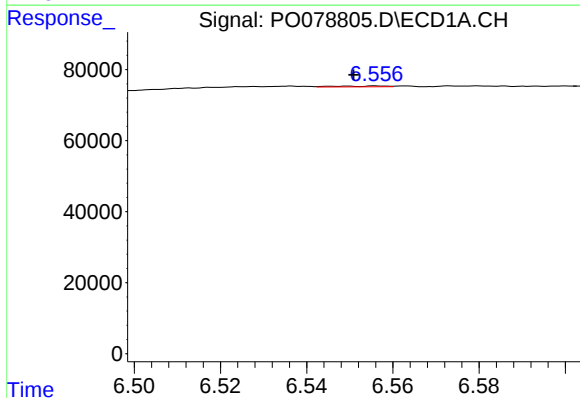


#24 AR-1248-4

R.T.: 6.556 min
Delta R.T.: 0.005 min
Response: 1943
Conc: 0.74 ng/ml

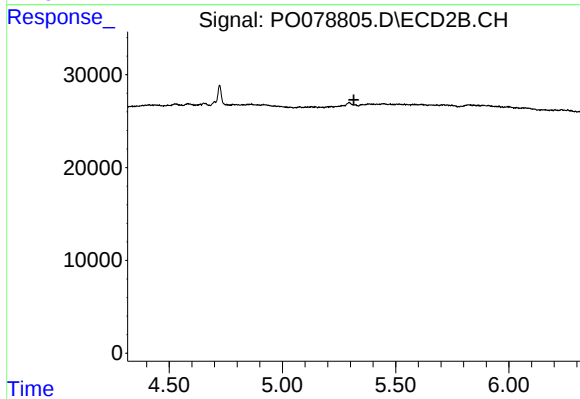

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.316 min
Response: 0
Conc: N.D.

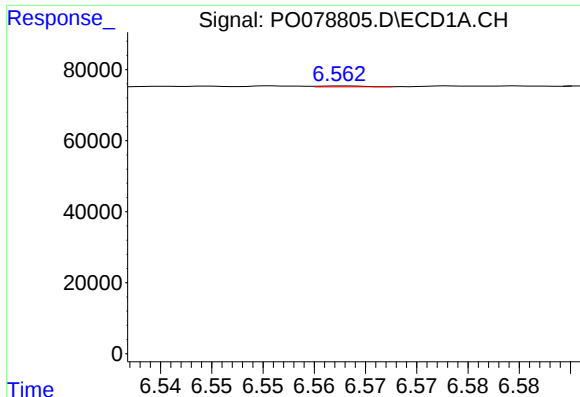

#25 AR-1248-5


R.T.: 6.563 min
Delta R.T.: -0.025 min
Response: 697
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

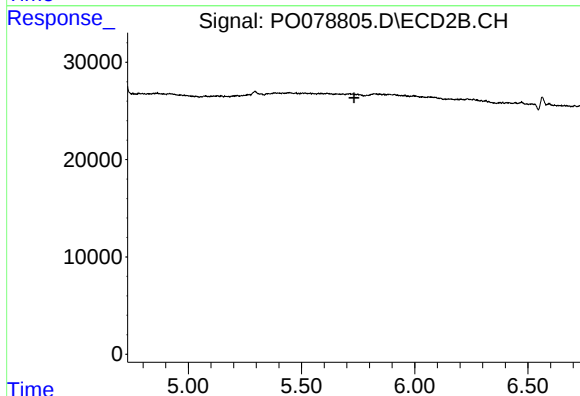


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.732 min
Response: 0
Conc: N.D.

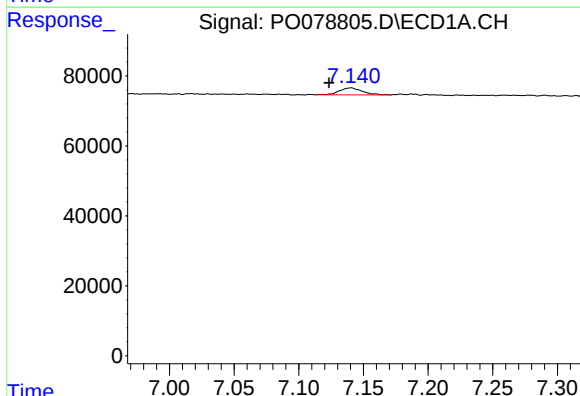


#28 AR-1254-3

R.T.: 7.141 min
Delta R.T.: 0.017 min
Response: 25068
Conc: 5.76 ng/ml

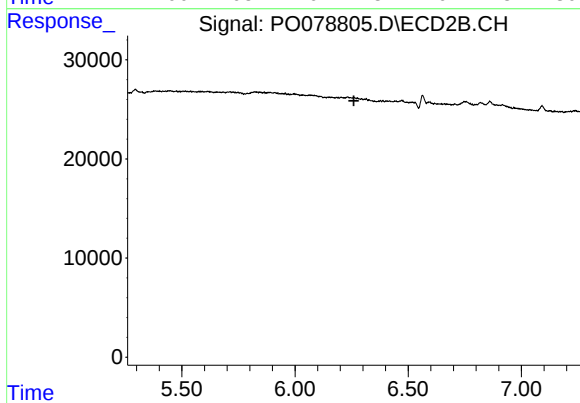

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.260 min
Response: 0
Conc: N.D.

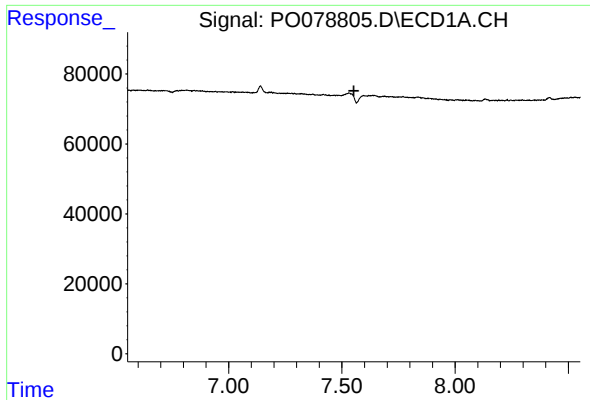

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.553 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

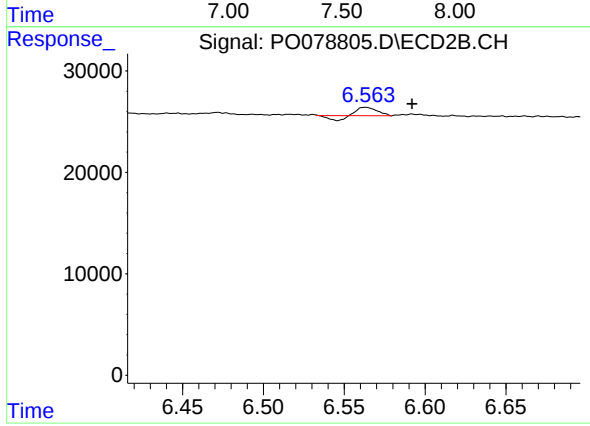

#32 AR-1260-2

R.T.: 6.563 min
Delta R.T.: -0.029 min
Response: 4546
Conc: 2.26 ng/ml