

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061522\
 Data File : P0087177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2022 10:53
 Operator : YP/AJ
 Sample : N3315-08 10X (Sig #1); N3315-08RE 10X (Sig #2)
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDA375-1-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 11:54:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.638	3543411	1781152	1.516	1.582
2) SA Decachlor...	10.345	8.645	3636191	1628325	1.976	2.071

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061522\
Data File : P0087177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2022 10:53
Operator : YP/AJ
Sample : N3315-08 10X (Sig #1); N3315-08RE 10X (Sig #2)
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FDA375-1-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 11:54:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

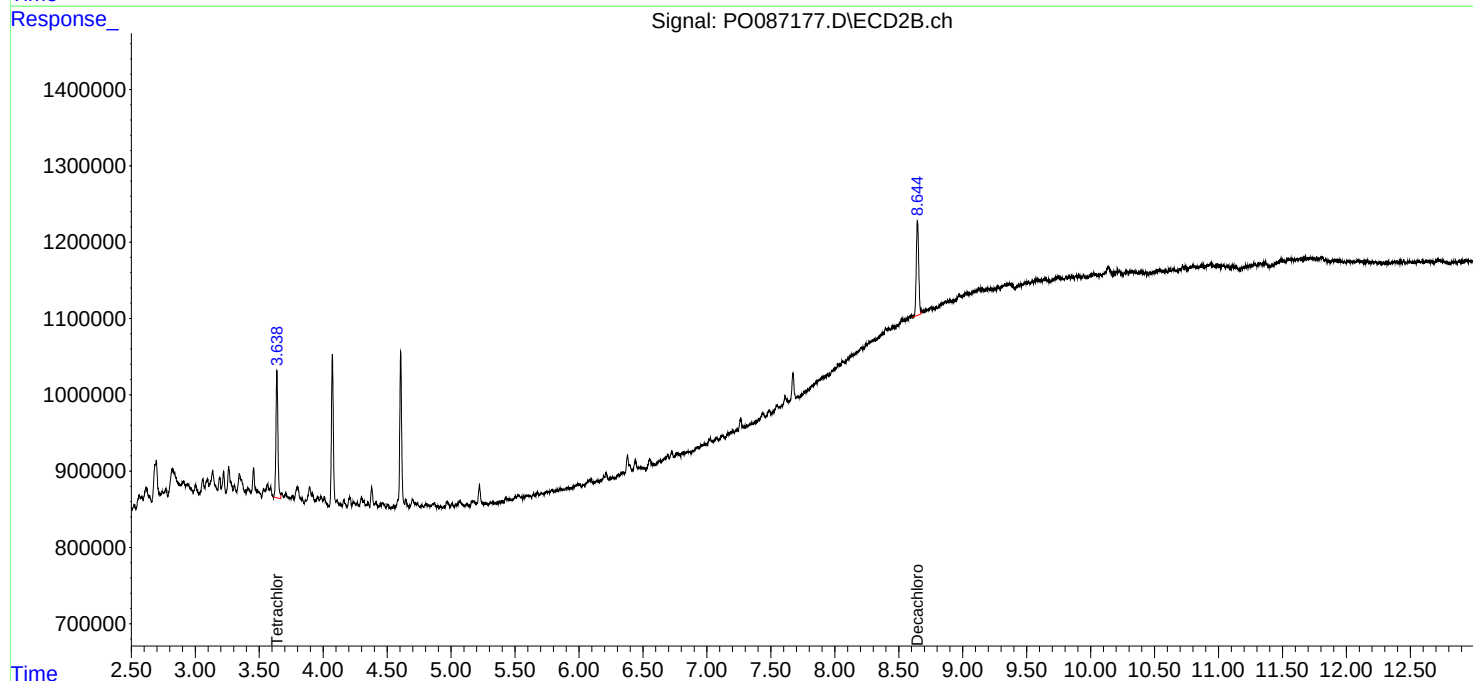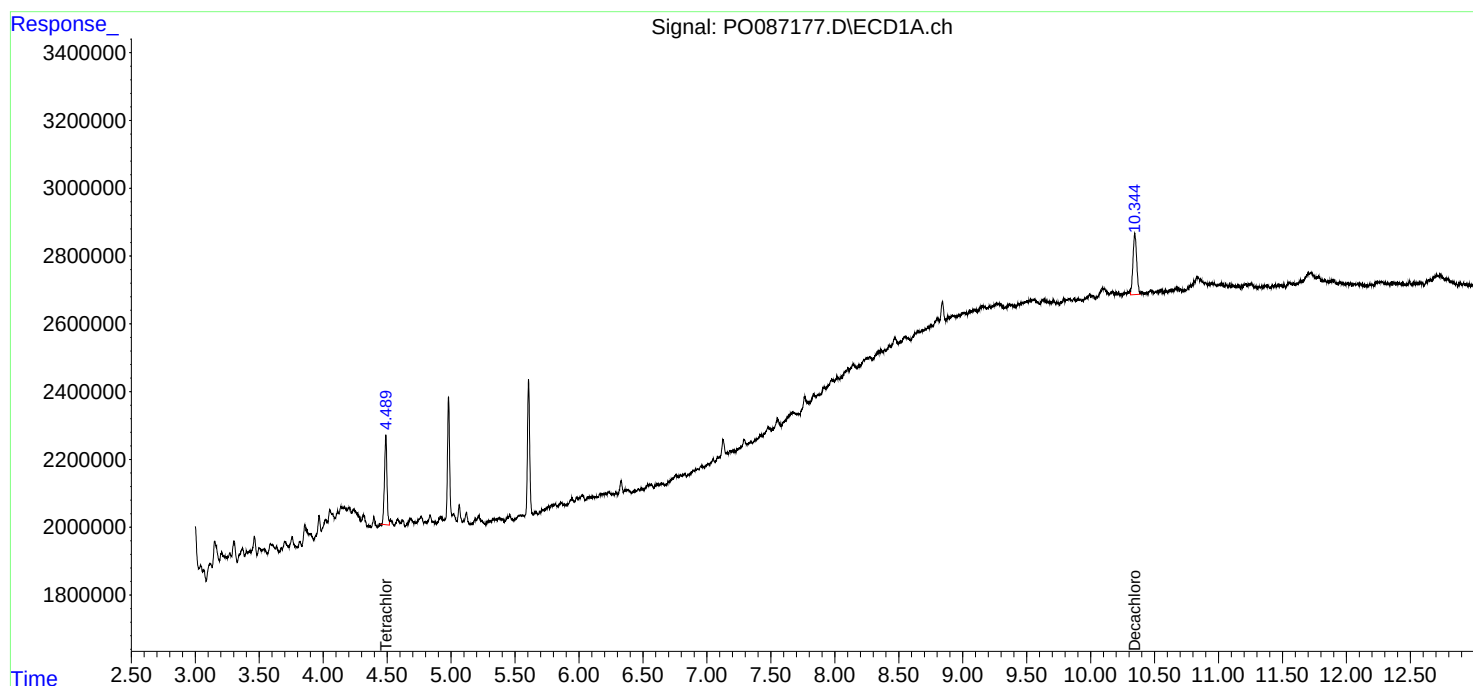


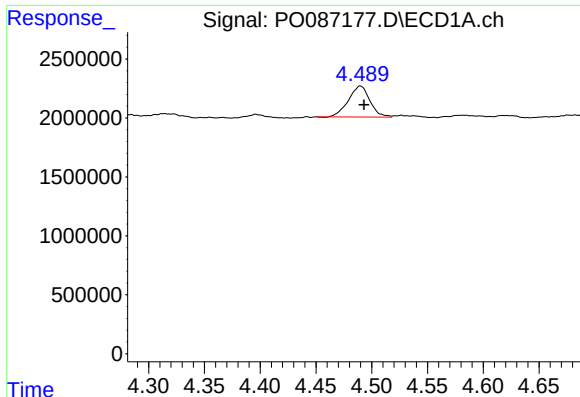

#1 Tetrachloro-m-xylene


R.T.: 4.490 min
Delta R.T.: -0.003 min
Response: 3543411
Conc: 1.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDA375-1-3

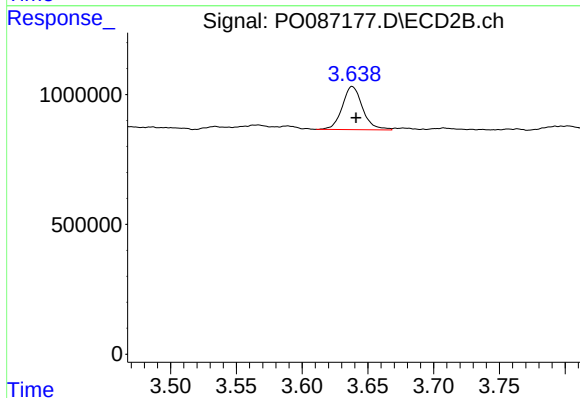


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 1781152
Conc: 1.58 ng/ml

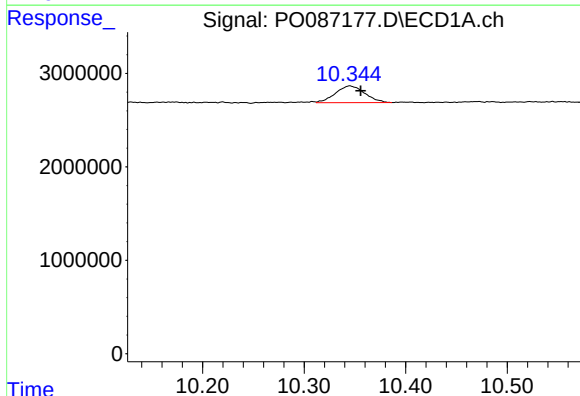

#2 Decachlorobiphenyl

R.T.: 10.345 min
Delta R.T.: -0.011 min
Response: 3636191
Conc: 1.98 ng/ml

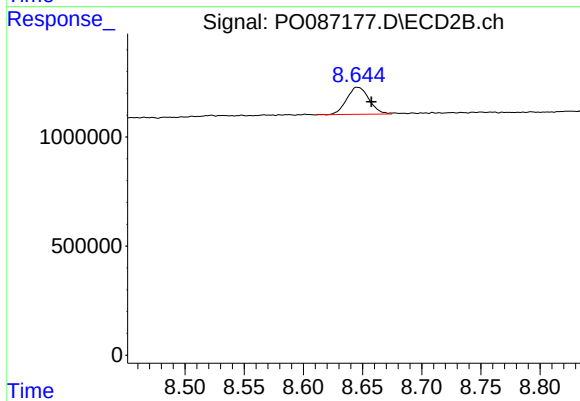

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: -0.012 min
Response: 1628325
Conc: 2.07 ng/ml