

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061522\
 Data File : P0087179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2022 11:26
 Operator : YP/AJ
 Sample : N3334-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-14A-1A-5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/16/2022
 Supervised By :Ankita Jodhani 06/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 11:55:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.642	33822962	19051176	14.473m	16.920
2) SA Decachlor...	10.362	8.661	32791338	15273288	17.818	19.426

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061522\
Data File : PO087179.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2022 11:26
Operator : YP/AJ
Sample : N3334-19
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-14A-1A-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2022
Supervised By :Ankita Jodhani 06/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 11:55:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

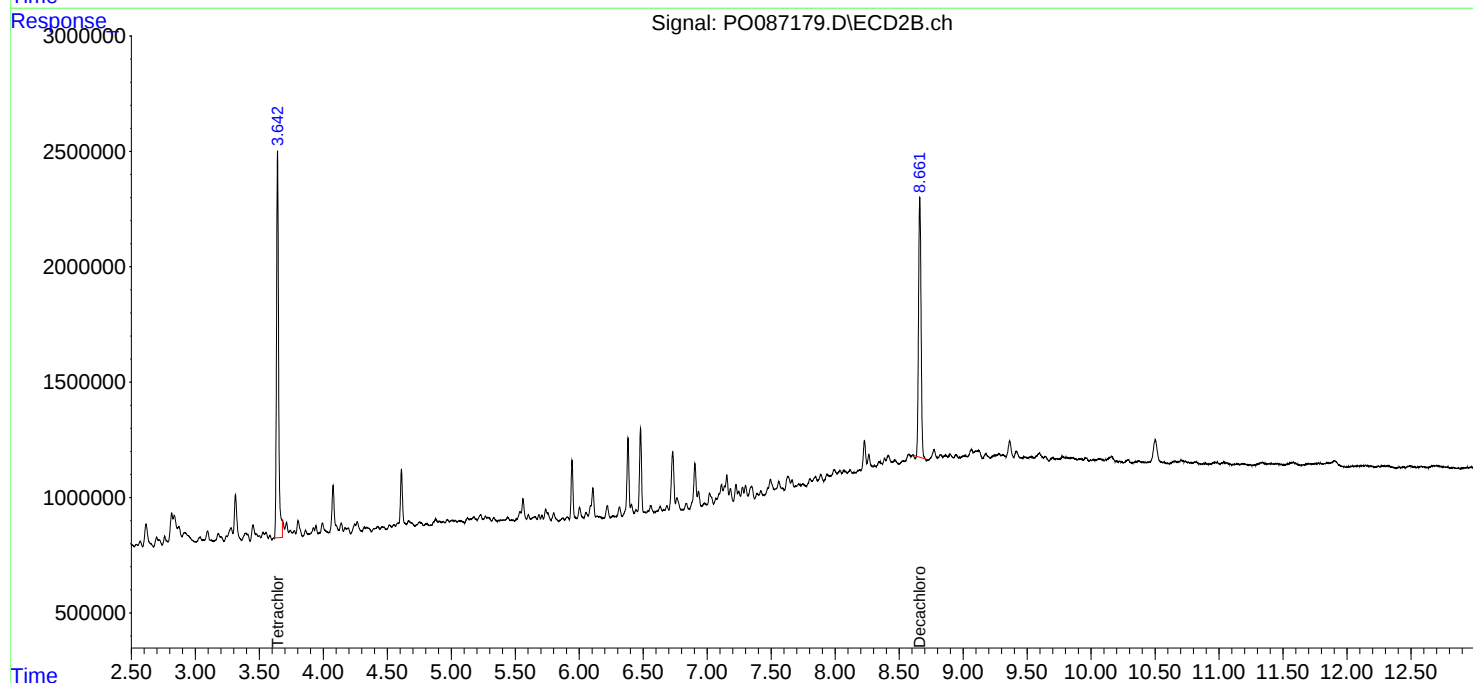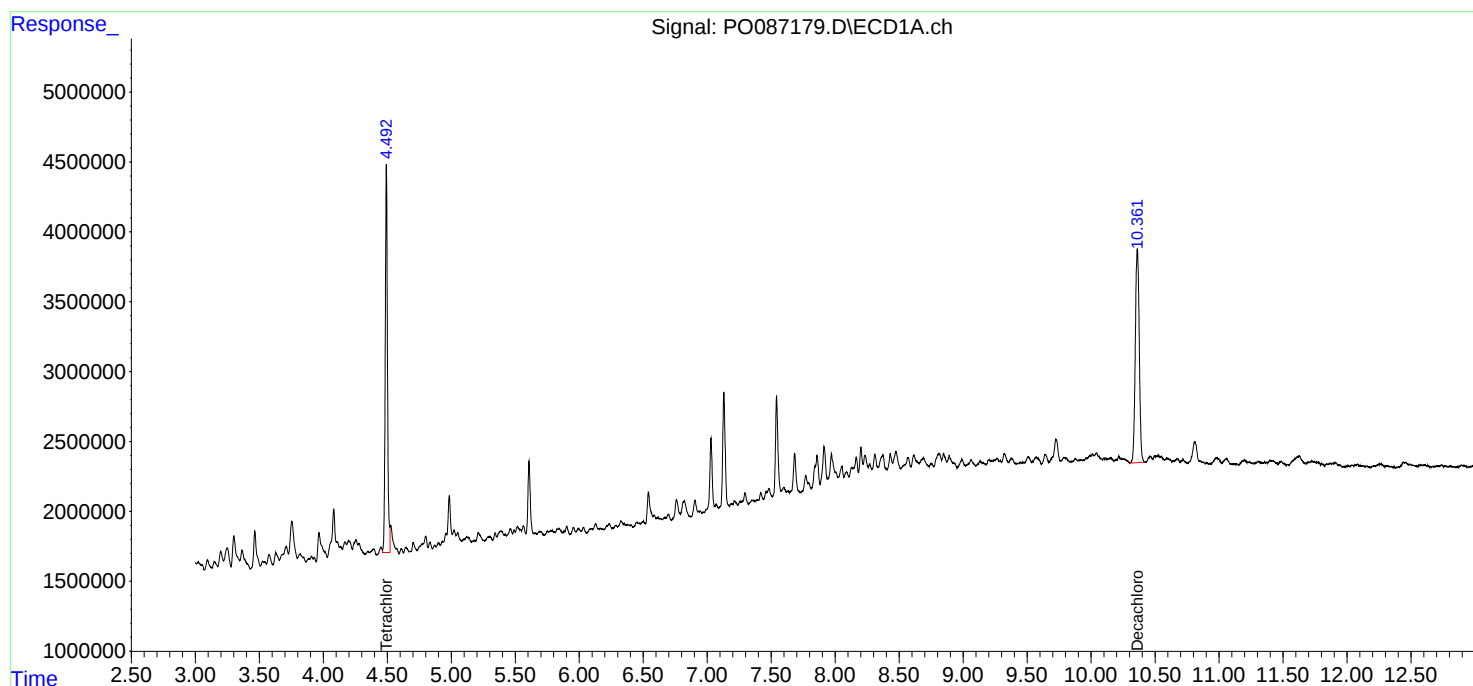

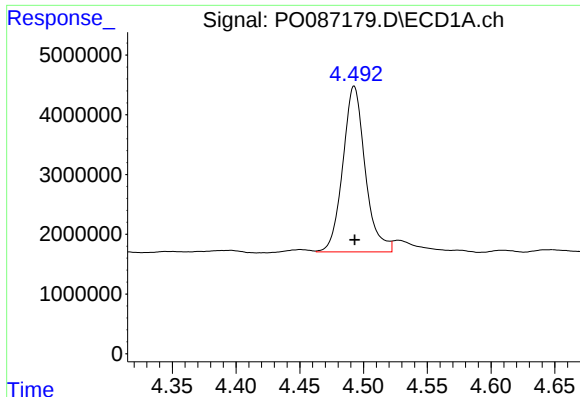


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: 0.000 min
Response: 33822962
Conc: 14.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-14A-1A-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2022
Supervised By :Ankita Jodhani 06/16/2022

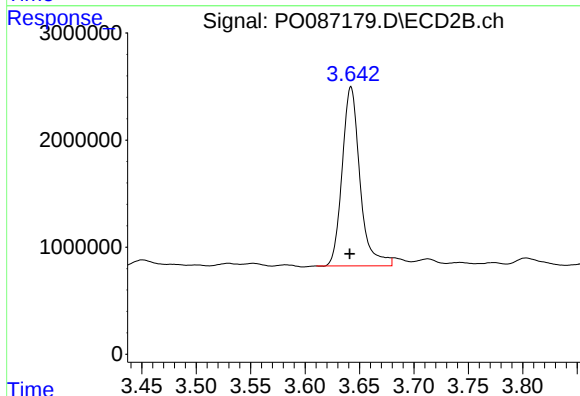


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: 0.001 min
Response: 19051176
Conc: 16.92 ng/ml

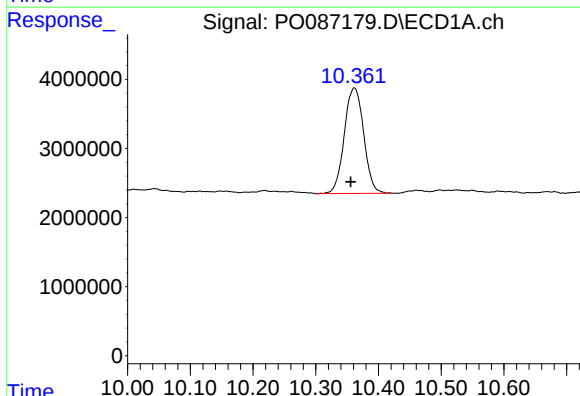

#2 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: 0.006 min
Response: 32791338
Conc: 17.82 ng/ml

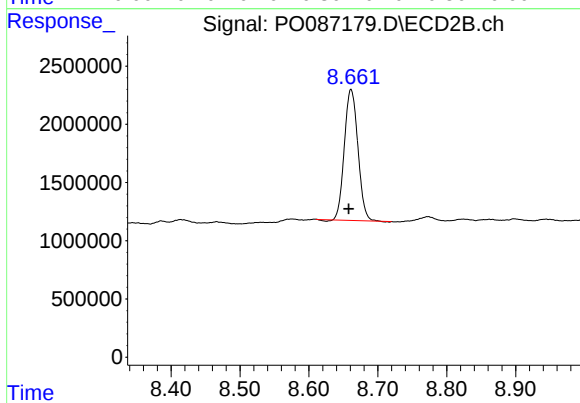

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: 0.004 min
Response: 15273288
Conc: 19.43 ng/ml