

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0061618\
 Data File : P0045845.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jun 2018 17:29
 Operator : SM/UA
 Sample : J3481-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-021-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 01:54:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 15 08:20:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.392	3.623	4667638	2231657	23.790	23.812
2) SA Decachlor...	10.058	8.602	2955262	1161025	14.662m	14.698

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061618\
Data File : P0045845.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2018 17:29
Operator : SM/UA
Sample : J3481-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-021-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 01:54:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

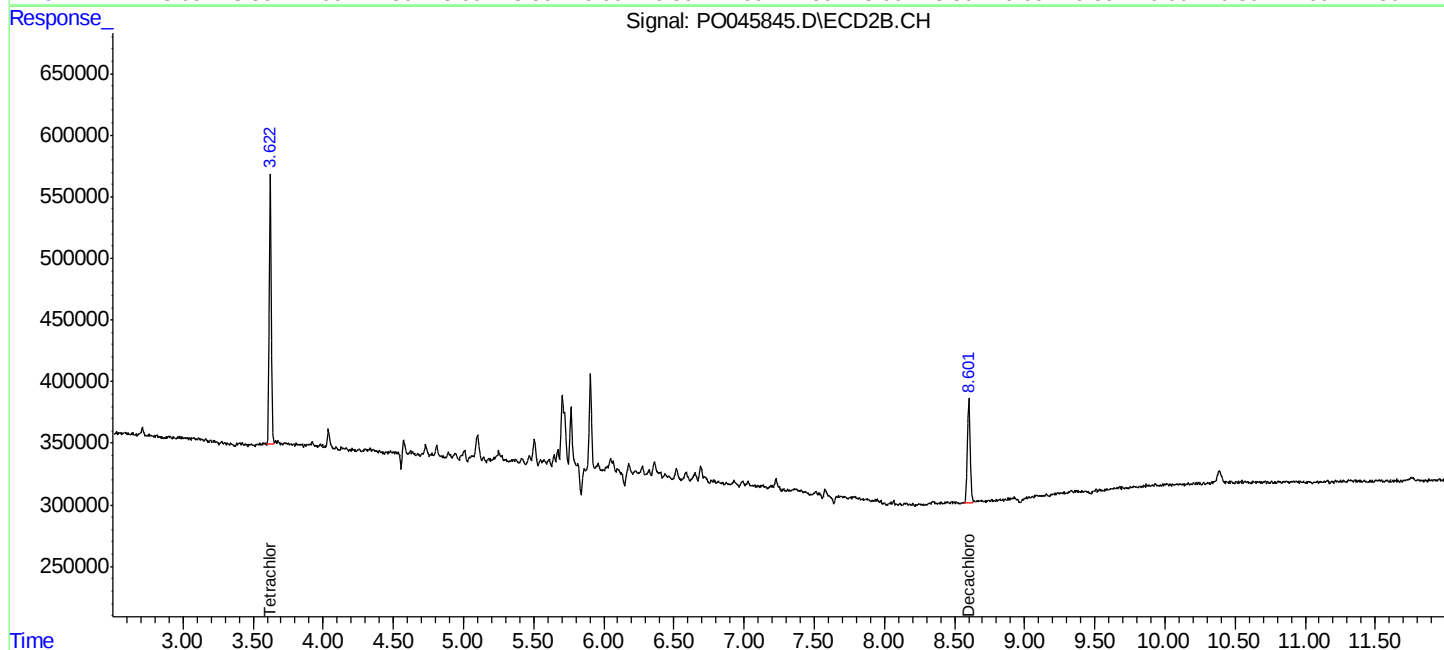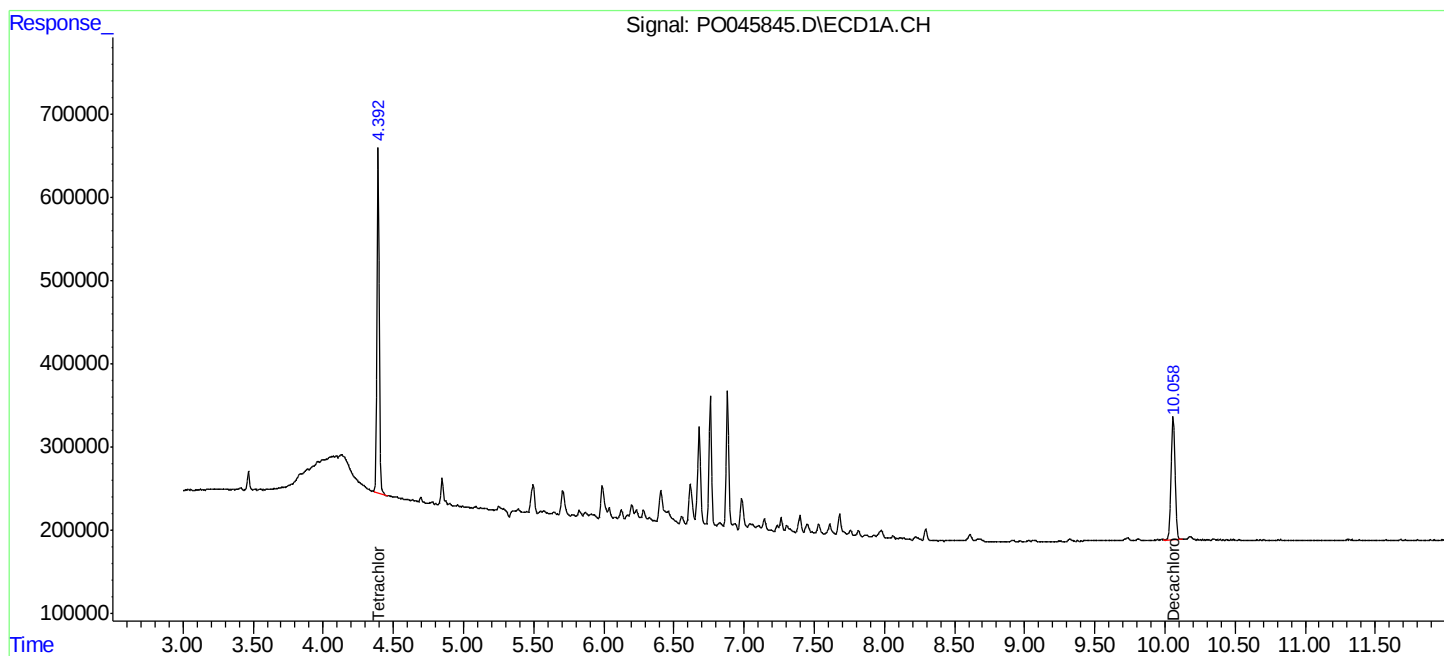


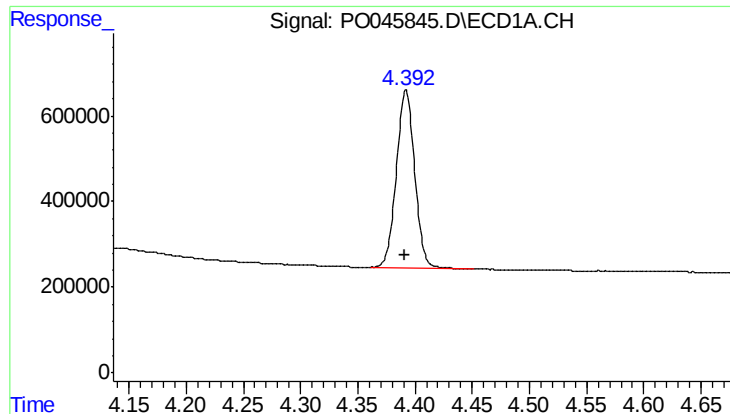

#1 Tetrachloro-m-xylene


R.T.: 4.392 min
Delta R.T.: 0.001 min
Response: 4667638
Conc: 23.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-021-A

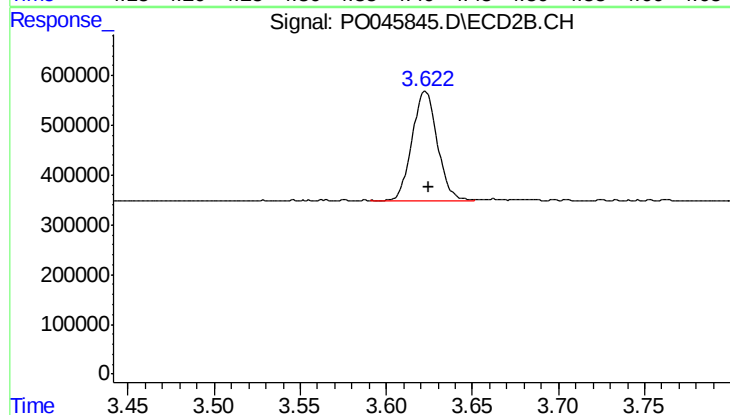


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.002 min
Response: 2231657
Conc: 23.81 ng/ml

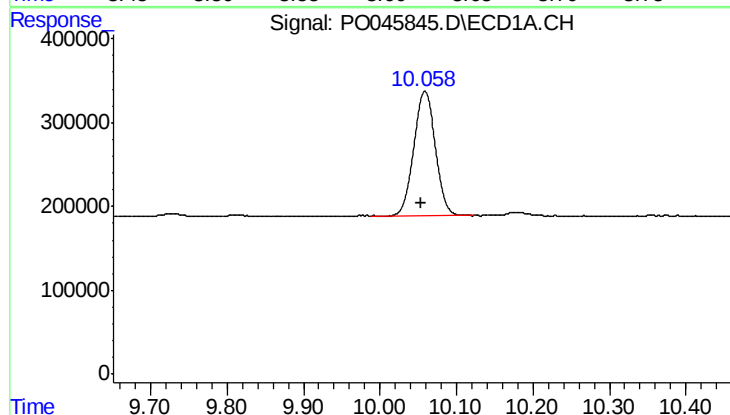

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: 0.003 min
Response: 2955262
Conc: 14.66 ng/ml m

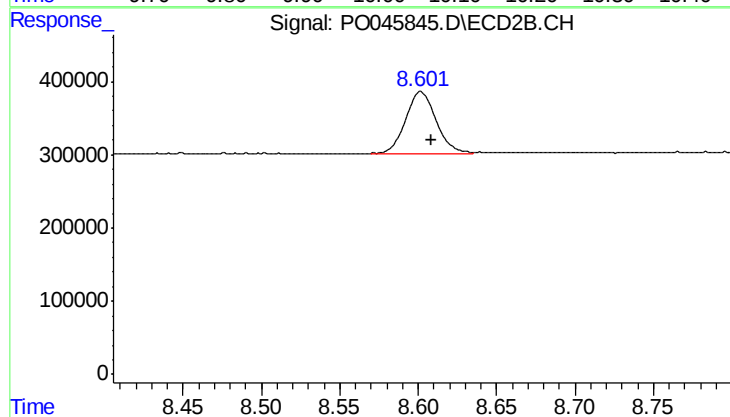

#2 Decachlorobiphenyl

R.T.: 8.602 min
Delta R.T.: -0.007 min
Response: 1161025
Conc: 14.70 ng/ml