

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0061618\
Data File : P0045848.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2018 18:17
Operator : SM/UA
Sample : J3498-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 02:32:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.623	4419781	2385701	22.527m	25.456
2) SA Decachlor...	10.055	8.601	2815594	1156217	13.969	14.637

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061618\
Data File : P0045848.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2018 18:17
Operator : SM/UA
Sample : J3498-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 02:32:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

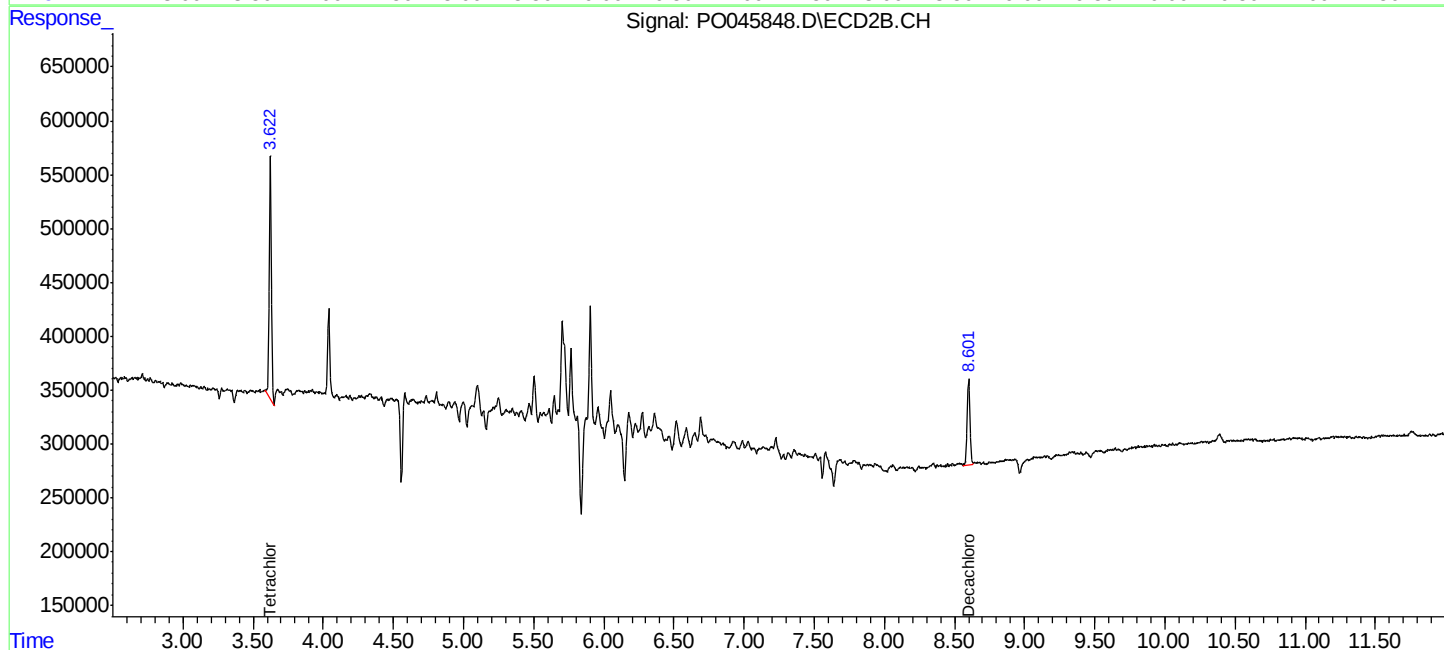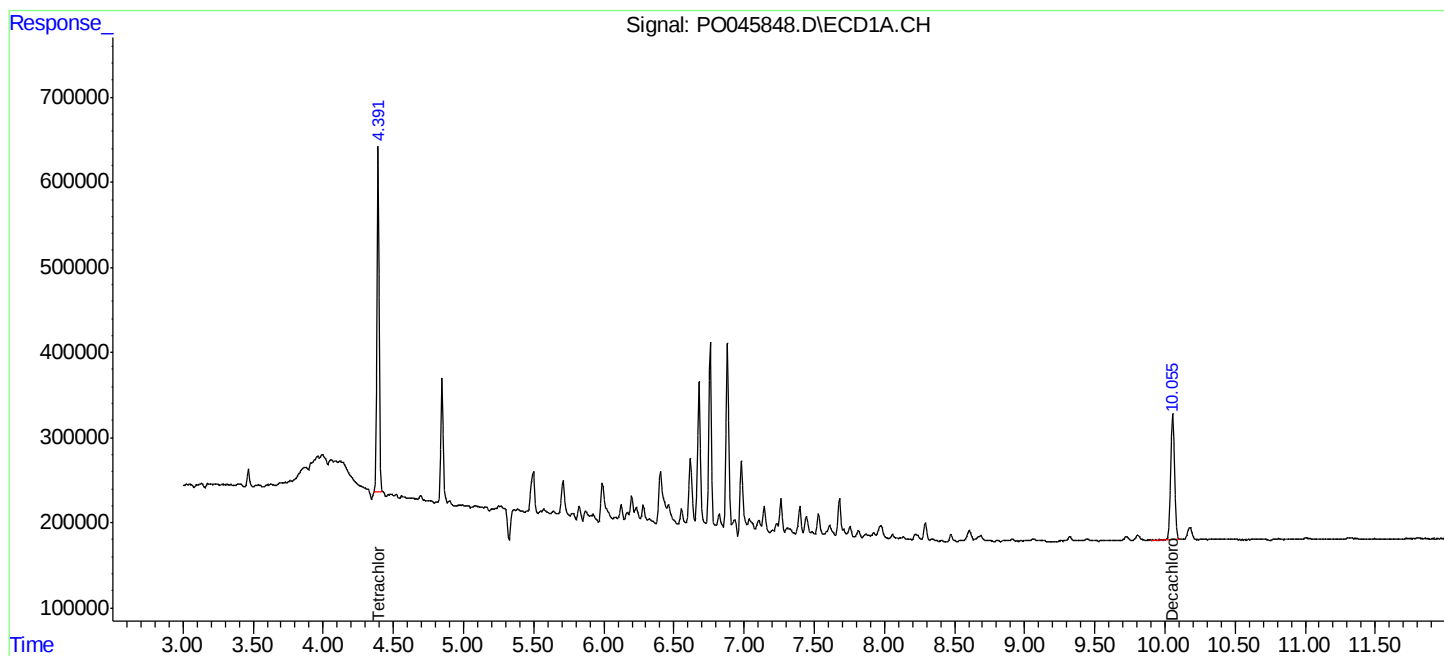


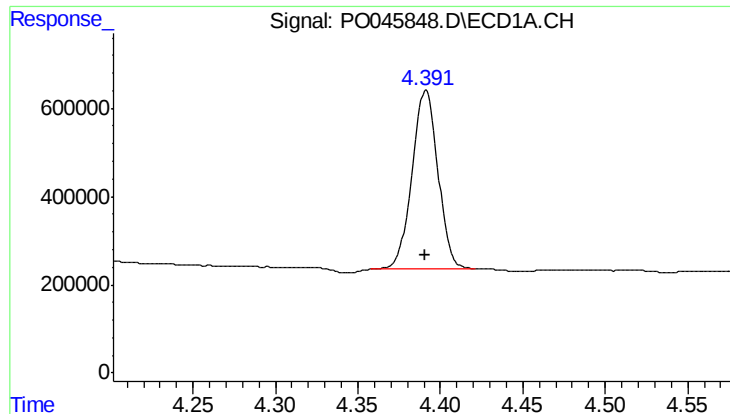

#1 Tetrachloro-m-xylene


R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 4419781
Conc: 22.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-D-S

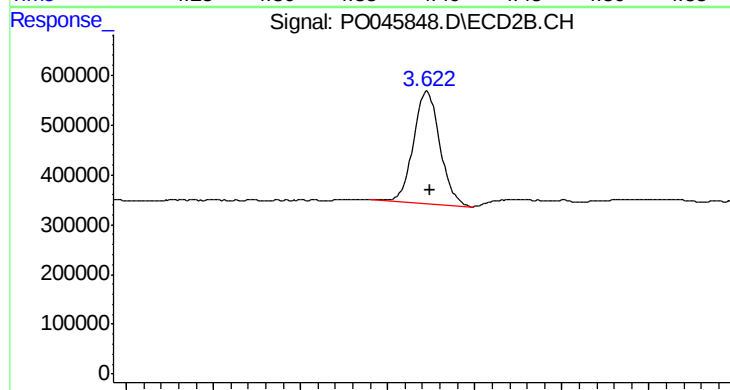


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.002 min
Response: 2385701
Conc: 25.46 ng/ml

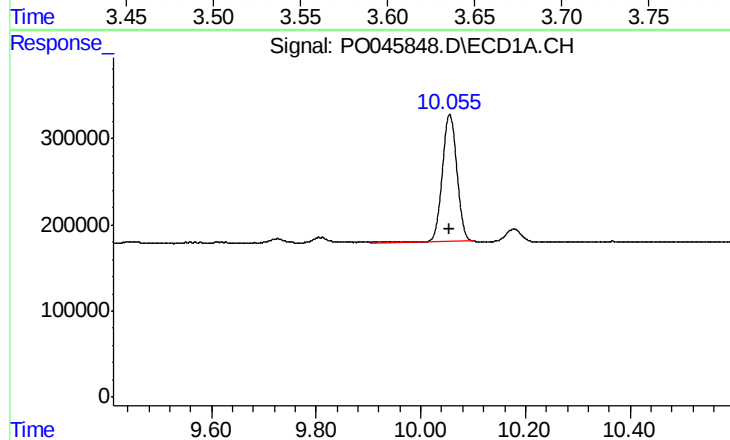

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.000 min
Response: 2815594
Conc: 13.97 ng/ml

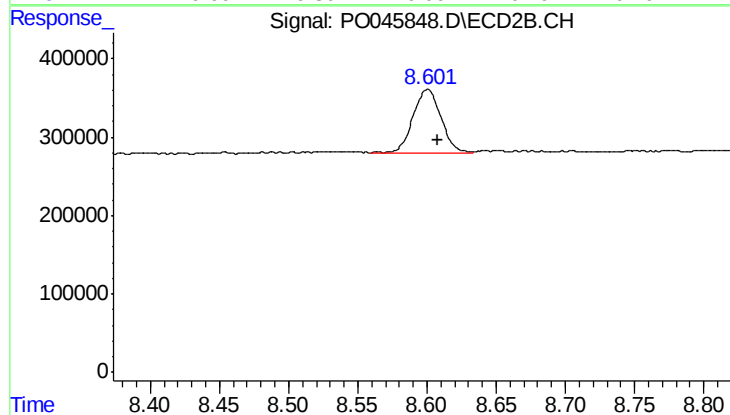

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: -0.008 min
Response: 1156217
Conc: 14.64 ng/ml