

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061620\
 Data File : P0068997.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jun 2020 18:19
 Operator : DD\AJ
 Sample : L2815-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-061520

Manual Integrations
 APPROVED

Sohil
 6/17/2020 8:22:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 18:51:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 13 01:32:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.568	875581	1086356	32.091m	30.578m
2) SA Decachlor...	10.073	8.774	987819	1032443	21.998	20.176

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061620\
Data File : PO068997.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jun 2020 18:19
Operator : DD\AJ
Sample : L2815-06
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-03-061520


Manual Integrations
APPROVED

Sohil
6/17/2020 8:22:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 18:51:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061220.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 13 01:32:21 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

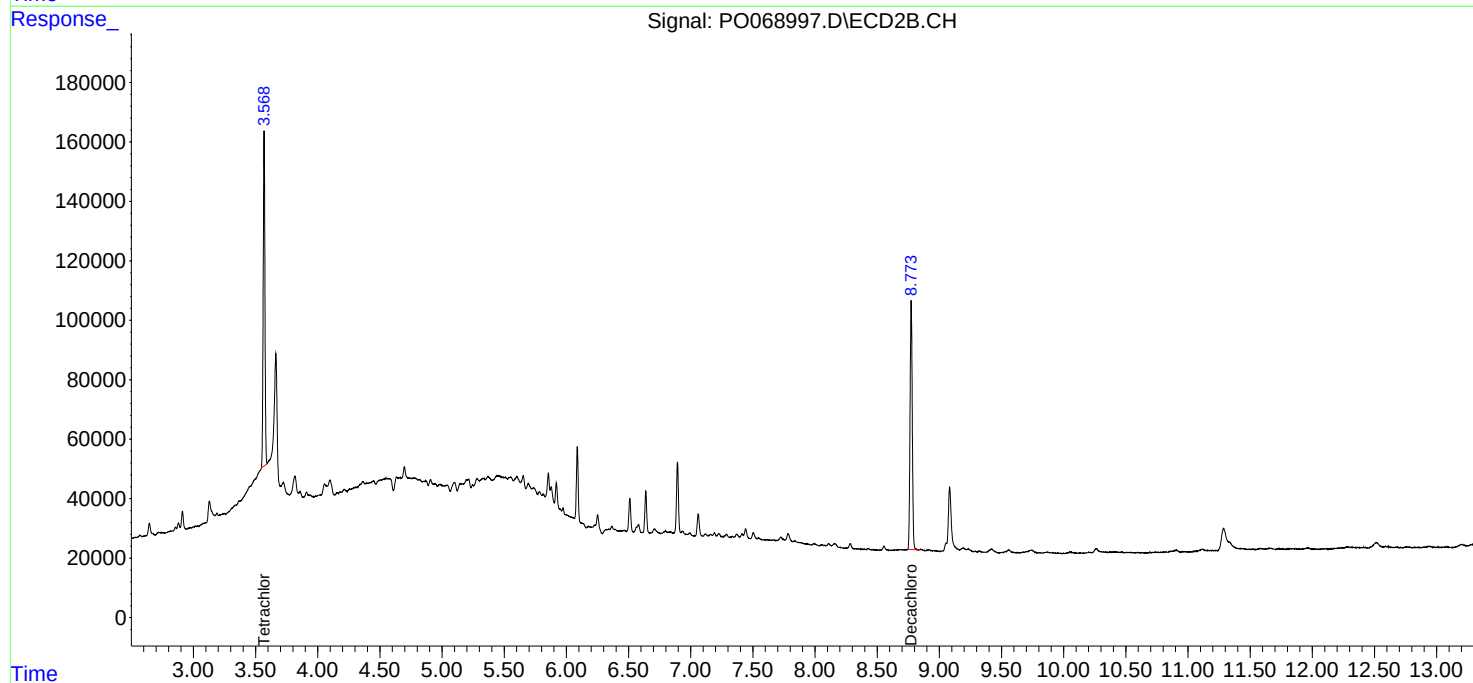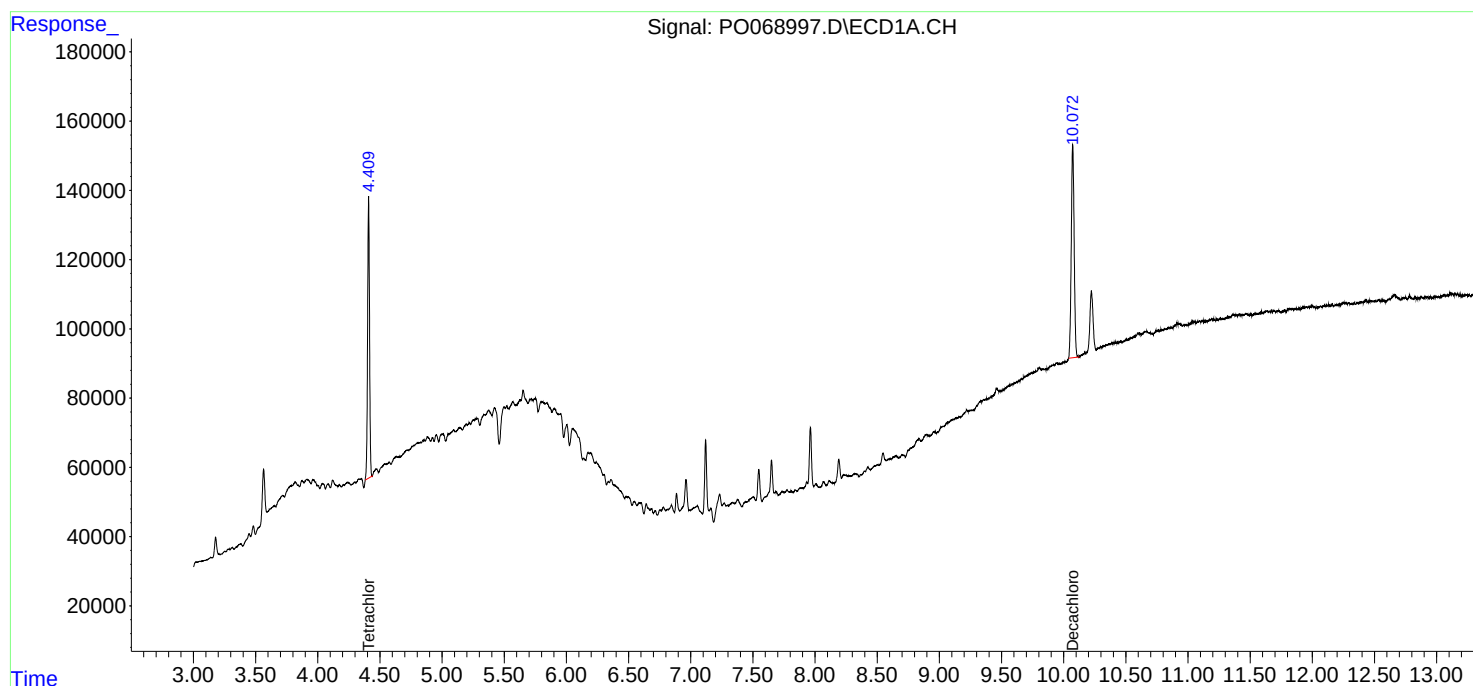

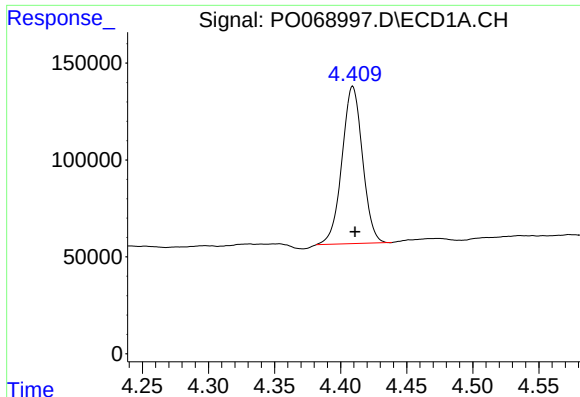


#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: -0.002 min
Response: 875581
Conc: 32.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-03-061520


Manual Integrations
APPROVED

Sohil
6/17/2020 8:22:24 AM

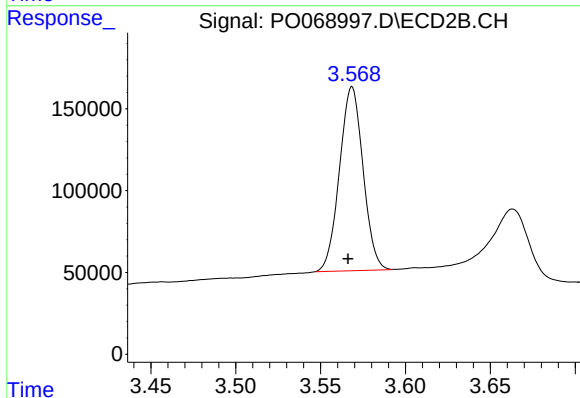


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: 0.002 min
Response: 1086356
Conc: 30.58 ng/ml m

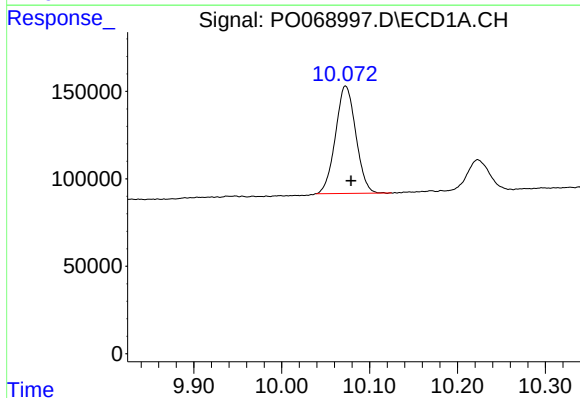

#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: -0.006 min
Response: 987819
Conc: 22.00 ng/ml

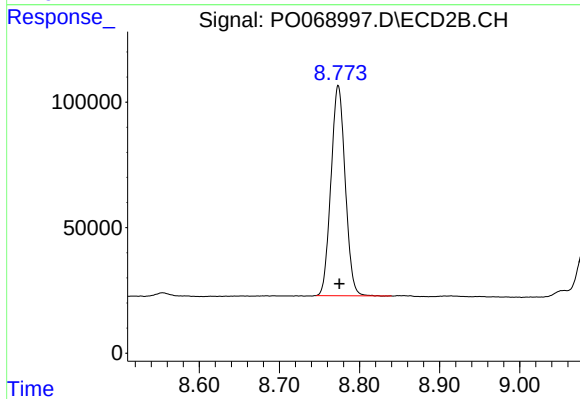

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.001 min
Response: 1032443
Conc: 20.18 ng/ml