

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061621\
 Data File : P0078831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jun 2021 15:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 15:54:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.330	3.606	1599930	641813	18.897	18.540
2)	SA Decachlor...	9.939	8.788	1221804	626844	20.820	20.161
Target Compounds							
9)	L2 AR-1221-2	4.672	0.000	18924	0	28.522	N.D. #
15)	L3 AR-1232-5	5.926	0.000	26384	0	50.490	N.D. #
22)	L5 AR-1248-2	5.926	0.000	26384	0	12.644	N.D. #
24)	L5 AR-1248-4	6.549	0.000	1681	0	0.642	N.D. #
26)	L6 AR-1254-1	6.543f	0.000	12244	0	4.467	N.D. #
28)	L6 AR-1254-3	7.140f	0.000	86240	0	19.808	N.D. #
32)	L7 AR-1260-2	0.000	6.562f	0	39858	N.D.	19.778 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061621\
Data File : P0078831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jun 2021 15:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 15:54:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

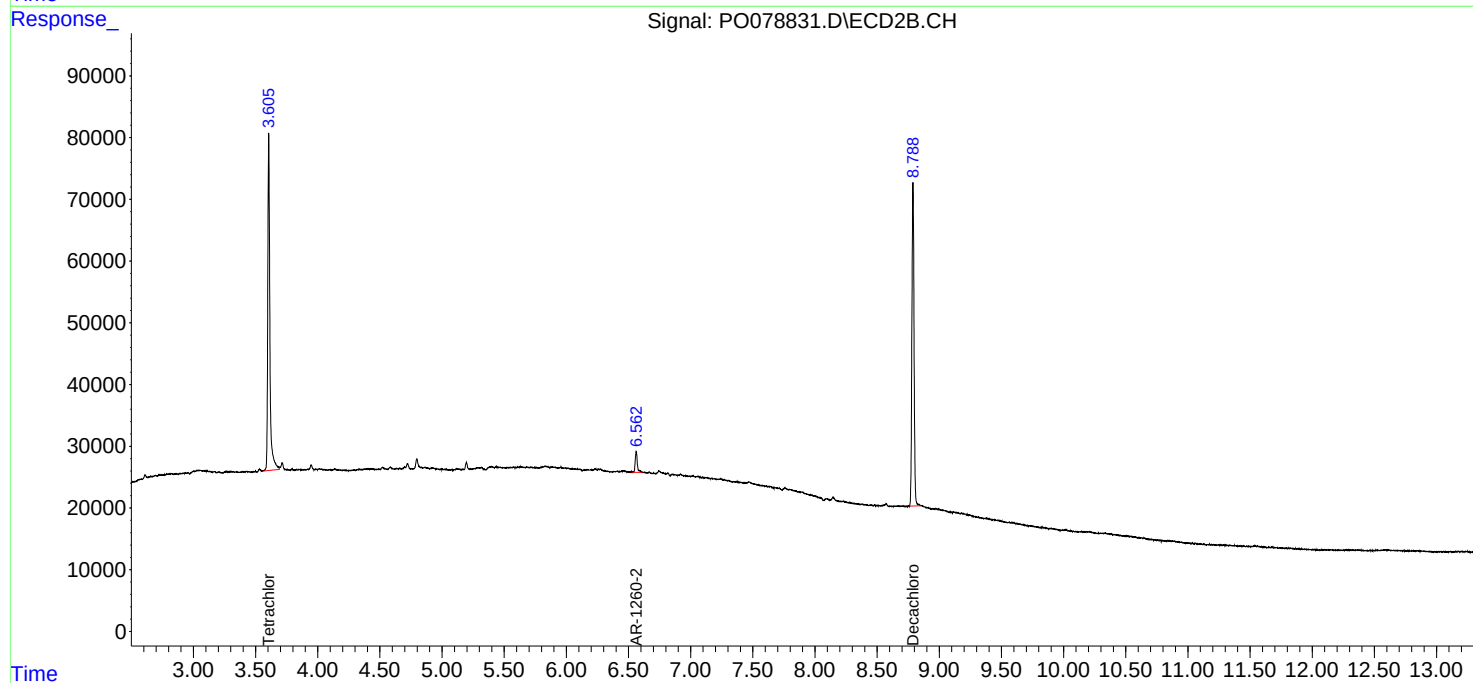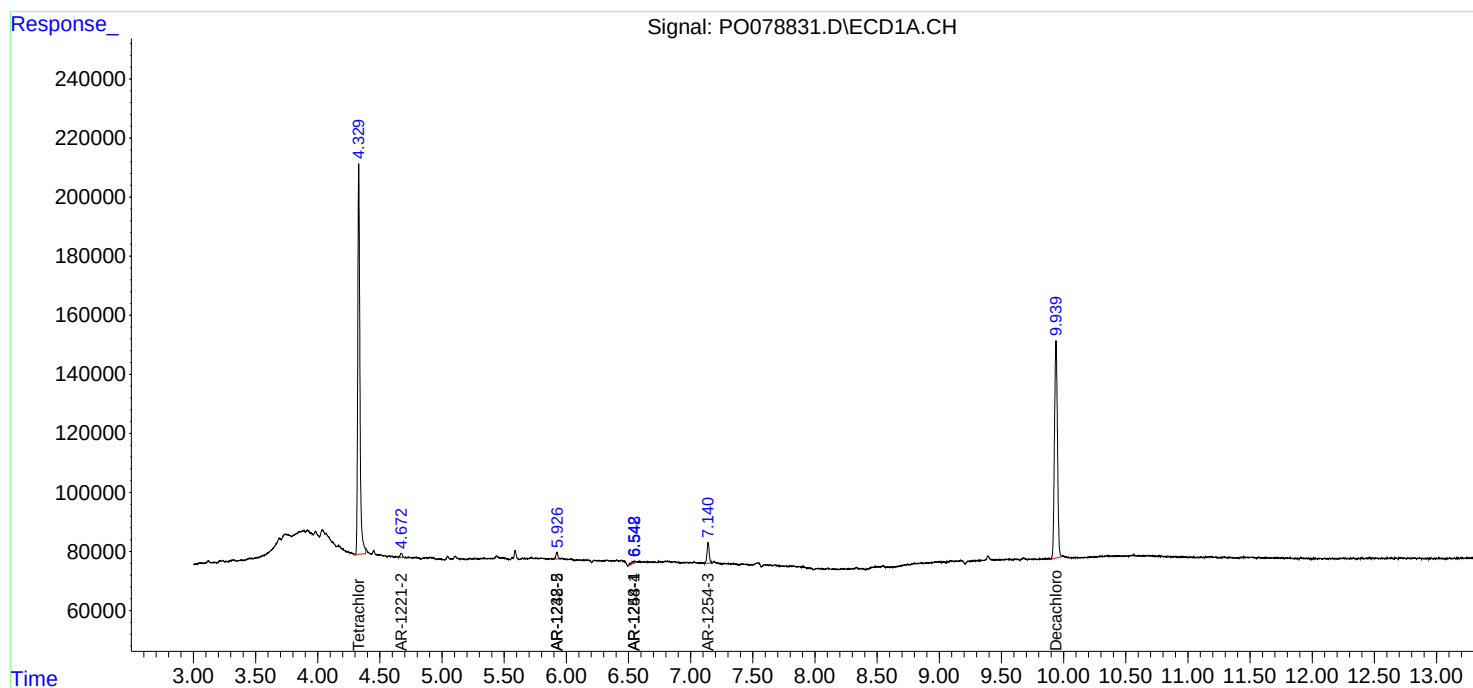


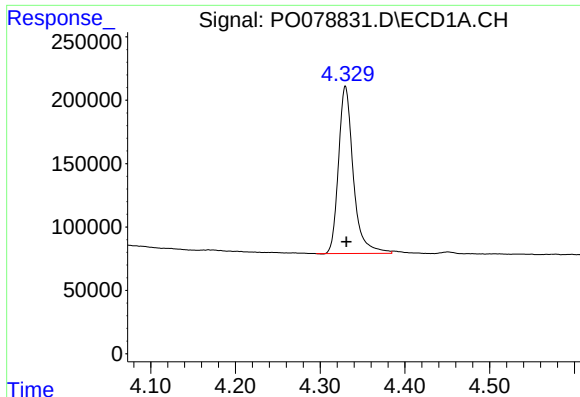

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: -0.001 min
Response: 1599930
Conc: 18.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

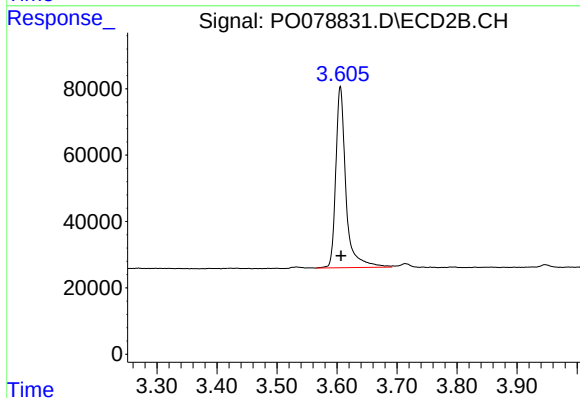


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: -0.001 min
Response: 641813
Conc: 18.54 ng/ml

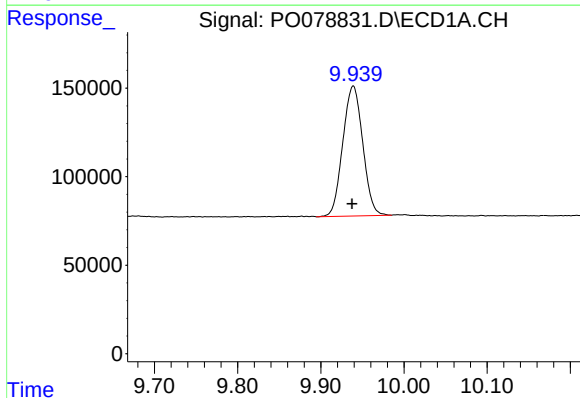


#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: 0.002 min
Response: 1221804
Conc: 20.82 ng/ml

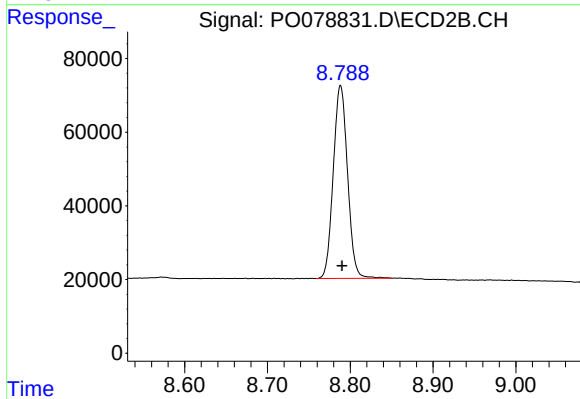

#2 Decachlorobiphenyl


R.T.: 8.788 min
Delta R.T.: -0.002 min
Response: 626844
Conc: 20.16 ng/ml

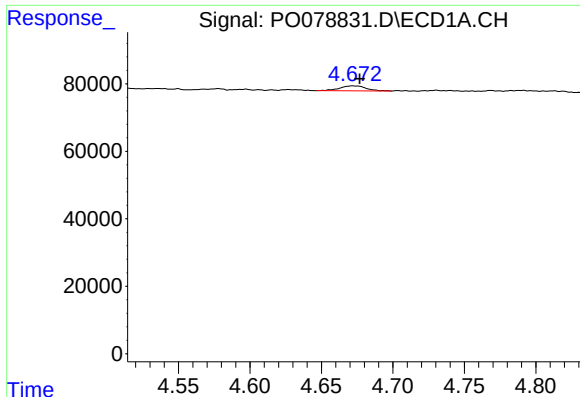

#9 AR-1221-2


R.T.: 4.672 min
Delta R.T.: -0.005 min
Response: 18924
Conc: 28.52 ng/ml

Instrument :
ECD_O
ClientSampleId :

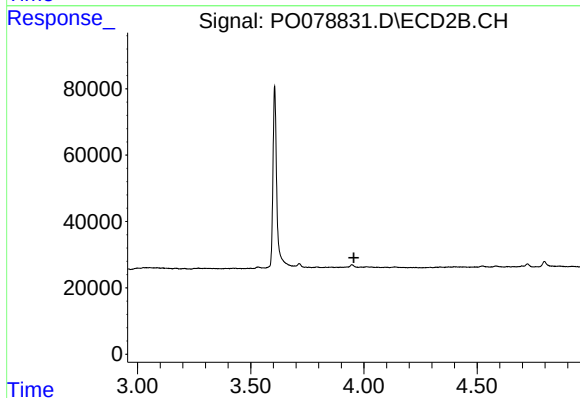


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.956 min
Response: 0
Conc: N.D.

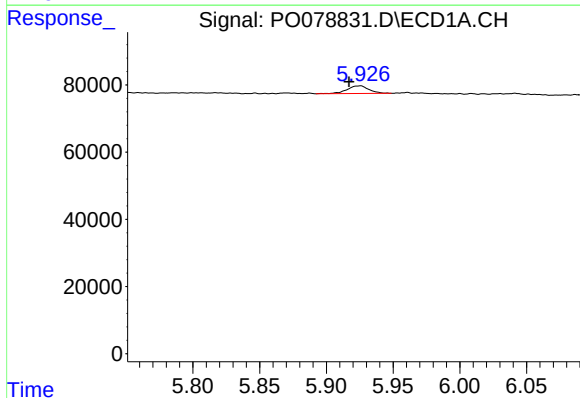


#15 AR-1232-5

R.T.: 5.926 min
Delta R.T.: 0.009 min
Response: 26384
Conc: 50.49 ng/ml

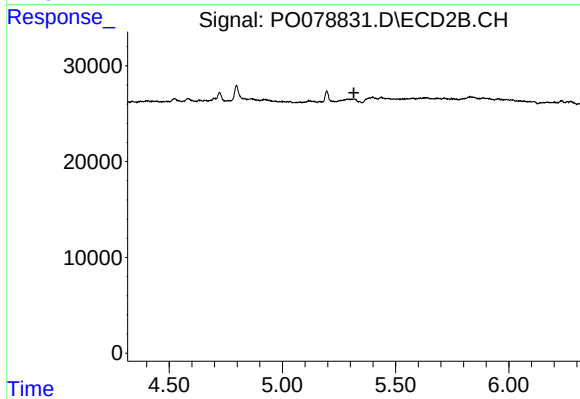

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.316 min
Response: 0
Conc: N.D.

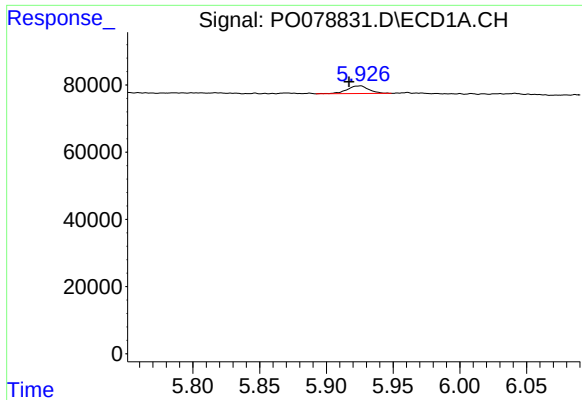

#22 AR-1248-2


R.T.: 5.926 min
Delta R.T.: 0.009 min
Response: 26384
Conc: 12.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

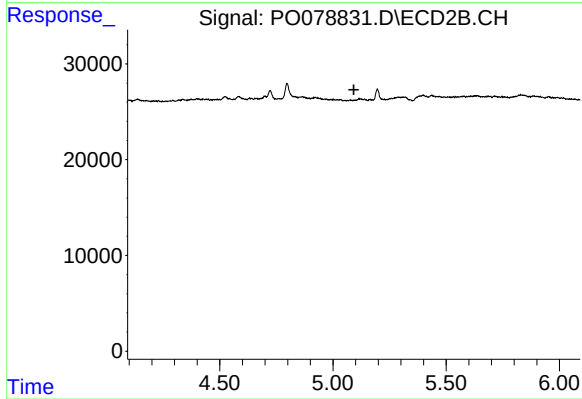


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

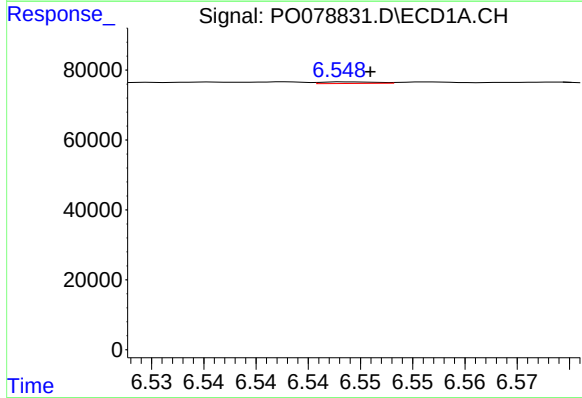


#24 AR-1248-4

R.T.: 6.549 min
Delta R.T.: -0.002 min
Response: 1681
Conc: 0.64 ng/ml

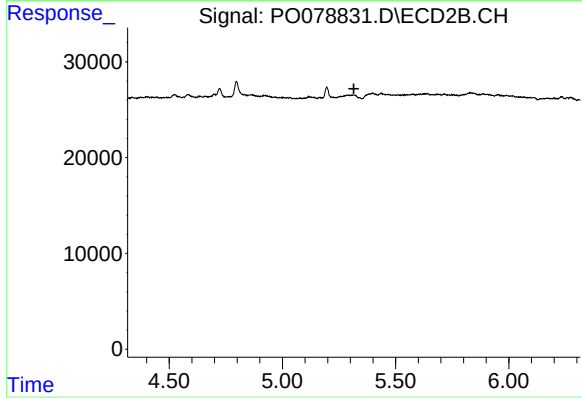

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.316 min
Response: 0
Conc: N.D.

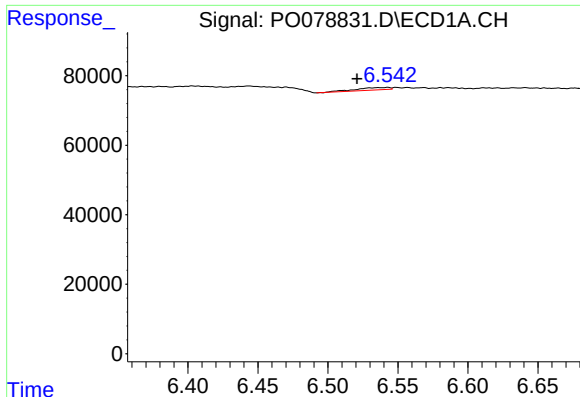

#26 AR-1254-1


R.T.: 6.543 min
Delta R.T.: 0.022 min
Response: 12244
Conc: 4.47 ng/ml

Instrument :
ECD_O
ClientSampleId :

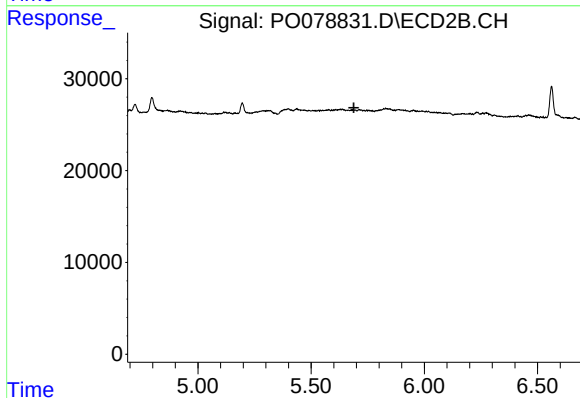


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.689 min
Response: 0
Conc: N.D.

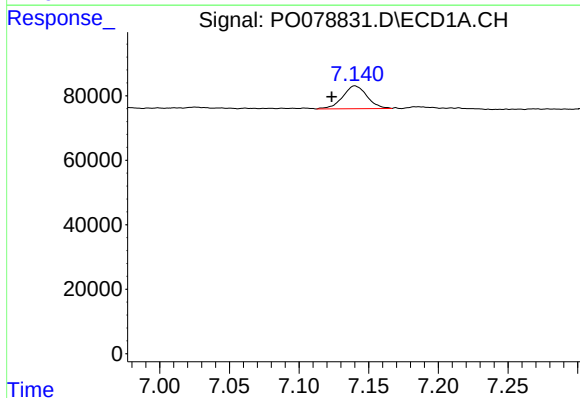


#28 AR-1254-3

R.T.: 7.140 min
Delta R.T.: 0.017 min
Response: 86240
Conc: 19.81 ng/ml

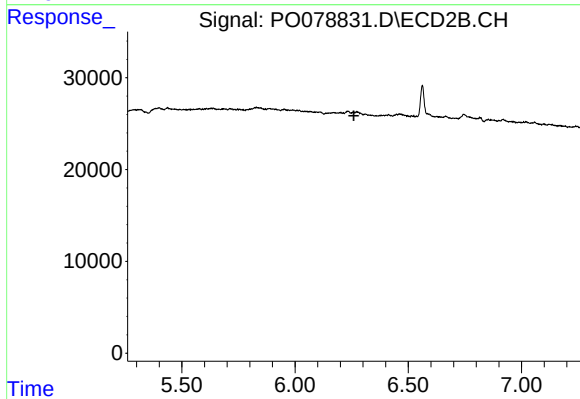

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.260 min
Response: 0
Conc: N.D.

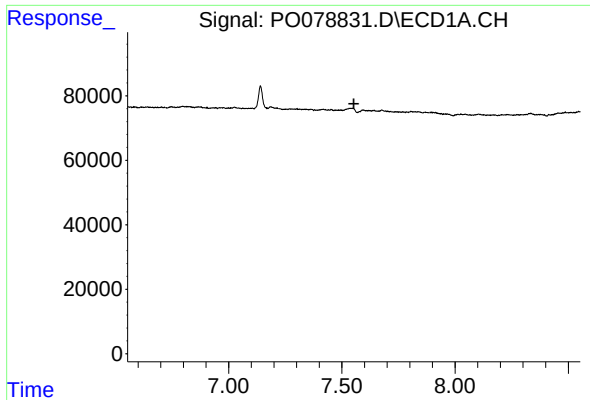

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.553 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

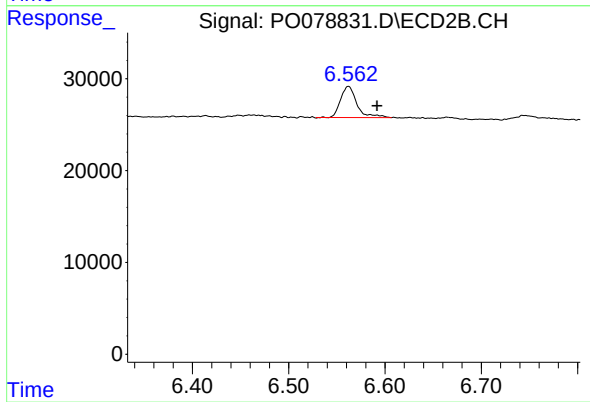

#32 AR-1260-2

R.T.: 6.562 min
Delta R.T.: -0.030 min
Response: 39858
Conc: 19.78 ng/ml