

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061721\
 Data File : P0078846.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jun 2021 14:03
 Operator : DD\AJ
 Sample : M2707-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-216

Manual Integrations
 APPROVED

Ankita
 6/18/2021 12:12:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 15:47:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.606	1951459	620673	23.049	17.929
2) SA Decachlor...	9.939	8.788	1201265	628203	20.470m	20.205m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061721\
Data File : P0078846.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jun 2021 14:03
Operator : DD\AJ
Sample : M2707-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-216


Manual Integrations
APPROVED

Ankita
6/18/2021 12:12:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 15:47:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

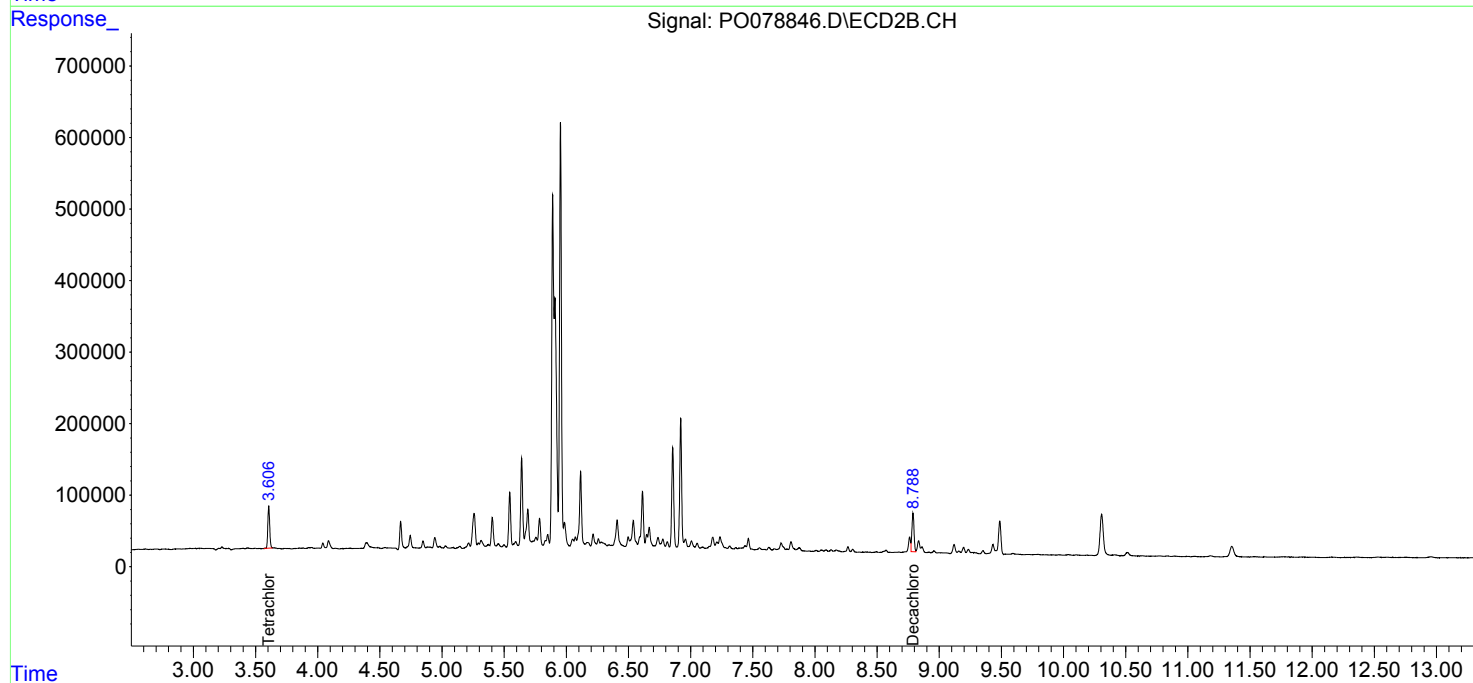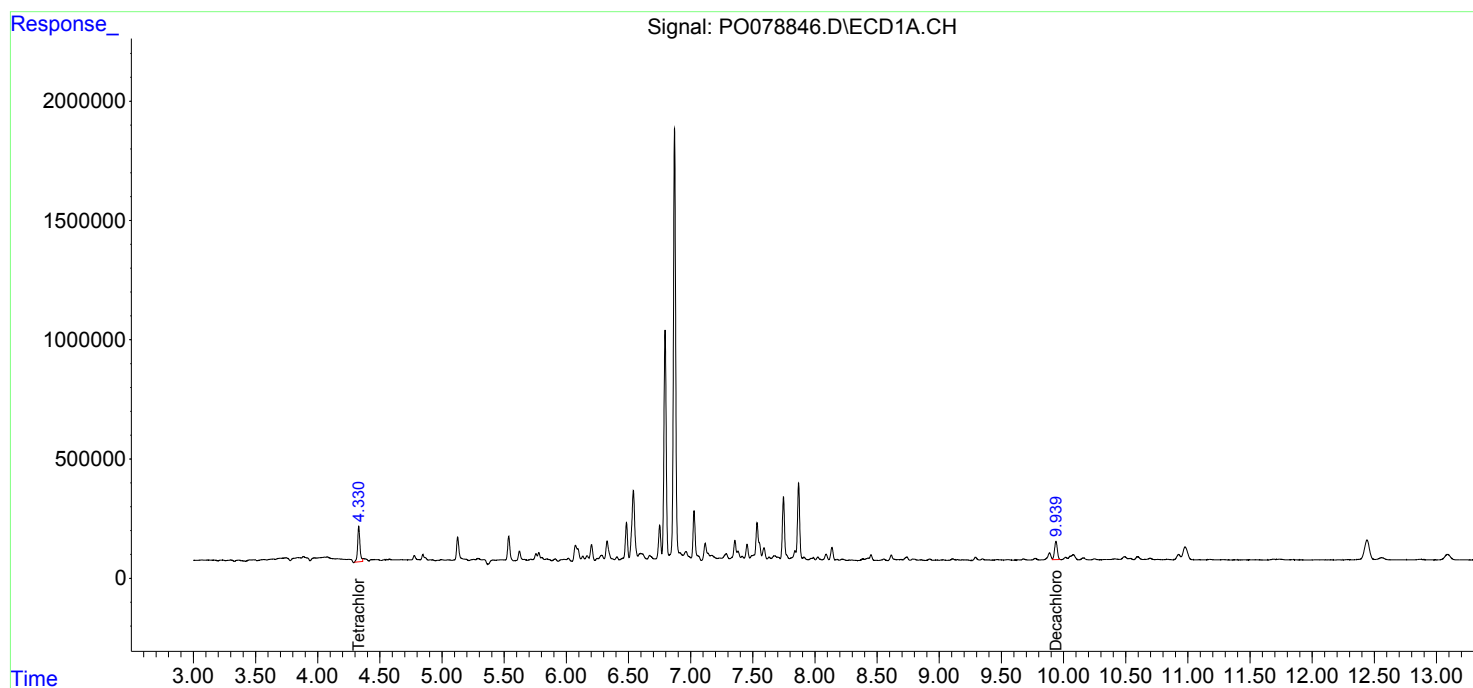

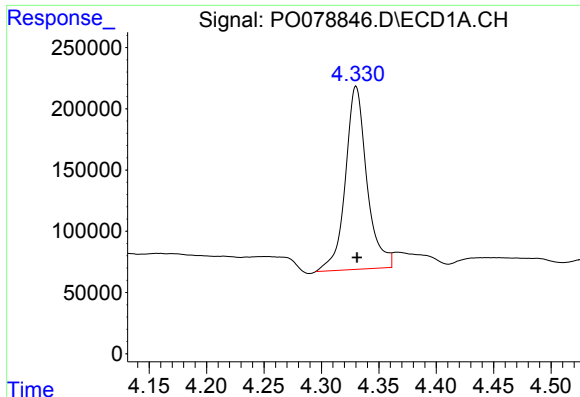


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 1951459
Conc: 23.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-216


Manual Integrations
APPROVED

Ankita
6/18/2021 12:12:08 PM

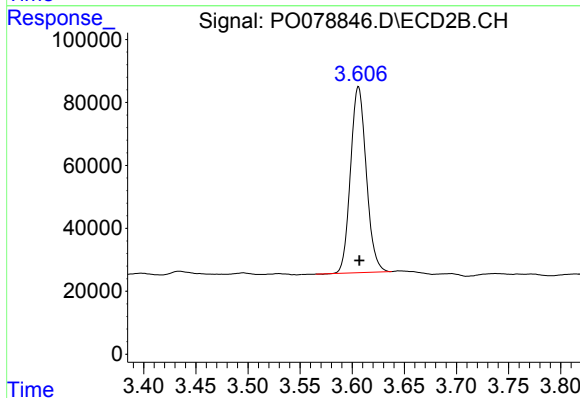


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 620673
Conc: 17.93 ng/ml

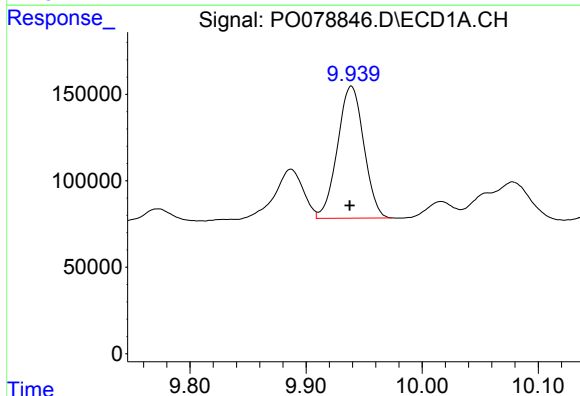

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: 0.000 min
Response: 1201265
Conc: 20.47 ng/ml m

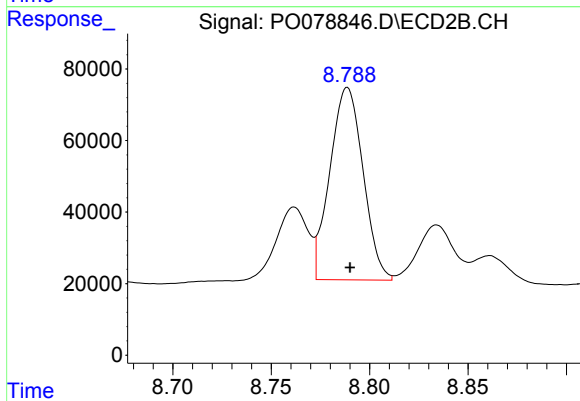

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: -0.002 min
Response: 628203
Conc: 20.20 ng/ml m