

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061721\
 Data File : P0078858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jun 2021 17:30
 Operator : DD\AJ
 Sample : M2715-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33258

Manual Integrations
 APPROVED

Ankita
 6/18/2021 12:14:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:29:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.605	1477109	710376	17.446m	20.520
2) SA Decachlor...	9.936	8.787	1497471	729549	25.517	23.464

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061721\
Data File : P0078858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jun 2021 17:30
Operator : DD\AJ
Sample : M2715-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
33258


Manual Integrations
APPROVED

Ankita
6/18/2021 12:14:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:29:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

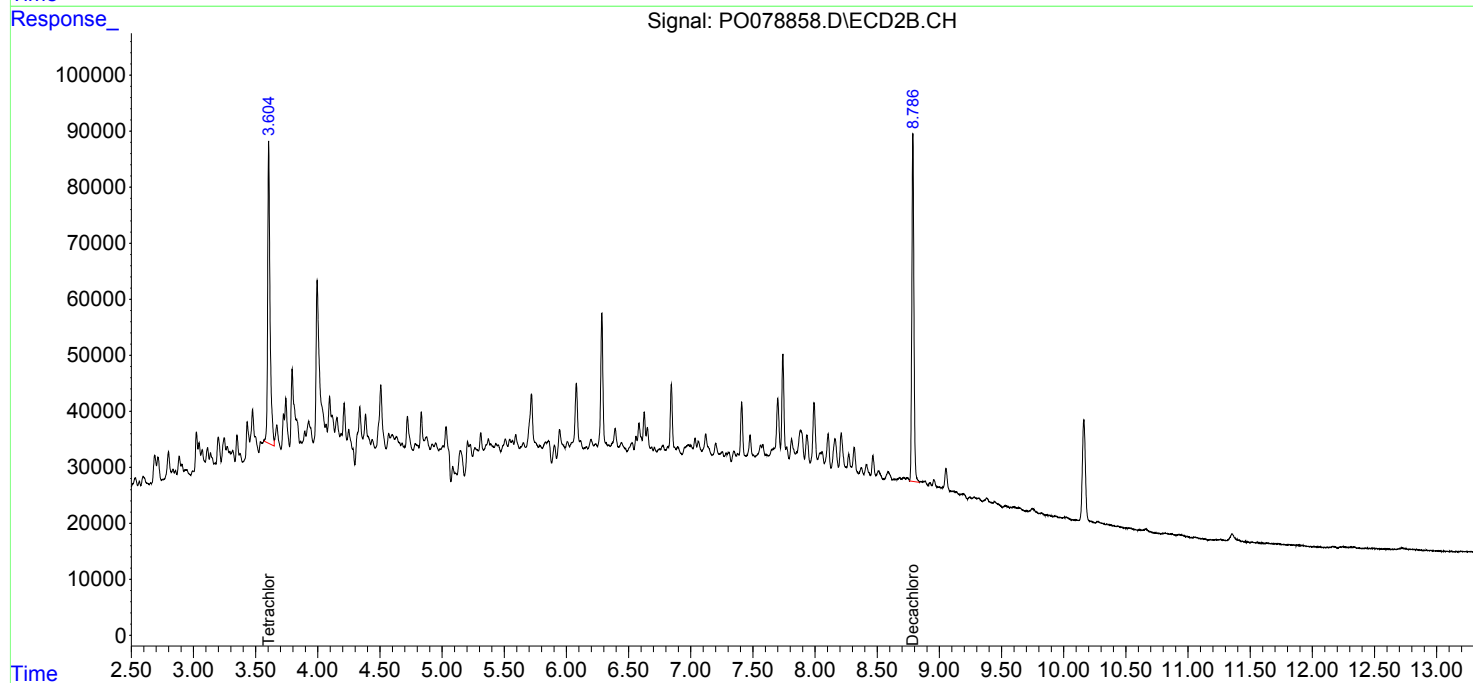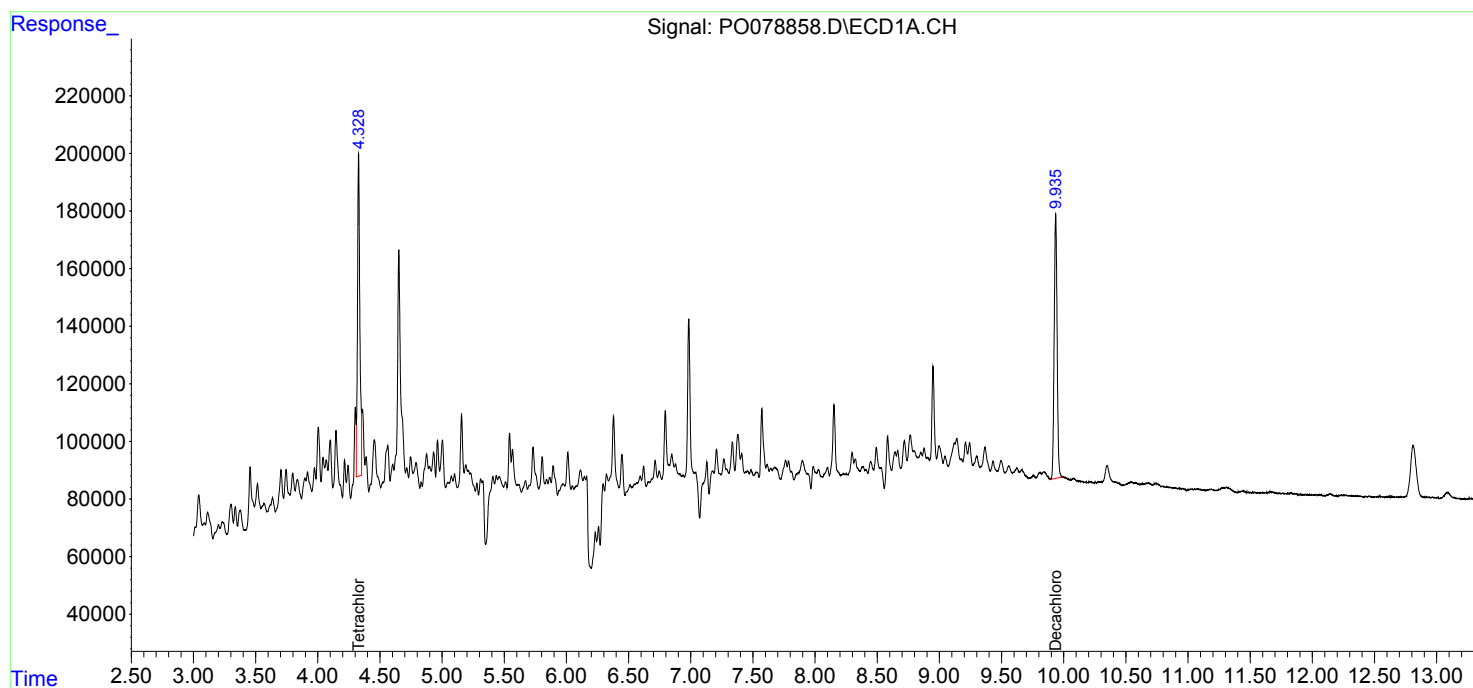

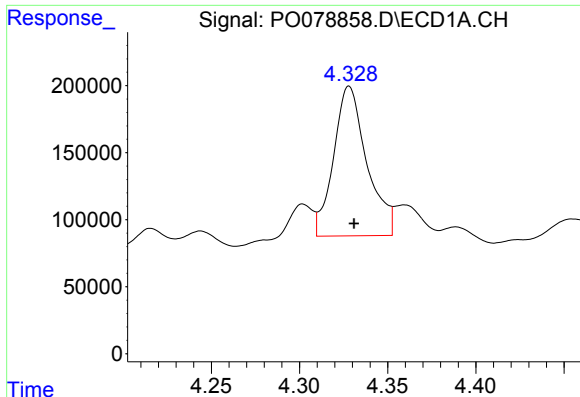


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.003 min
Response: 1477109
Conc: 17.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
33258


Manual Integrations
APPROVED

Ankita
6/18/2021 12:14:12 PM

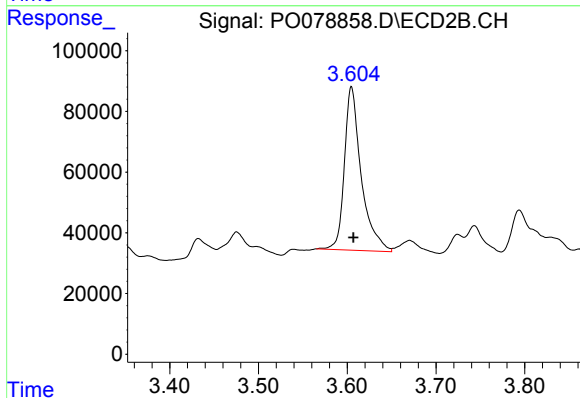


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.002 min
Response: 710376
Conc: 20.52 ng/ml

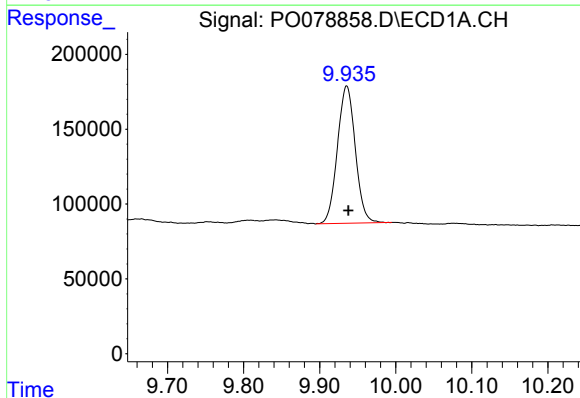

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: -0.002 min
Response: 1497471
Conc: 25.52 ng/ml

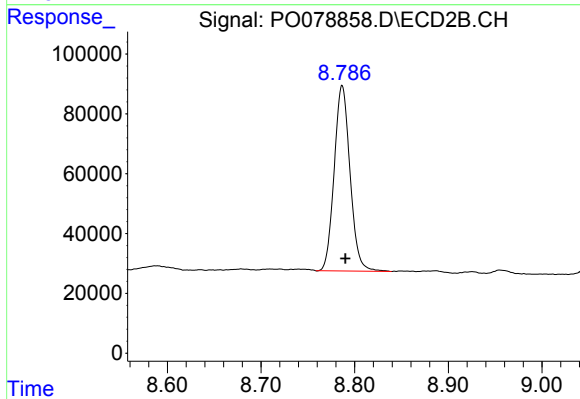

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.003 min
Response: 729549
Conc: 23.46 ng/ml