

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0061721\
 Data File : P0078872.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jun 2021 21:48
 Operator : DD\AJ
 Sample : M2736-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 PL-01-061621

Manual Integrations
 APPROVED

Ankita
 6/18/2021 12:14:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:36:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.605	2029566	758252	23.971	21.903
2) SA Decachlor...	9.937	8.788	1431861	665398	24.399	21.401
Target Compounds						
26) L6 AR-1254-1	6.517	5.688	38028	19155	13.873m	10.842
27) L6 AR-1254-2	6.750	5.844	69767	10078	16.495m	6.220m#
28) L6 AR-1254-3	7.123	6.257	85228	40136	19.575m	16.510m
29) L6 AR-1254-4	7.412	6.496	50731	8015	16.480m	5.353m#
30) L6 AR-1254-5	7.837	6.918	72140	63969	20.929m	27.867 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061721\
Data File : P0078872.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jun 2021 21:48
Operator : DD\AJ
Sample : M2736-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PL-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 12:14:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:36:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

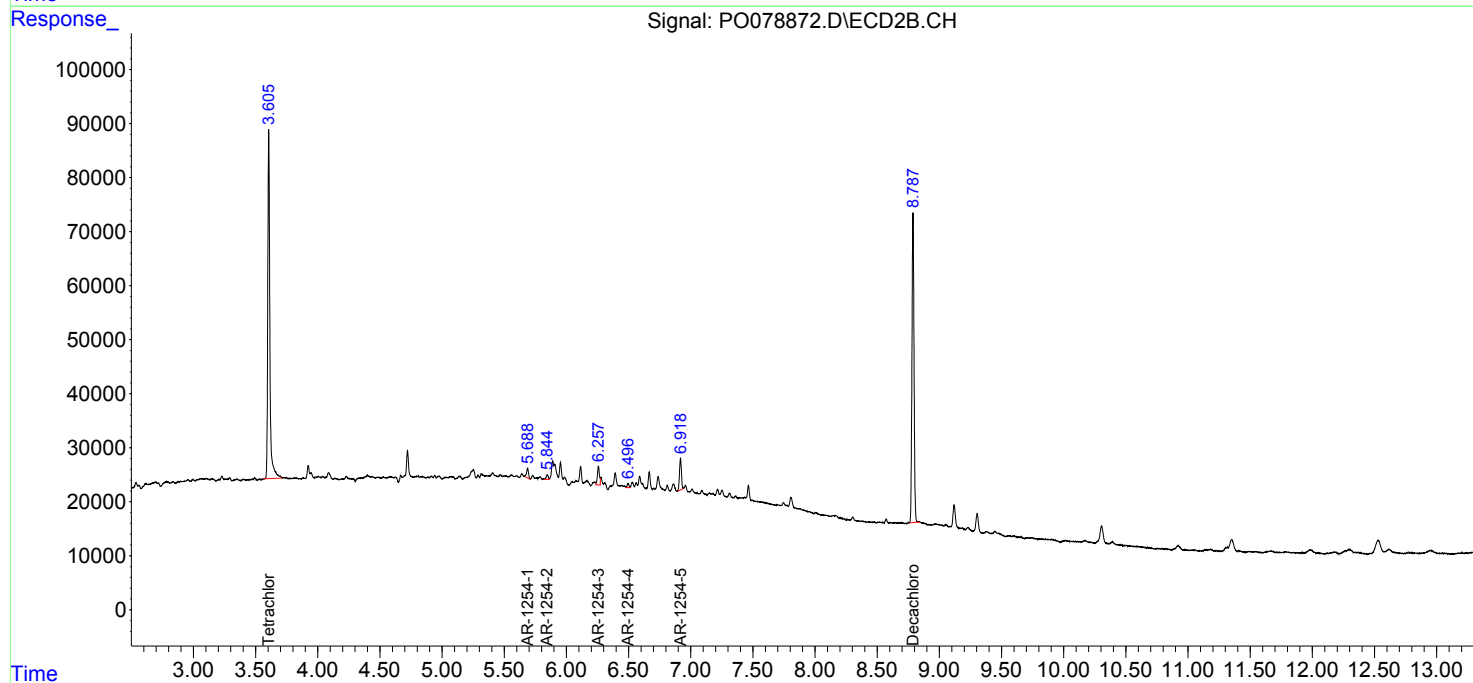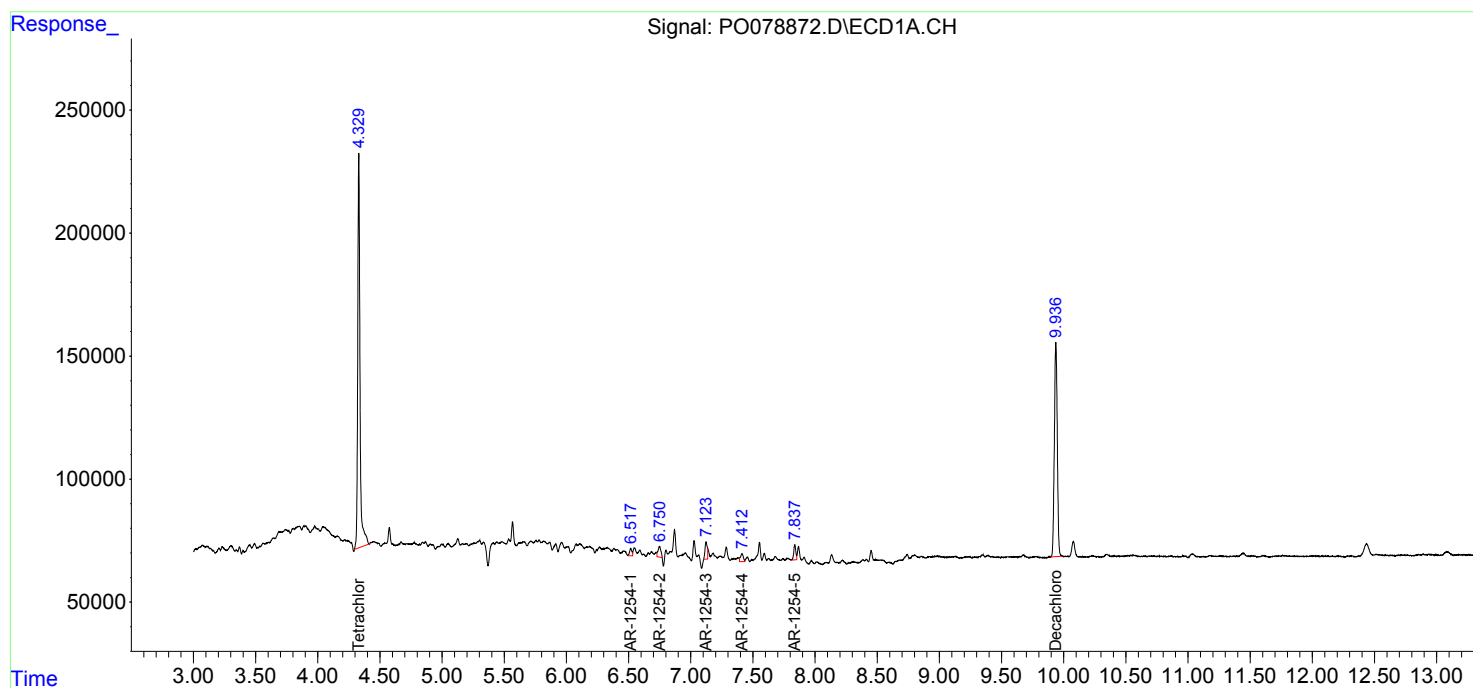

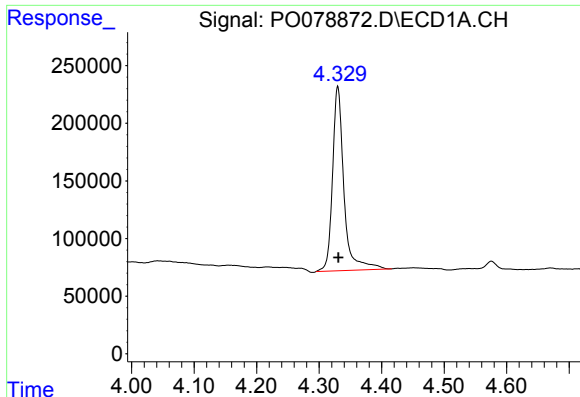


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: -0.001 min
Response: 2029566
Conc: 23.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 12:14:14 PM

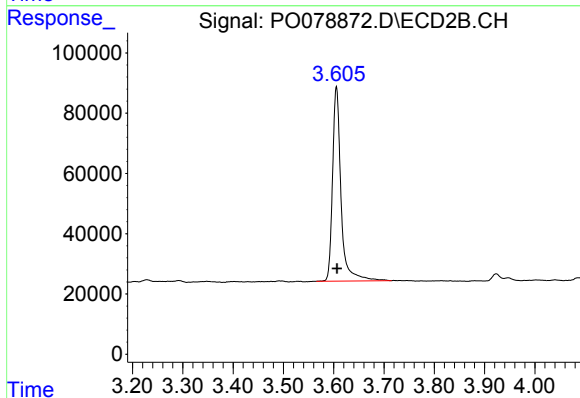


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.001 min
Response: 758252
Conc: 21.90 ng/ml

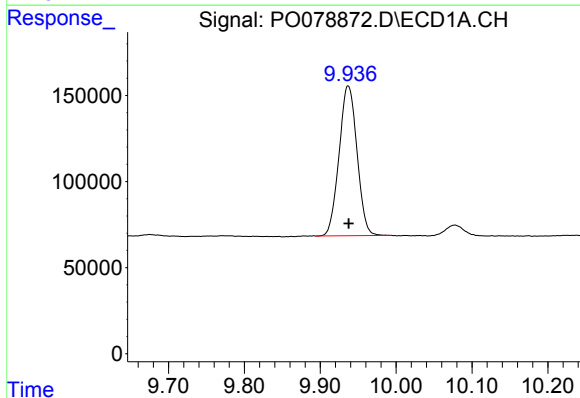


#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: 0.000 min
Response: 1431861
Conc: 24.40 ng/ml

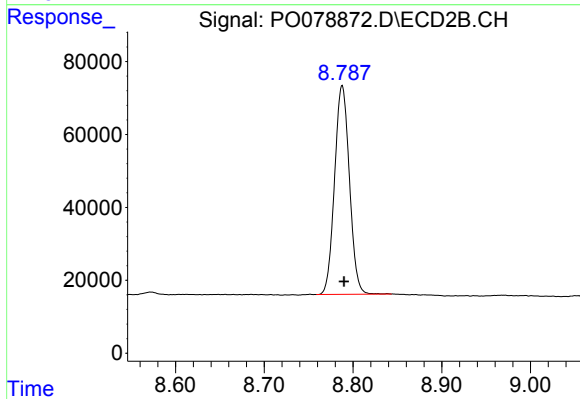

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: -0.002 min
Response: 665398
Conc: 21.40 ng/ml

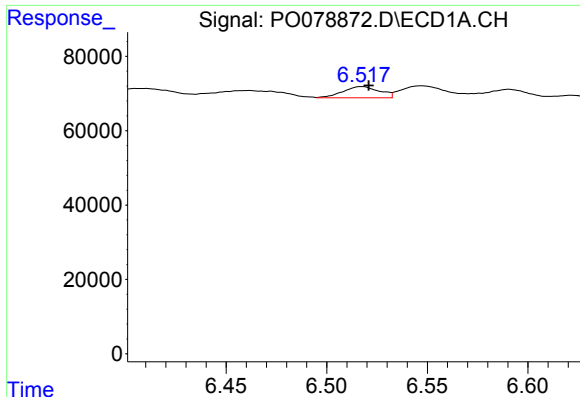


#26 AR-1254-1

R.T.: 6.517 min
Delta R.T.: -0.004 min
Response: 38028
Conc: 13.87 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PL-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 12:14:14 PM

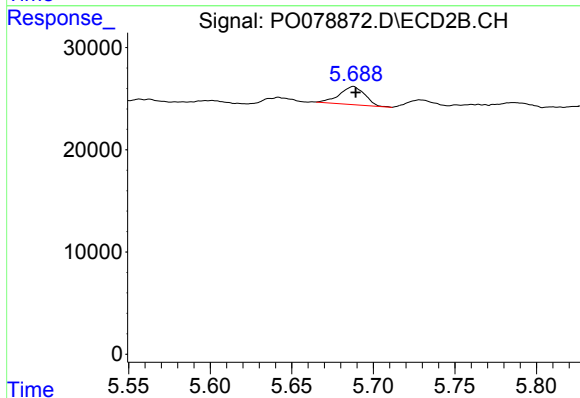


#26 AR-1254-1

R.T.: 5.688 min
Delta R.T.: -0.001 min
Response: 19155
Conc: 10.84 ng/ml

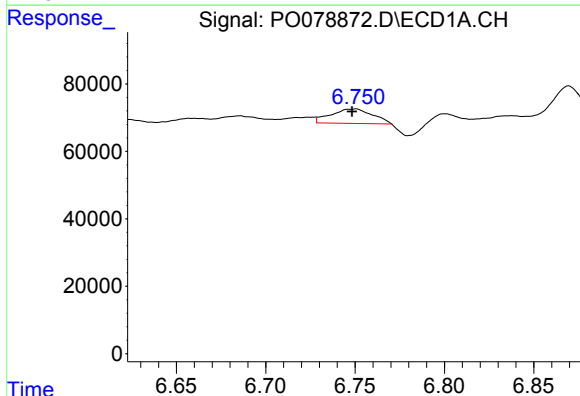


#27 AR-1254-2

R.T.: 6.750 min
Delta R.T.: 0.002 min
Response: 69767
Conc: 16.49 ng/ml m

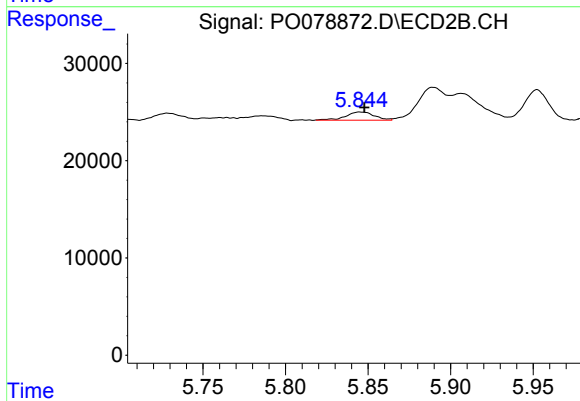

#27 AR-1254-2

R.T.: 5.844 min
Delta R.T.: -0.003 min
Response: 10078
Conc: 6.22 ng/ml m

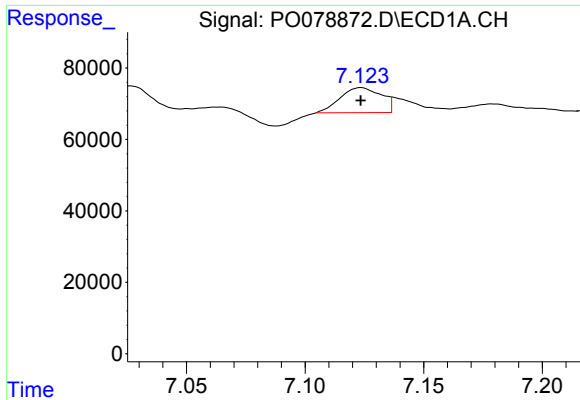


#28 AR-1254-3

R.T.: 7.123 min
Delta R.T.: 0.000 min
Response: 85228
Conc: 19.58 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PL-01-061621


Manual Integrations
APPROVED

Ankita
6/18/2021 12:14:14 PM

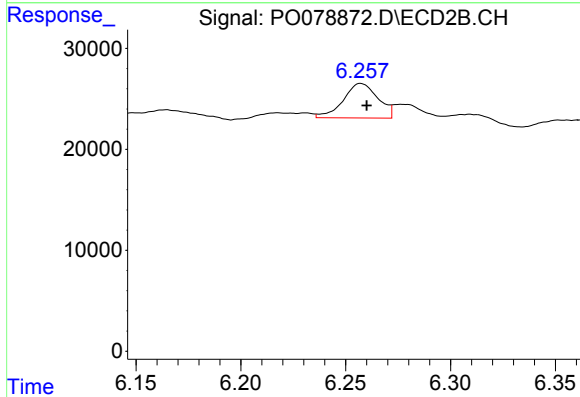


#28 AR-1254-3

R.T.: 6.257 min
Delta R.T.: -0.003 min
Response: 40136
Conc: 16.51 ng/ml m

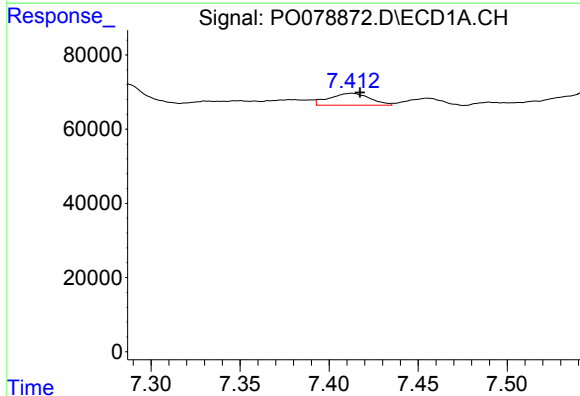


#29 AR-1254-4

R.T.: 7.412 min
Delta R.T.: -0.005 min
Response: 50731
Conc: 16.48 ng/ml m

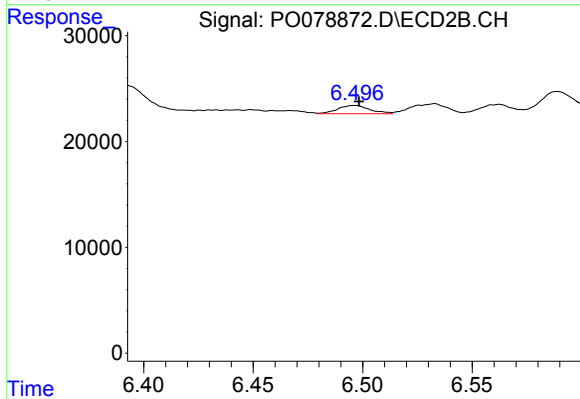

#29 AR-1254-4

R.T.: 6.496 min
Delta R.T.: -0.002 min
Response: 8015
Conc: 5.35 ng/ml m

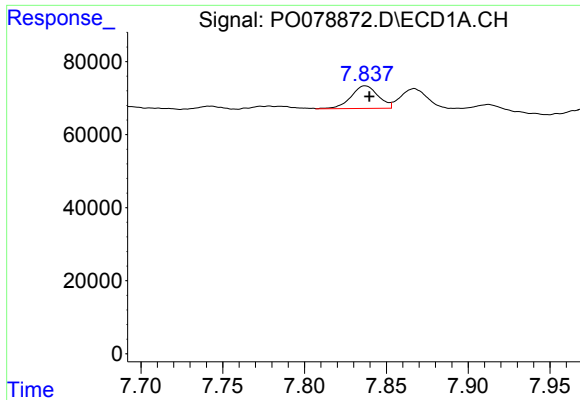


#30 AR-1254-5

R.T.: 7.837 min
Delta R.T.: -0.003 min
Response: 72140
Conc: 20.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PL-01-061621

Manual Integrations
APPROVED

Ankita
6/18/2021 12:14:14 PM

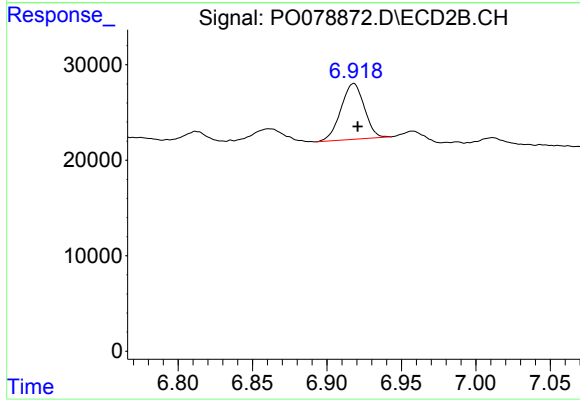

#30 AR-1254-5

R.T.: 6.918 min
Delta R.T.: -0.003 min
Response: 63969
Conc: 27.87 ng/ml