

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061819\
 Data File : P0057239.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2019 20:21
 Operator : SM/SJ
 Sample : K3419-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-A

Manual Integrations
 APPROVED

Ankita
 6/19/2019 1:38:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:27:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.237	3.560	1213928	946972	31.709	28.715
2)	SA Decachlor...	9.795	8.484	1010603	688413	20.589	19.307m
Target Compounds							
31)	L7 AR-1260-1	6.983	6.089	1001290	819837	390.187	409.841
32)	L7 AR-1260-2	7.239	6.277	1220721	1021728	403.656m	414.501
33)	L7 AR-1260-3	7.595	6.428	793684	876977	329.459	390.944
34)	L7 AR-1260-4	7.820	6.894	862565	651136	329.322	349.881m
35)	L7 AR-1260-5	8.127	7.137	1706872	1595715	356.931m	370.035

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061819\
Data File : P0057239.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2019 20:21
Operator : SM/SJ
Sample : K3419-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-A


Manual Integrations
APPROVED

Ankita
6/19/2019 1:38:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:27:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

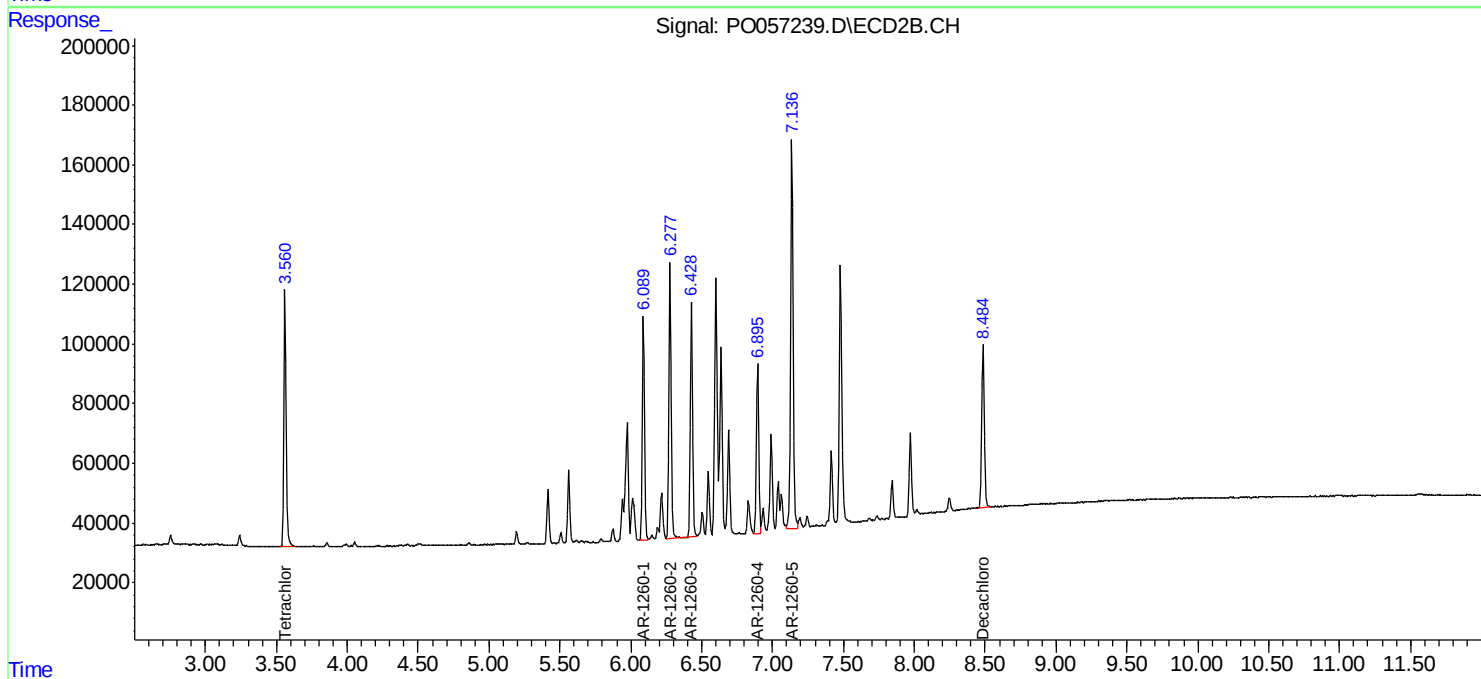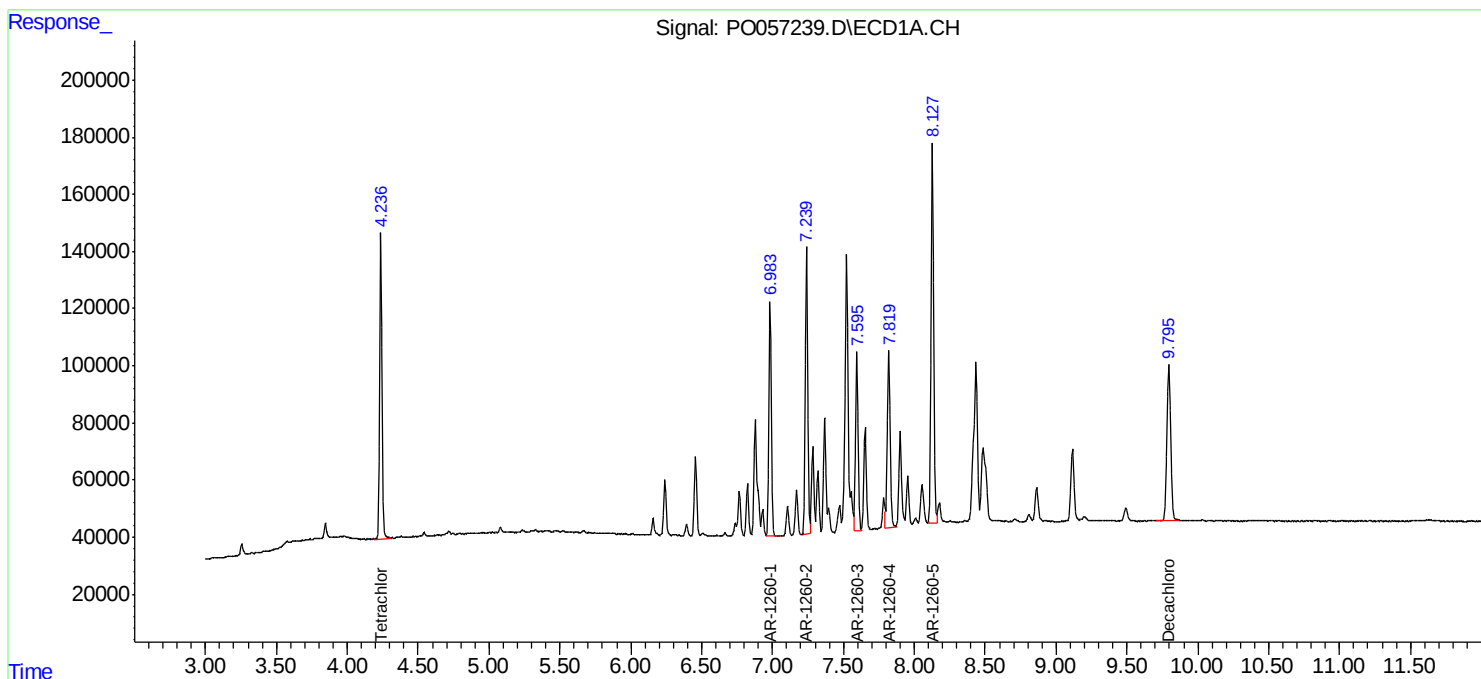

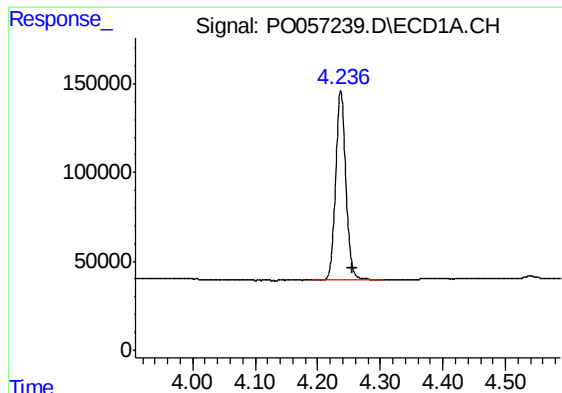


#1 Tetrachloro-m-xylene

R.T.: 4.237 min
Delta R.T.: -0.019 min
Response: 1213928
Conc: 31.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A


Manual Integrations
APPROVED

Ankita
6/19/2019 1:38:06 PM

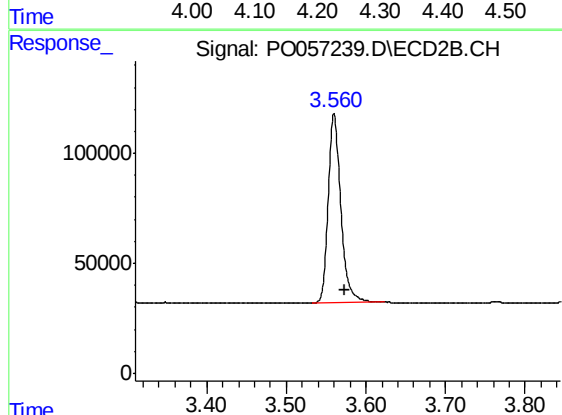


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.013 min
Response: 946972
Conc: 28.71 ng/ml

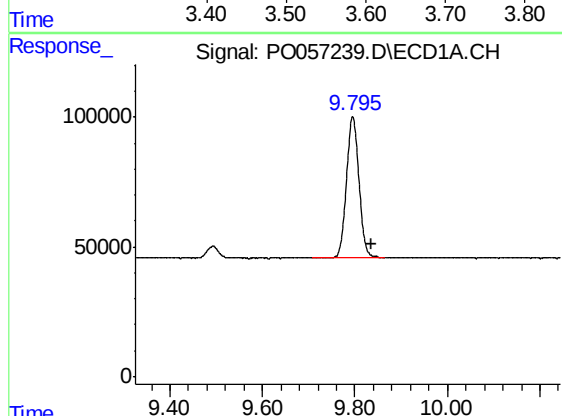


#2 Decachlorobiphenyl

R.T.: 9.795 min
Delta R.T.: -0.041 min
Response: 1010603
Conc: 20.59 ng/ml

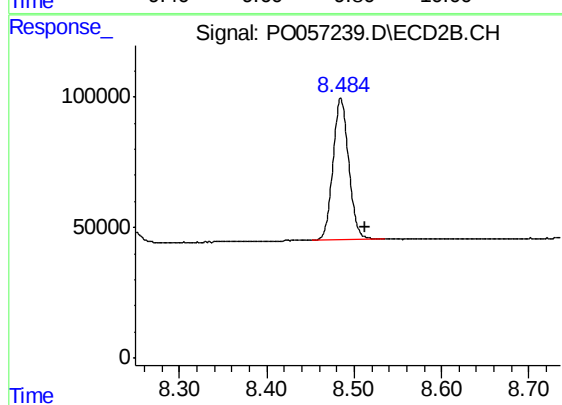

#2 Decachlorobiphenyl

R.T.: 8.484 min
Delta R.T.: -0.029 min
Response: 688413
Conc: 19.31 ng/ml m

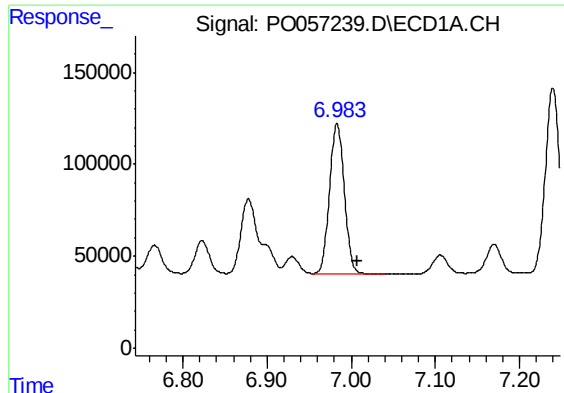


#31 AR-1260-1

R.T.: 6.983 min
Delta R.T.: -0.024 min
Response: 1001290
Conc: 390.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A


Manual Integrations
APPROVED

Ankita
6/19/2019 1:38:06 PM

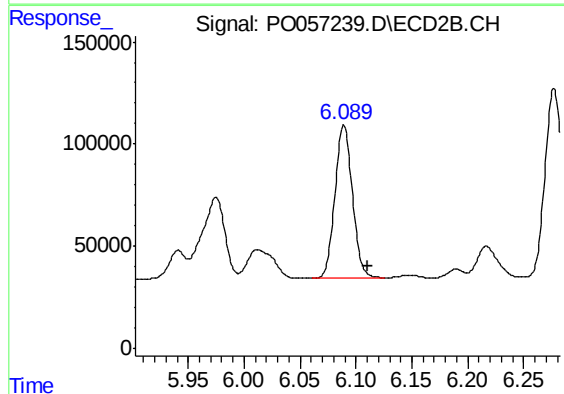


#31 AR-1260-1

R.T.: 6.089 min
Delta R.T.: -0.021 min
Response: 819837
Conc: 409.84 ng/ml

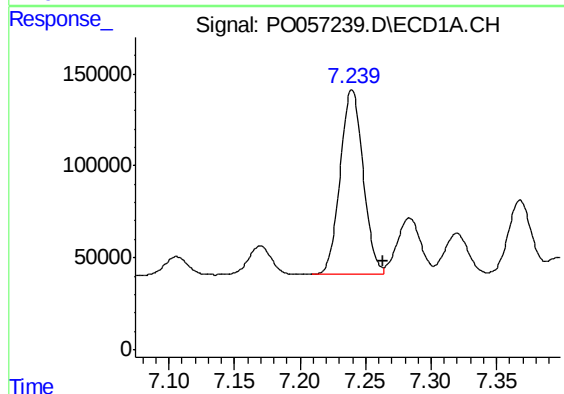


#32 AR-1260-2

R.T.: 7.239 min
Delta R.T.: -0.024 min
Response: 1220721
Conc: 403.66 ng/ml m

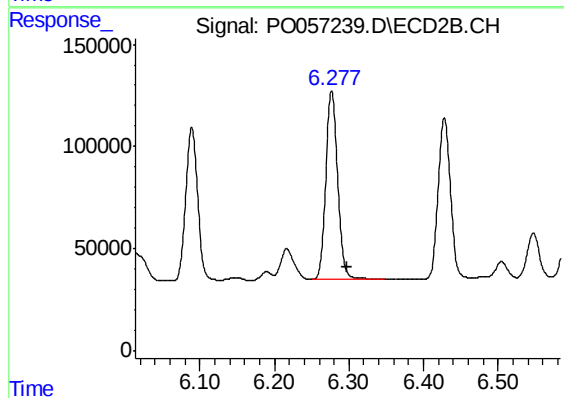

#32 AR-1260-2

R.T.: 6.277 min
Delta R.T.: -0.020 min
Response: 1021728
Conc: 414.50 ng/ml

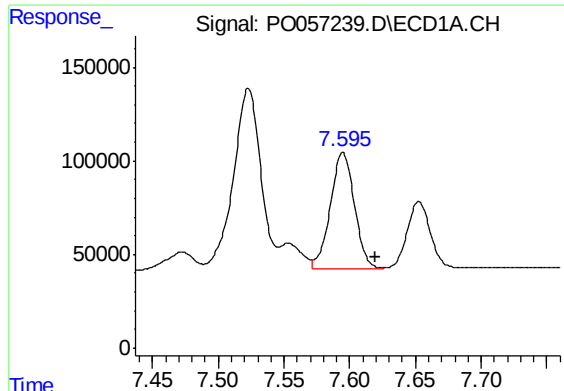


#33 AR-1260-3

R.T.: 7.595 min
Delta R.T.: -0.025 min
Response: 793684
Conc: 329.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A


Manual Integrations
APPROVED

Ankita
6/19/2019 1:38:06 PM

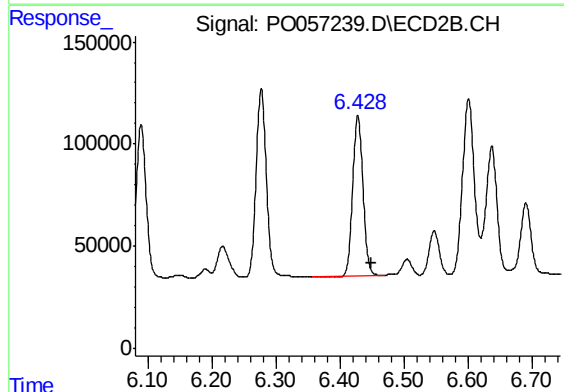


#33 AR-1260-3

R.T.: 6.428 min
Delta R.T.: -0.022 min
Response: 876977
Conc: 390.94 ng/ml

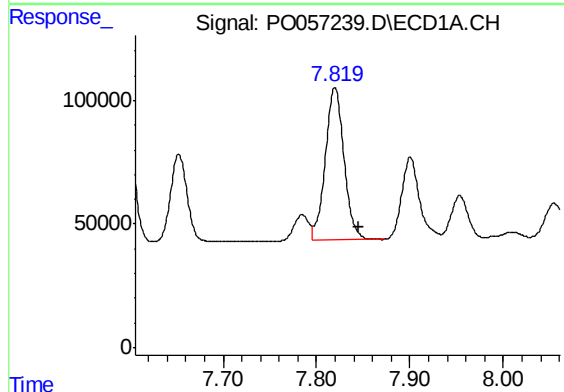


#34 AR-1260-4

R.T.: 7.820 min
Delta R.T.: -0.025 min
Response: 862565
Conc: 329.32 ng/ml

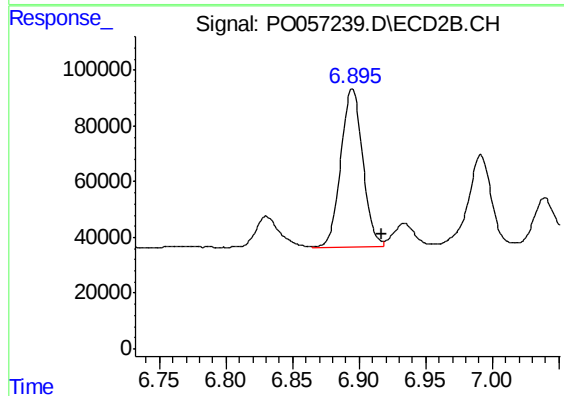

#34 AR-1260-4

R.T.: 6.894 min
Delta R.T.: -0.022 min
Response: 651136
Conc: 349.88 ng/ml m

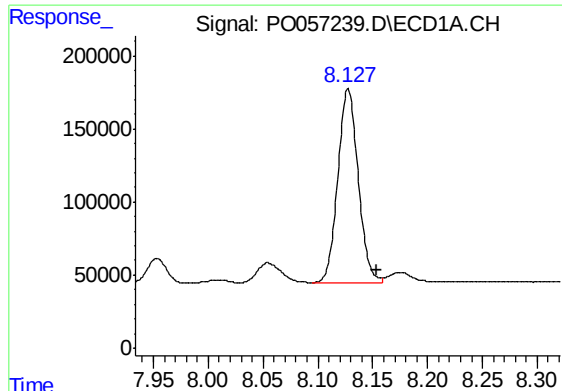


#35 AR-1260-5

R.T.: 8.127 min
Delta R.T.: -0.026 min
Response: 1706872
Conc: 356.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-A

Manual Integrations
APPROVED

Ankita
6/19/2019 1:38:06 PM

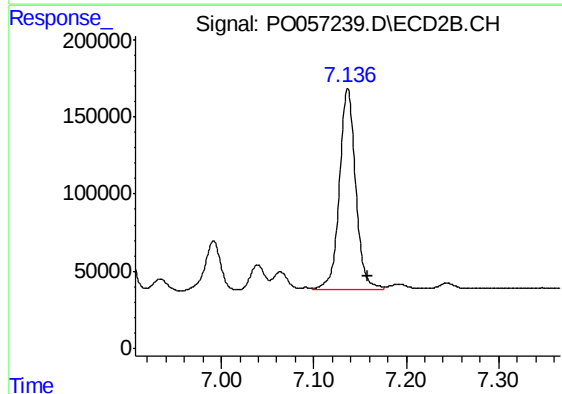

#35 AR-1260-5

R.T.: 7.137 min
Delta R.T.: -0.021 min
Response: 1595715
Conc: 370.04 ng/ml