

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061819\
 Data File : P0057246.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2019 22:21
 Operator : SM/SJ
 Sample : K3420-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BAT-B12

Manual Integrations
 APPROVED

Ankita
 6/19/2019 1:38:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:30:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.235	3.559	1289936	974783	33.694	29.558
2)	SA Decachlor...	9.794	8.483	1116598	763678	22.749	21.417m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061819\
Data File : PO057246.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2019 22:21
Operator : SM/SJ
Sample : K3420-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BAT-B12


Manual Integrations
APPROVED

Ankita
6/19/2019 1:38:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:30:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

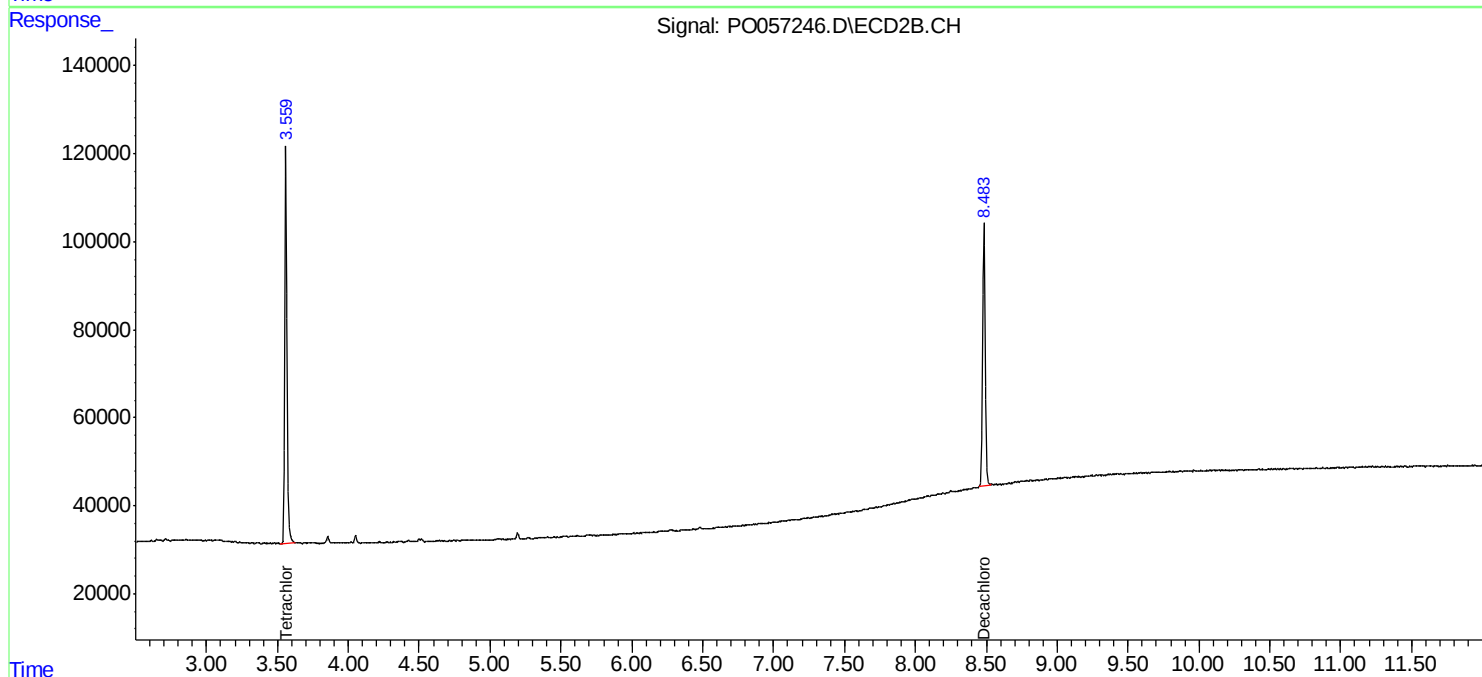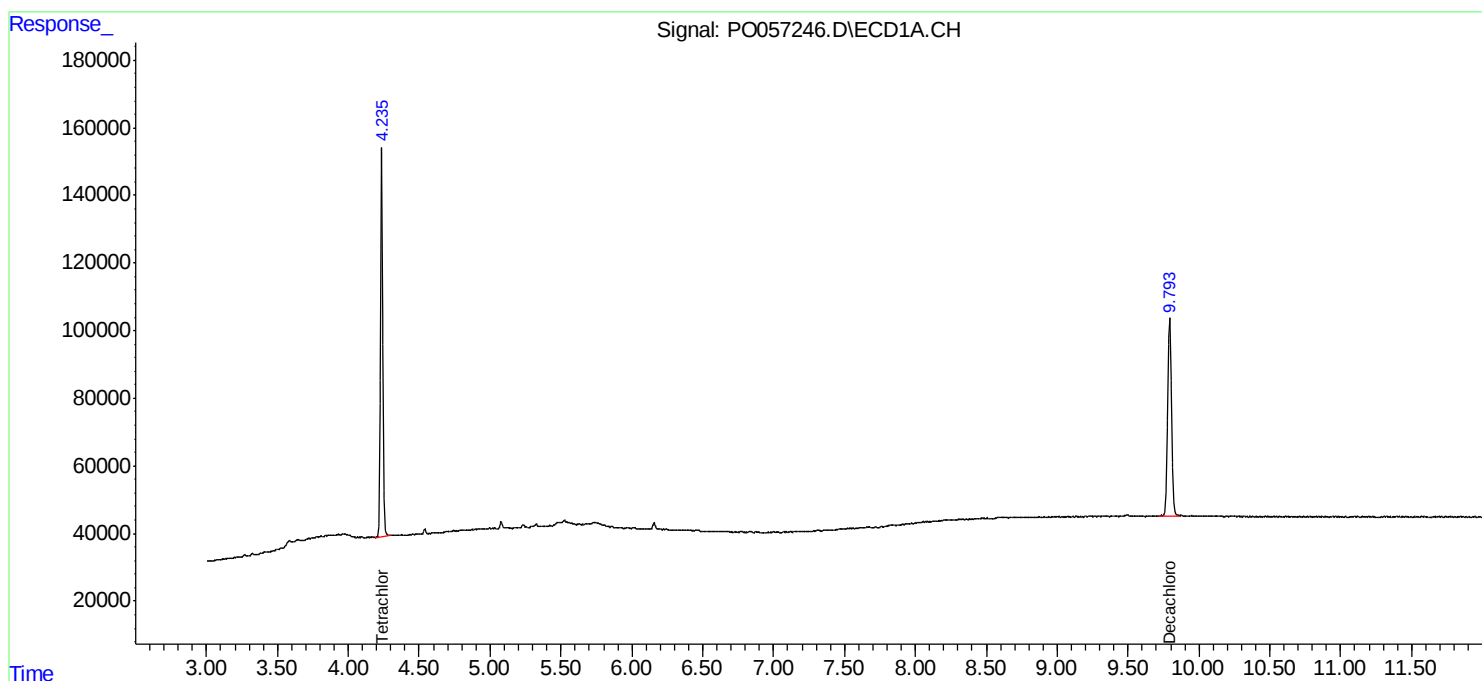

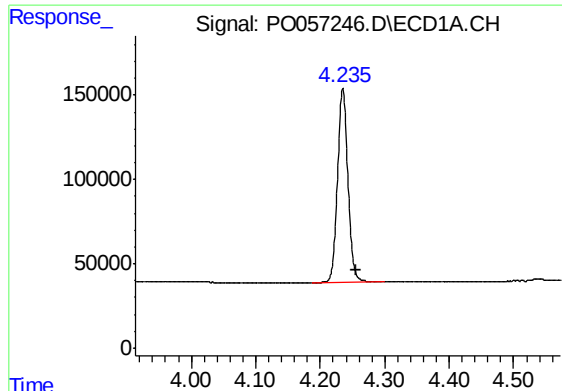


#1 Tetrachloro-m-xylene

R.T.: 4.235 min
Delta R.T.: -0.021 min
Response: 1289936
Conc: 33.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
BAT-B12


Manual Integrations
APPROVED

Ankita
6/19/2019 1:38:22 PM

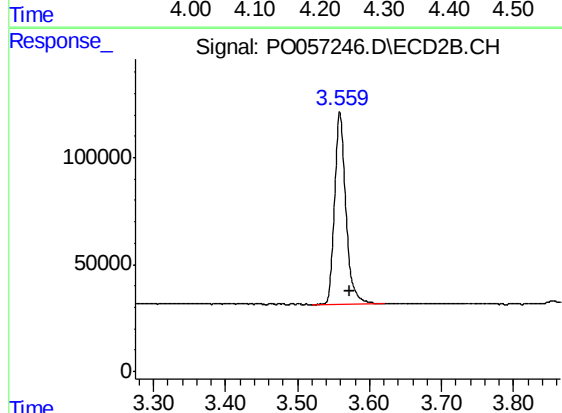


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 974783
Conc: 29.56 ng/ml

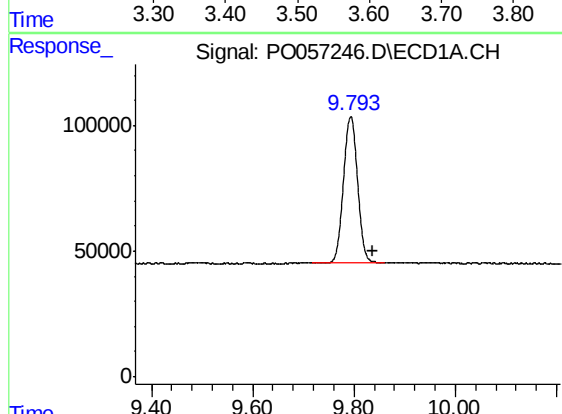

#2 Decachlorobiphenyl

R.T.: 9.794 min
Delta R.T.: -0.043 min
Response: 1116598
Conc: 22.75 ng/ml

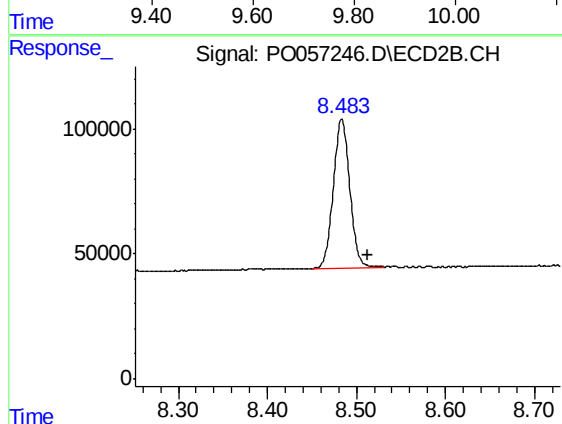

#2 Decachlorobiphenyl

R.T.: 8.483 min
Delta R.T.: -0.030 min
Response: 763678
Conc: 21.42 ng/ml m