

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061821\
 Data File : P0078897.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 9:46
 Operator : DD\AJ
 Sample : M2760-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 13:32:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 14 05:33:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.603	1998630	889038	23.606	25.681
2) SA Decachlor...	9.933	8.784	1938697	1055439	33.036	33.946m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 02-A-02-B-02-C

Manual Integrations
 APPROVED

Ankita
 6/21/2021 10:53:10 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061821\
Data File : PO078897.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 9:46
Operator : DD\AJ
Sample : M2760-02
Misc :
ALS Vial : 5 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 13:32:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061321.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 14 05:33:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C

Manual Integrations
APPROVED

Ankita
6/21/2021 10:53:10 AM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

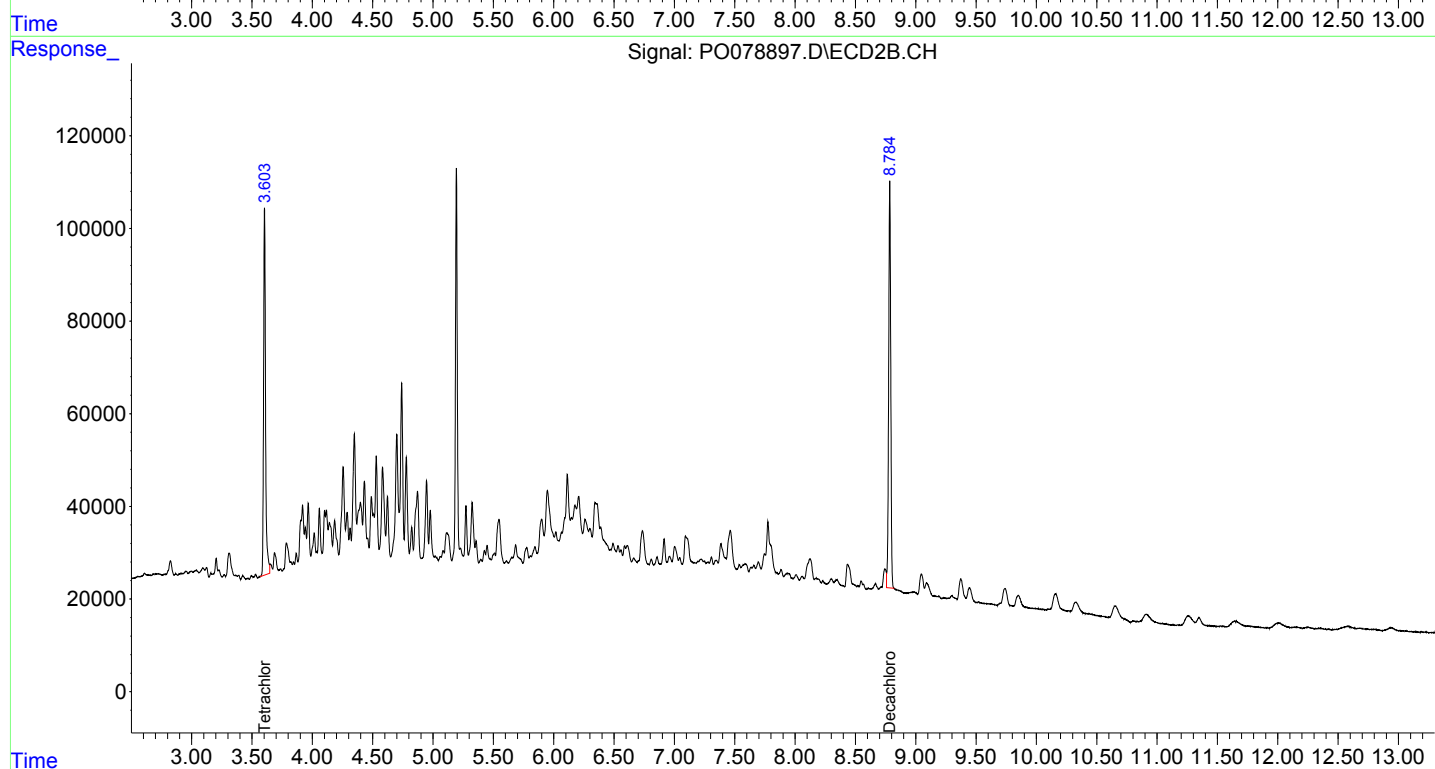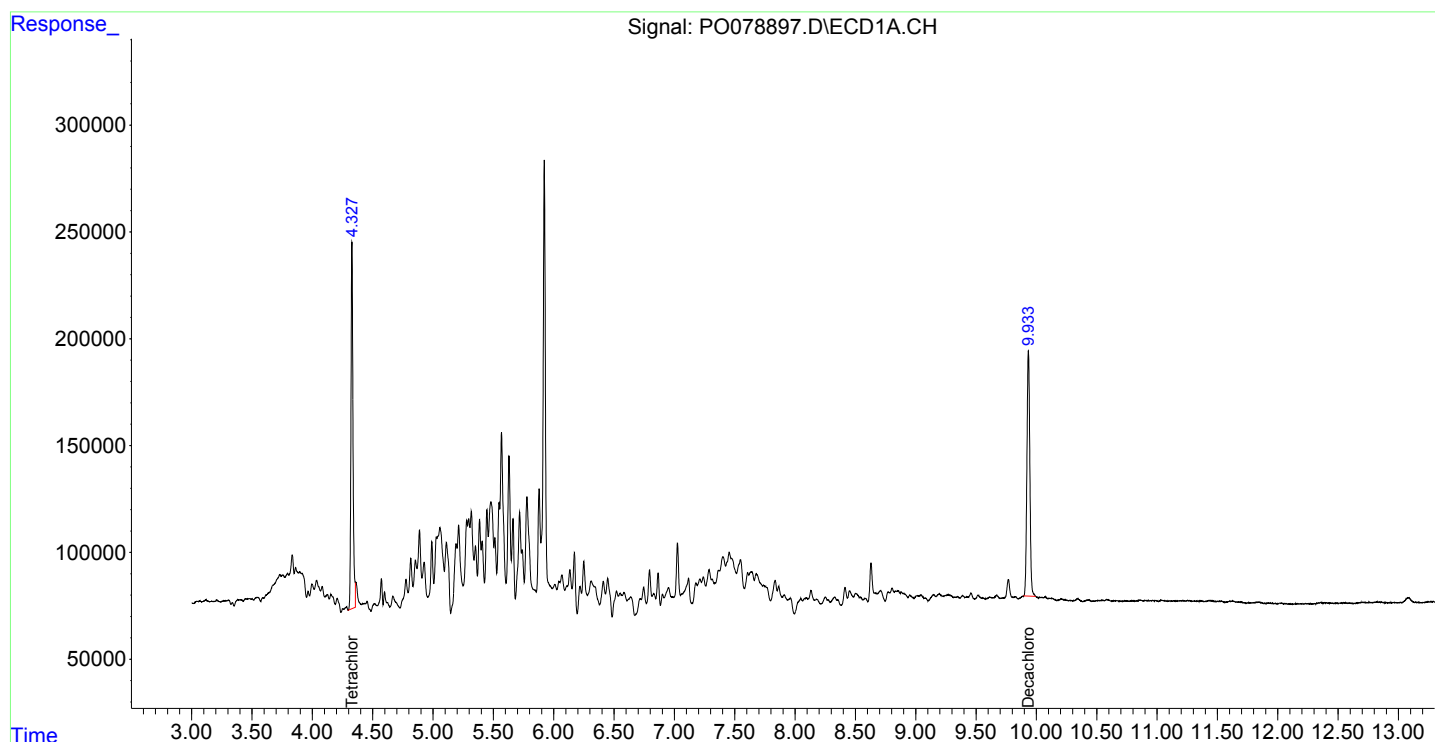

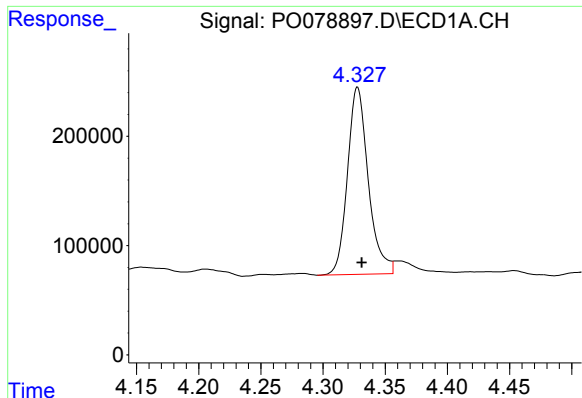


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.003 min
Response: 1998630
Conc: 23.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
6/21/2021 10:53:10 AM

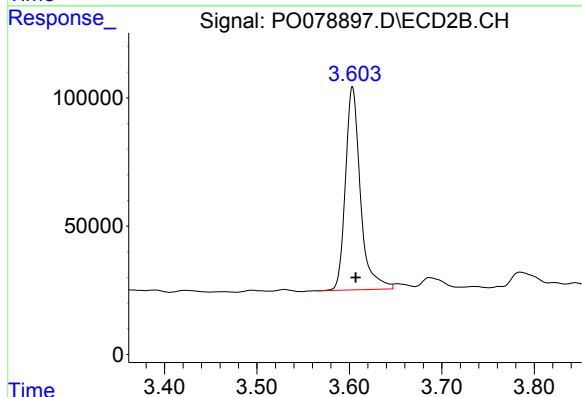


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.003 min
Response: 889038
Conc: 25.68 ng/ml

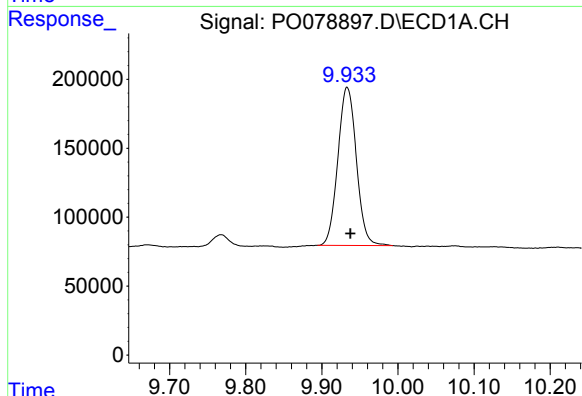

#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.004 min
Response: 1938697
Conc: 33.04 ng/ml

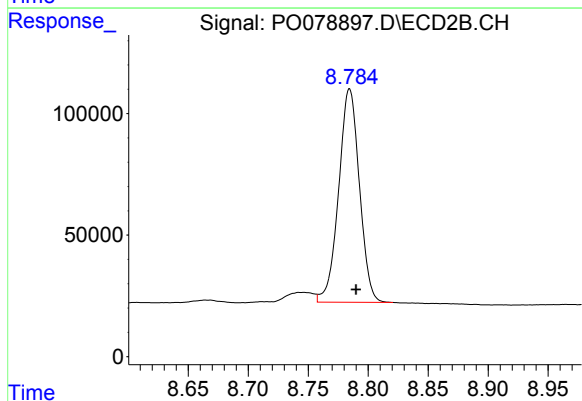

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: -0.006 min
Response: 1055439
Conc: 33.95 ng/ml m