

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061825\
 Data File : P0111686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 14:11
 Operator : YP/AJ
 Sample : DDT ANALOGUE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOGUE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:32:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.676	3.674	71867657	62263910	12.478	11.084
2) SA Decachlor...	8.711	8.660	108.5E6	39306072	20.668	22.111

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061825\
Data File : PO111686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 14:11
Operator : YP/AJ
Sample : DDT ANALOGUE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:32:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

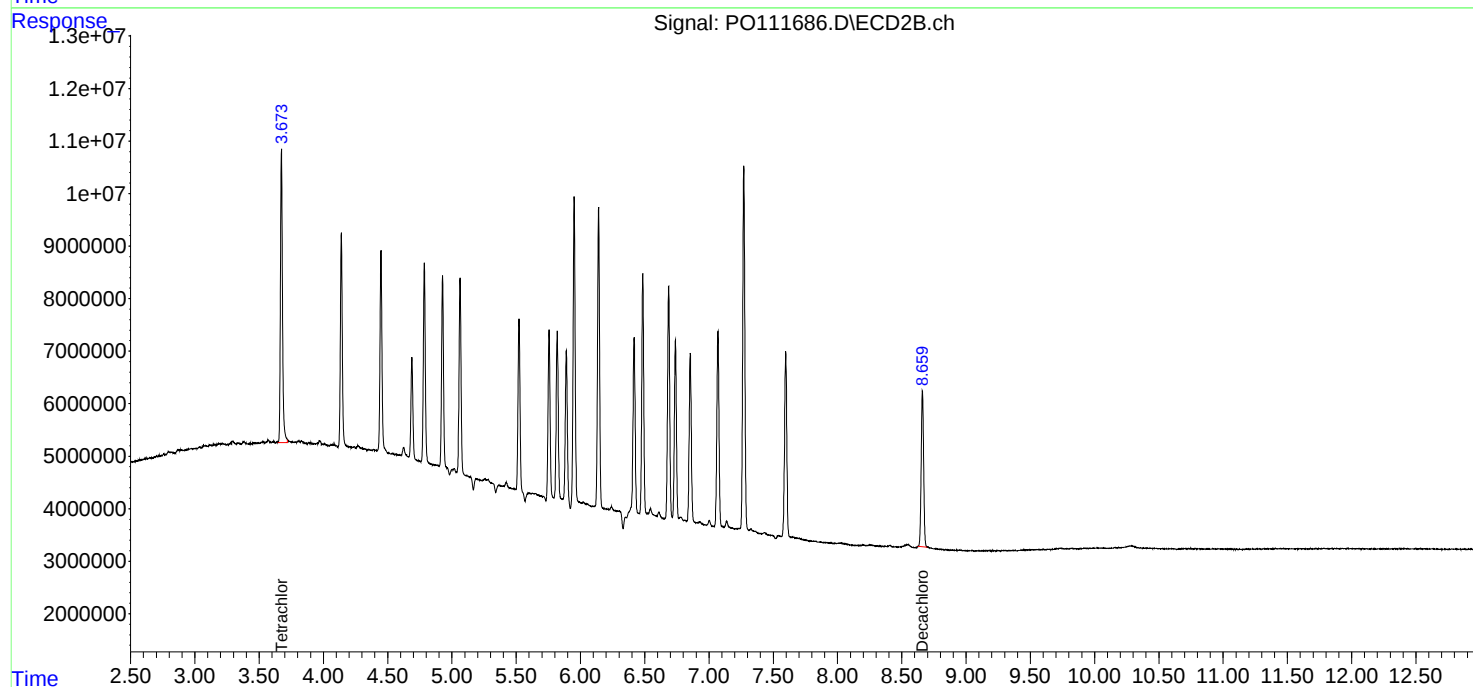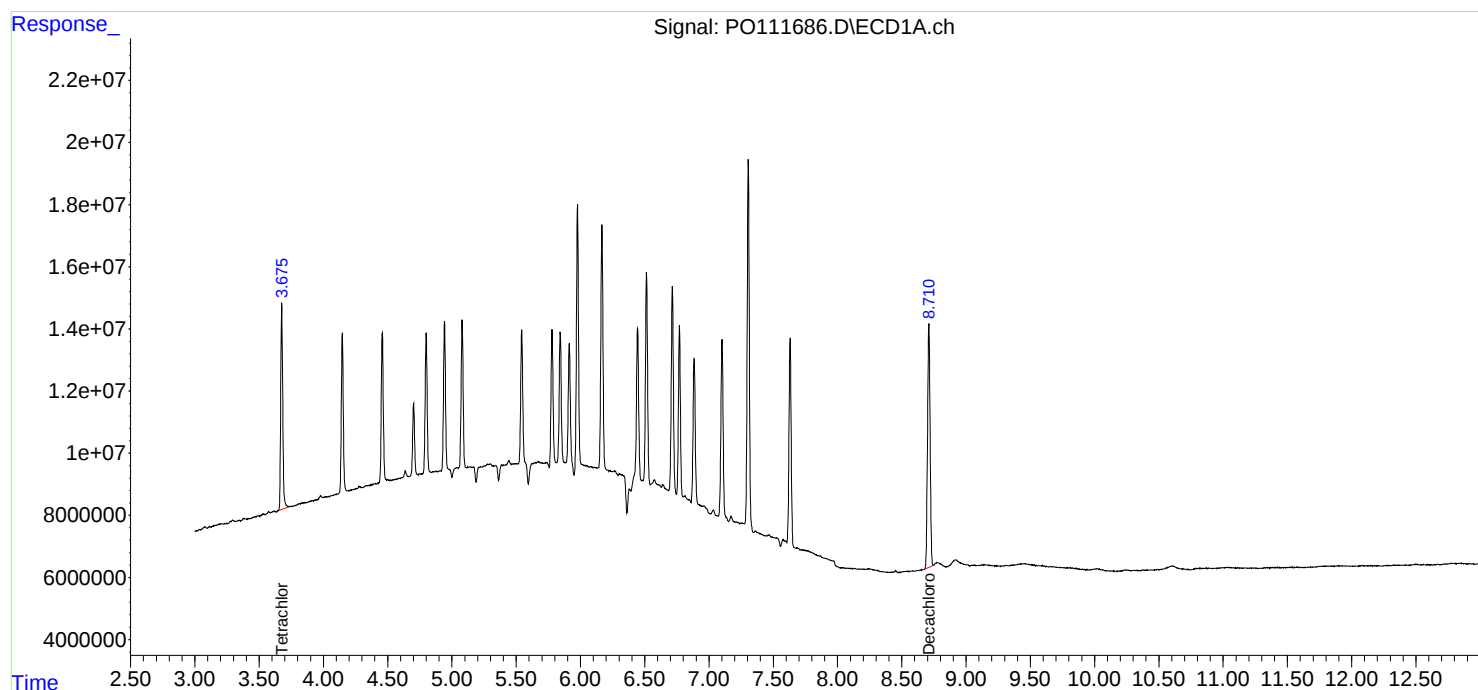


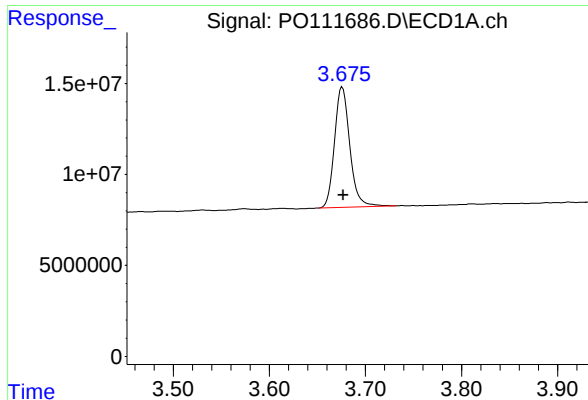

#1 Tetrachloro-m-xylene


R.T.: 3.676 min
Delta R.T.: -0.001 min
Response: 71867657
Conc: 12.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOGUE

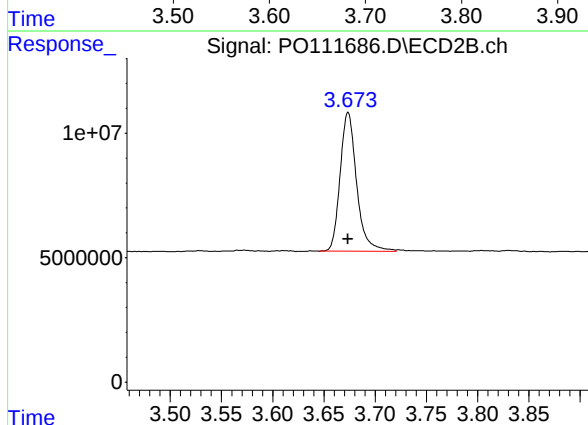


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: 0.000 min
Response: 62263910
Conc: 11.08 ng/ml

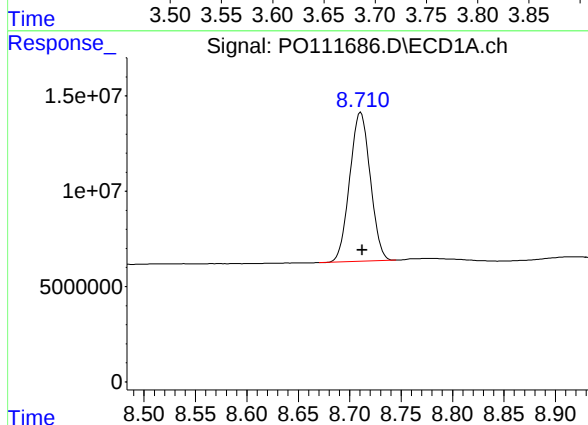

#2 Decachlorobiphenyl

R.T.: 8.711 min
Delta R.T.: -0.002 min
Response: 108489384
Conc: 20.67 ng/ml

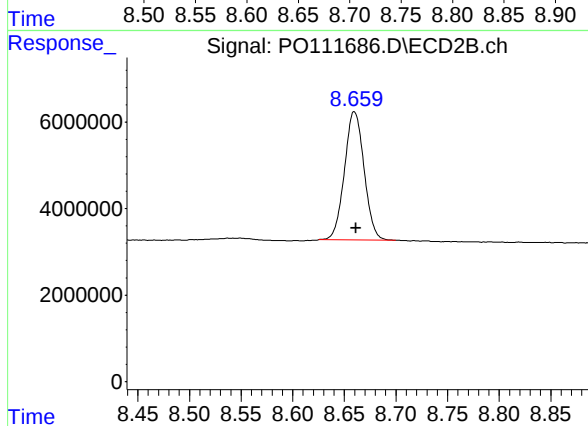

#2 Decachlorobiphenyl

R.T.: 8.660 min
Delta R.T.: -0.002 min
Response: 39306072
Conc: 22.11 ng/ml