

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0061825\  
 Data File : P0111695.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Jun 2025 18:02  
 Operator : YP/AJ  
 Sample : Q2307-03  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 LINDEN-SAA-WATER

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 06/19/2025  
 Supervised By :mohammad ahmed 06/20/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 19 04:20:20 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0061125.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Jun 12 06:25:26 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-------|-------|----------|----------|---------|---------|
| -----                       |       |       |          |          |         |         |
| System Monitoring Compounds |       |       |          |          |         |         |
| 1) SA Tetrachlo...          | 3.675 | 3.674 | 69639451 | 75260713 | 12.091m | 13.398m |
| 2) SA Decachlor...          | 8.711 | 8.660 | 40702476 | 14873082 | 7.754m  | 8.367m  |

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO061825\  
Data File : PO111695.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Jun 2025 18:02  
Operator : YP/AJ  
Sample : Q2307-03  
Misc :  
ALS Vial : 16 Sample Multiplier: 1



Instrument :  
ECD\_O  
ClientSampleId :  
LINDEN-SAA-WATER


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/19/2025  
Supervised By :mohammad ahmed 06/20/2025

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 19 04:20:20 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO061125.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Jun 12 06:25:26 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

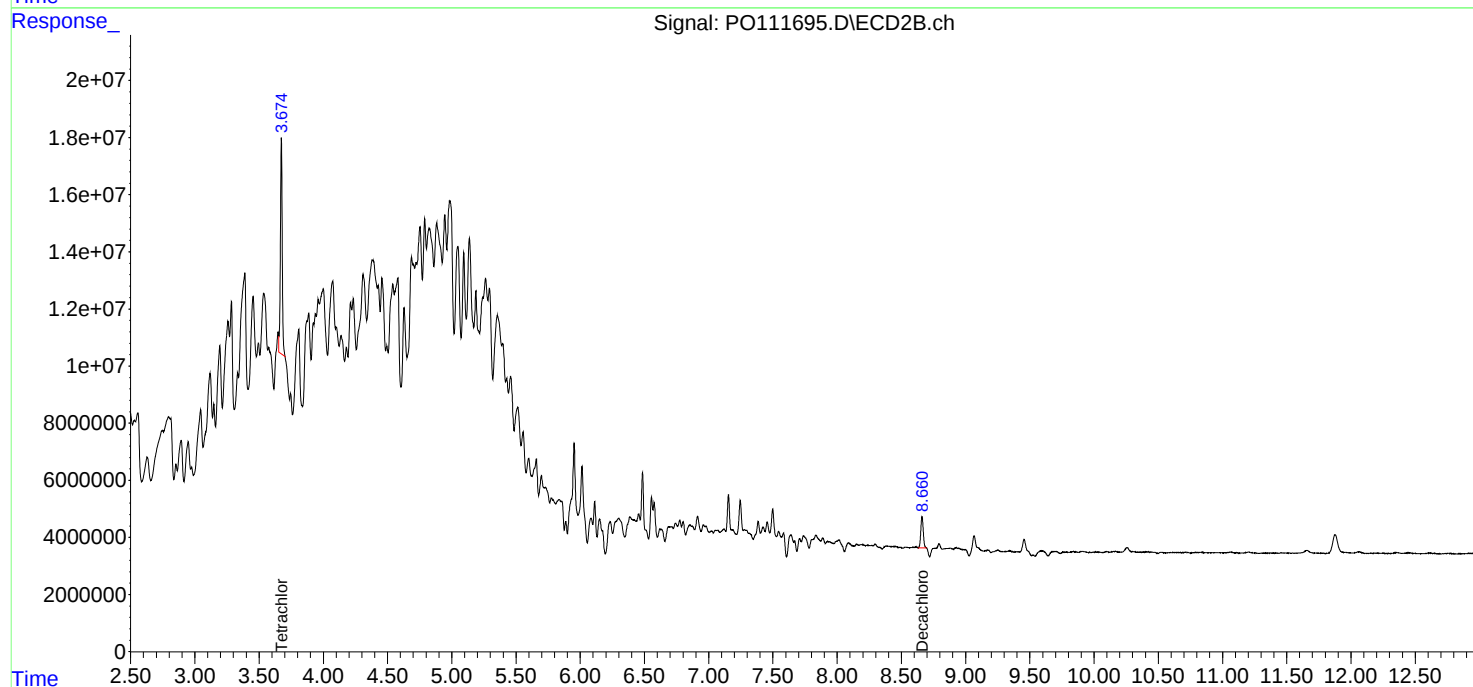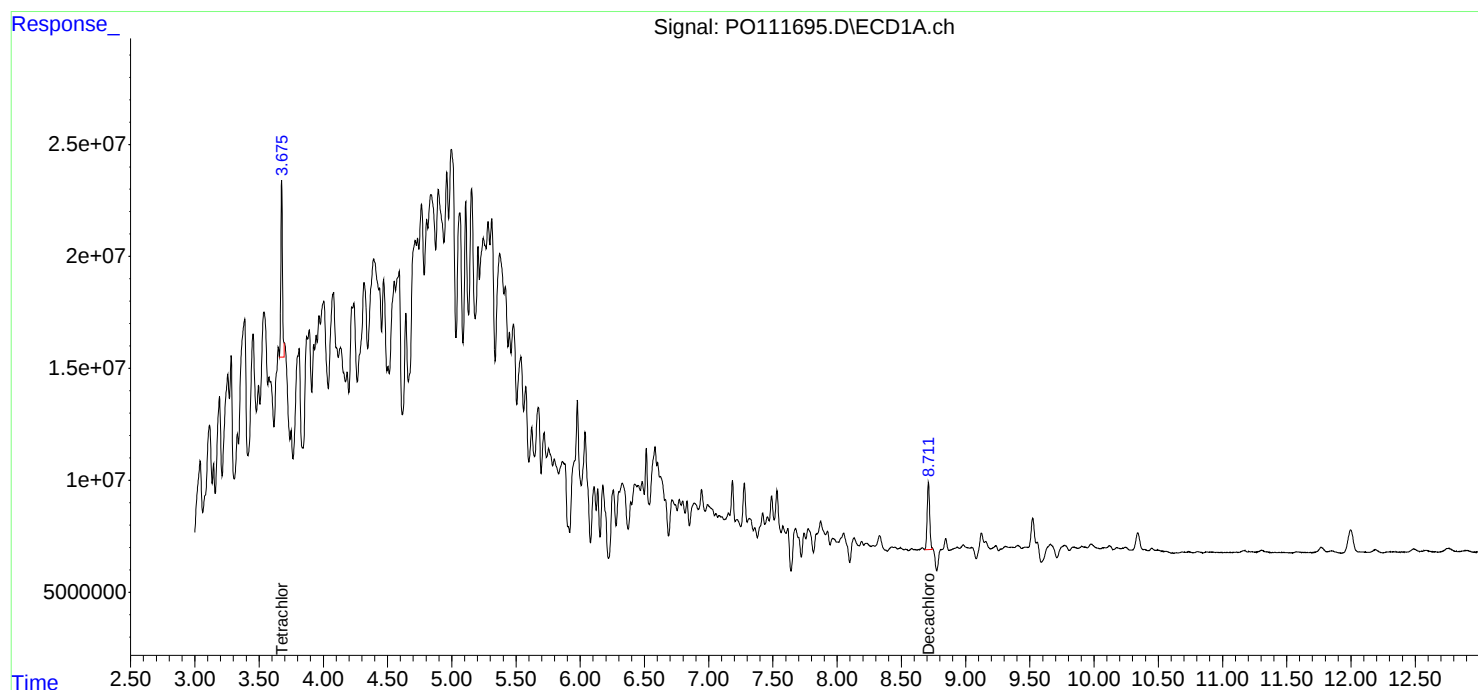

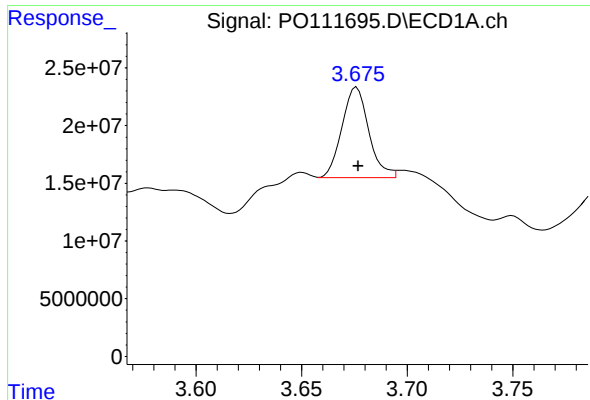


#1 Tetrachloro-m-xylene

R.T.: 3.675 min  
Delta R.T.: -0.002 min  
Response: 69639451  
Conc: 12.09 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
LINDEN-SAA-WATER


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/19/2025  
Supervised By :mohammad ahmed 06/20/2025

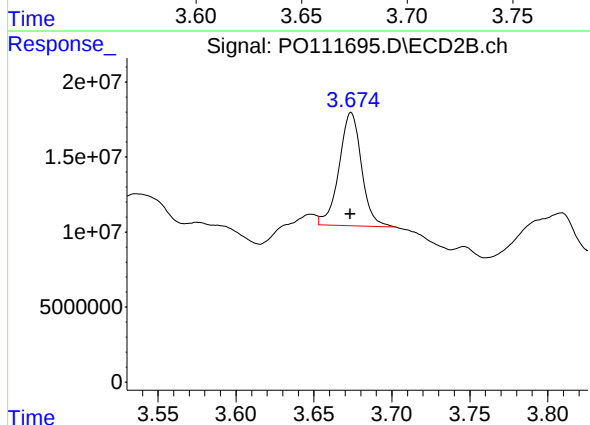


#1 Tetrachloro-m-xylene

R.T.: 3.674 min  
Delta R.T.: 0.000 min  
Response: 75260713  
Conc: 13.40 ng/ml

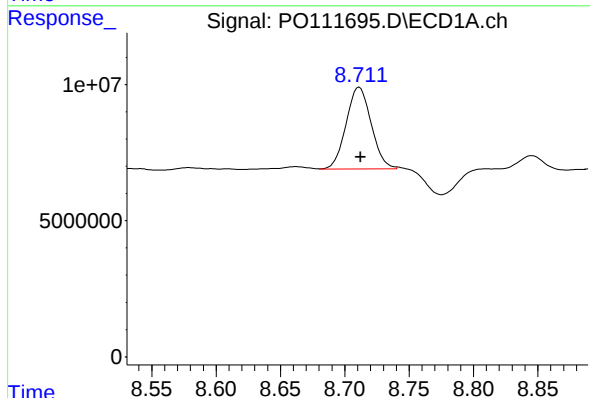

#2 Decachlorobiphenyl

R.T.: 8.711 min  
Delta R.T.: -0.002 min  
Response: 40702476  
Conc: 7.75 ng/ml

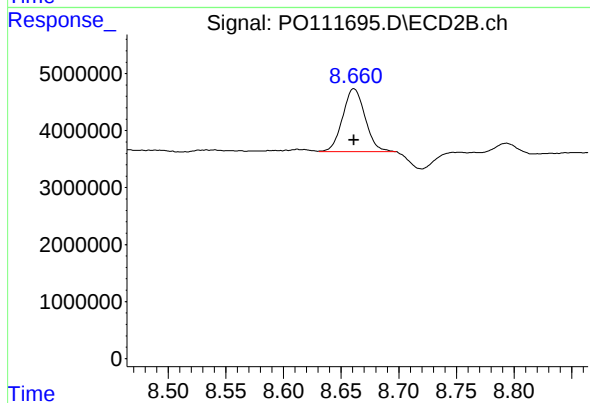

#2 Decachlorobiphenyl

R.T.: 8.660 min  
Delta R.T.: 0.000 min  
Response: 14873082  
Conc: 8.37 ng/ml