

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061825\
 Data File : P0111698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 18:55
 Operator : YP/AJ
 Sample : Q2353-02 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC271315-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/19/2025
 Supervised By :mohammad ahmed 06/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 04:21:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.675	3.673	7565335	5980632	1.314	1.065
2) SA Decachlor...	8.711	8.661	5324807	1802531	1.014	1.014m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061825\
Data File : PO111698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 18:55
Operator : YP/AJ
Sample : Q2353-02 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC271315-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/19/2025
Supervised By :mohammad ahmed 06/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 04:21:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

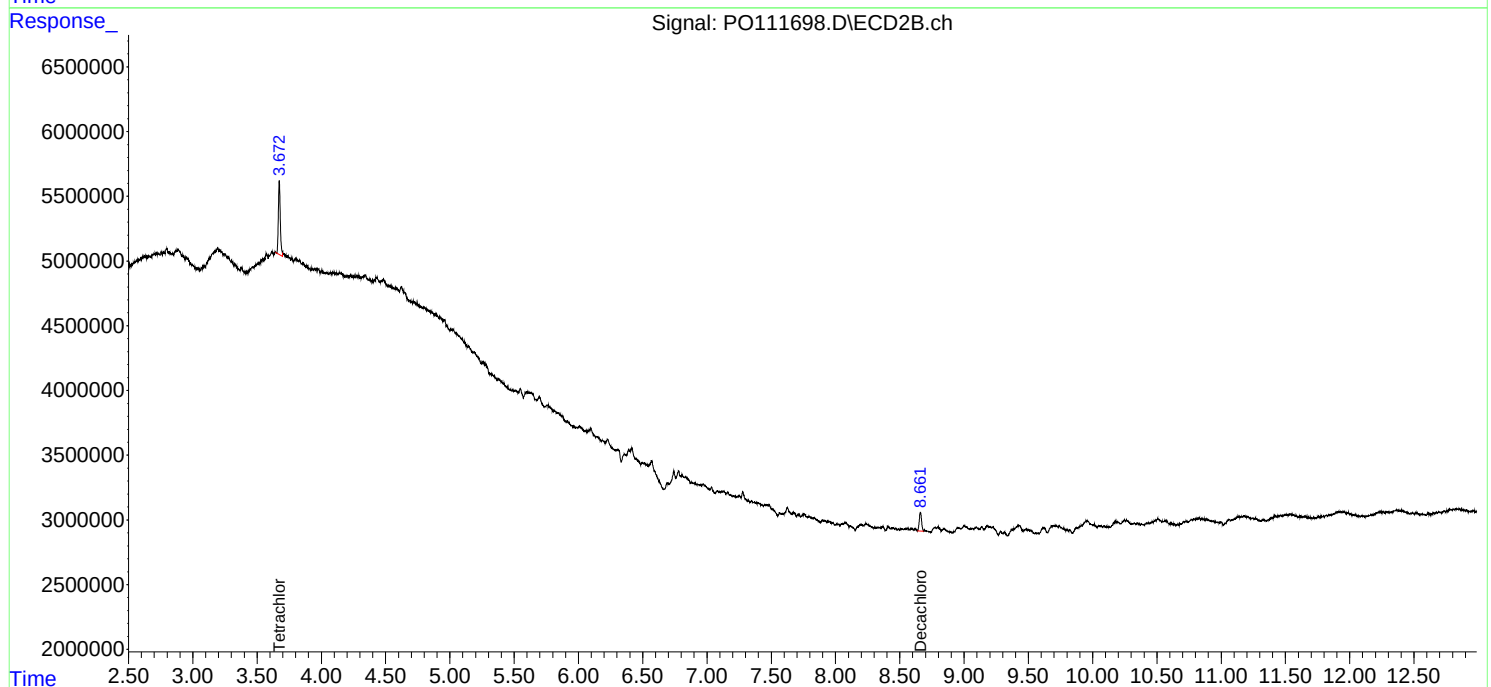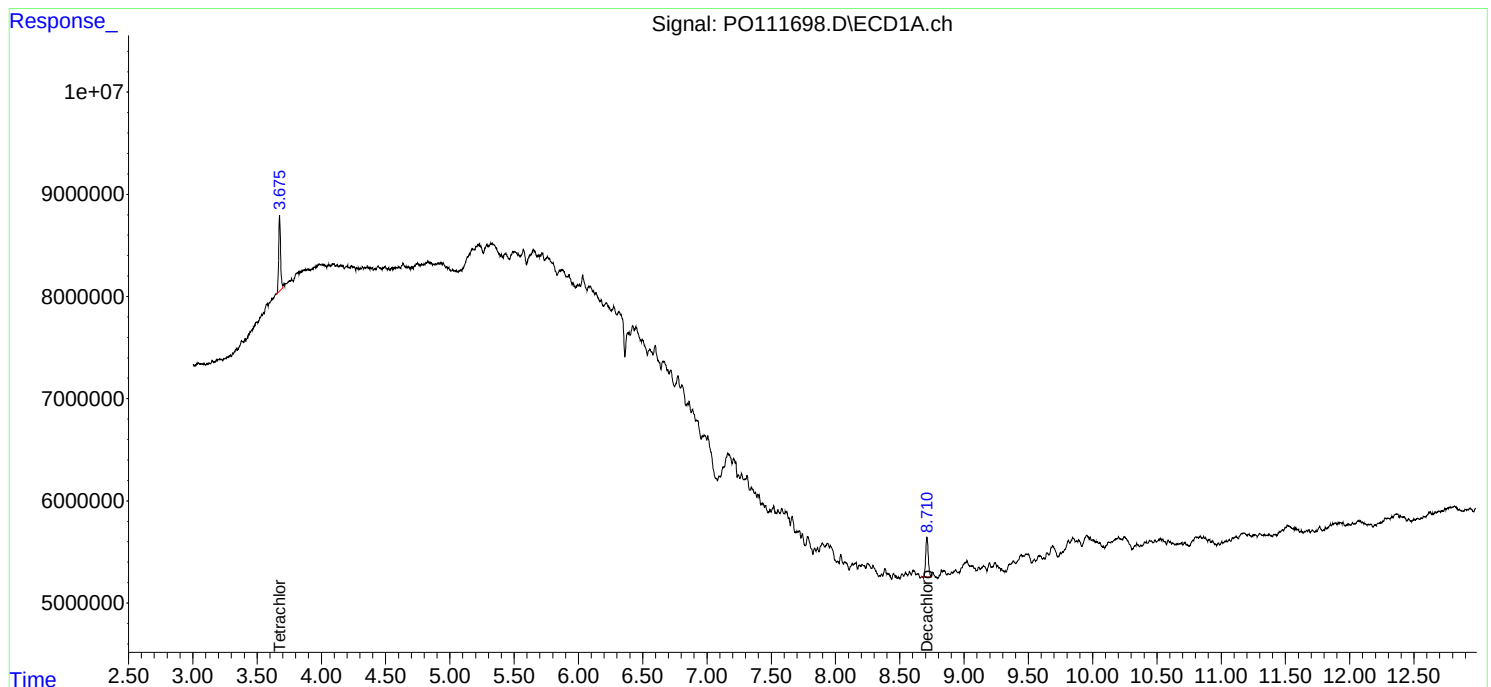

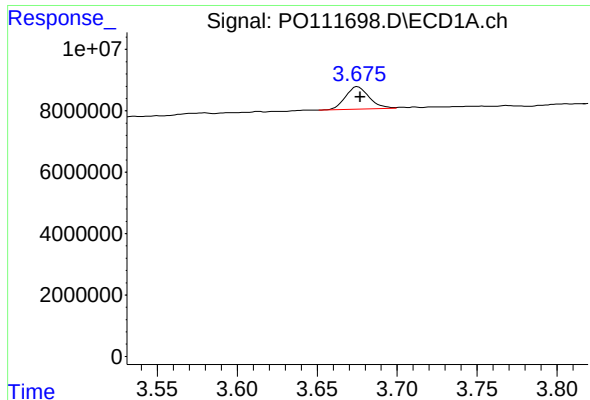


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.002 min
Response: 7565335
Conc: 1.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC271315-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/19/2025
Supervised By :mohammad ahmed 06/20/2025

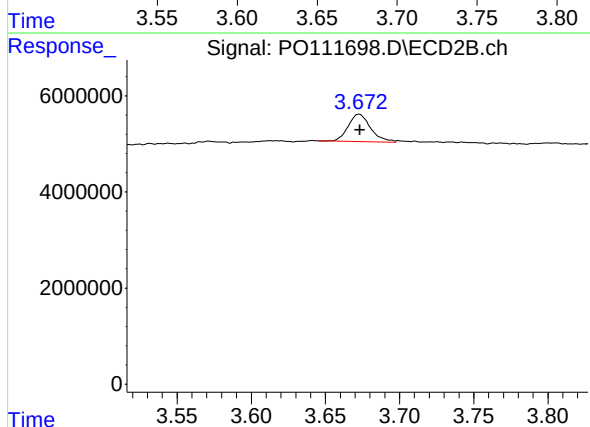


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 5980632
Conc: 1.06 ng/ml

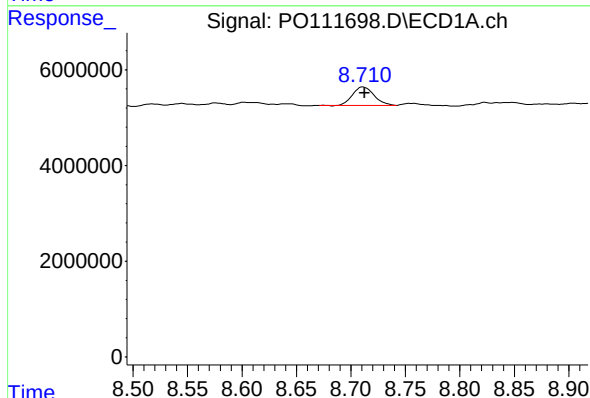

#2 Decachlorobiphenyl

R.T.: 8.711 min
Delta R.T.: -0.001 min
Response: 5324807
Conc: 1.01 ng/ml

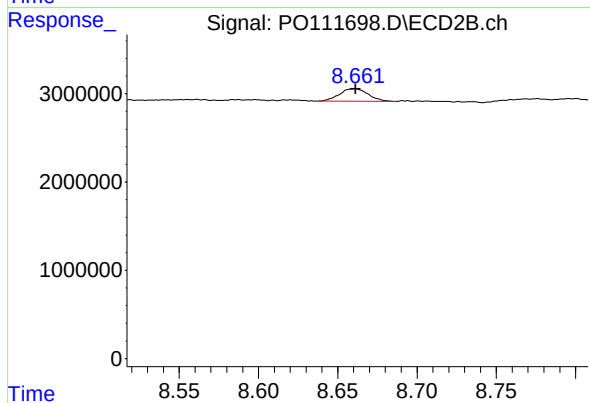

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: 0.000 min
Response: 1802531
Conc: 1.01 ng/ml m