

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061921\
 Data File : P0078913.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 18:42
 Operator : DD\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 05:02:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 19 04:53:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.329	3.606	412304	180126	5.092	5.605
2)	SA Decachlor...	9.938	8.787	342877	183057	5.781	6.110
Target Compounds							
16)	L4 AR-1242-1	5.626	4.832	110922	45120	56.232m	56.784
17)	L4 AR-1242-2	5.648	4.850	164472	60732	55.065m	52.274
18)	L4 AR-1242-3	5.711	5.038	104408	33646	56.382m	54.962
19)	L4 AR-1242-4	5.817	5.133	75817	30543	52.515	49.899
20)	L4 AR-1242-5	6.588	5.688	82646	44435	53.612m	56.825

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 Client Sample ID :
 AR1242ICC050

Manual Integrations
 APPROVED

Ankita
 6/21/2021 10:54:28 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061921\
Data File : PO078913.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 18:42
Operator : DD\AJ
Sample : AR1242IC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 05:02:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 19 04:53:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampled :
AR1242IC050

Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:28 AM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

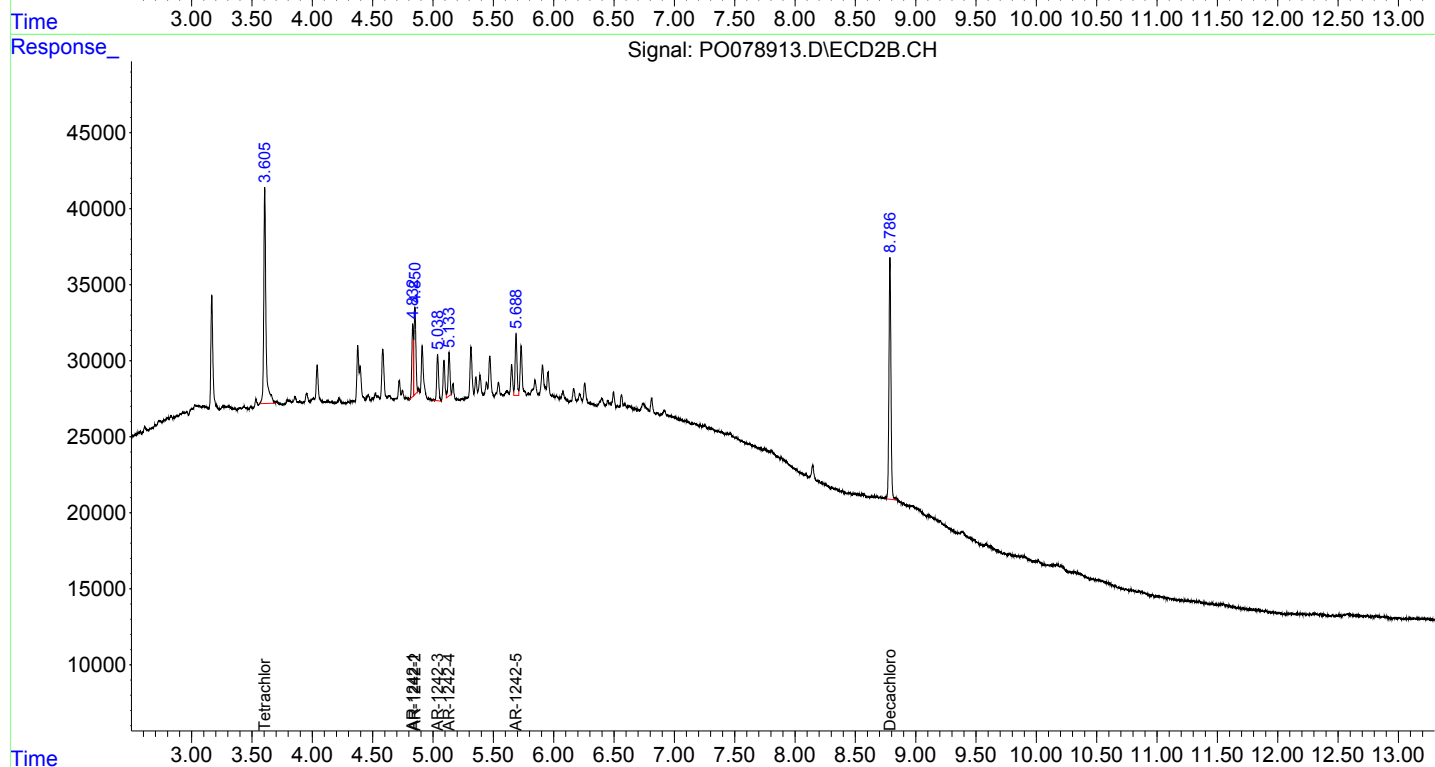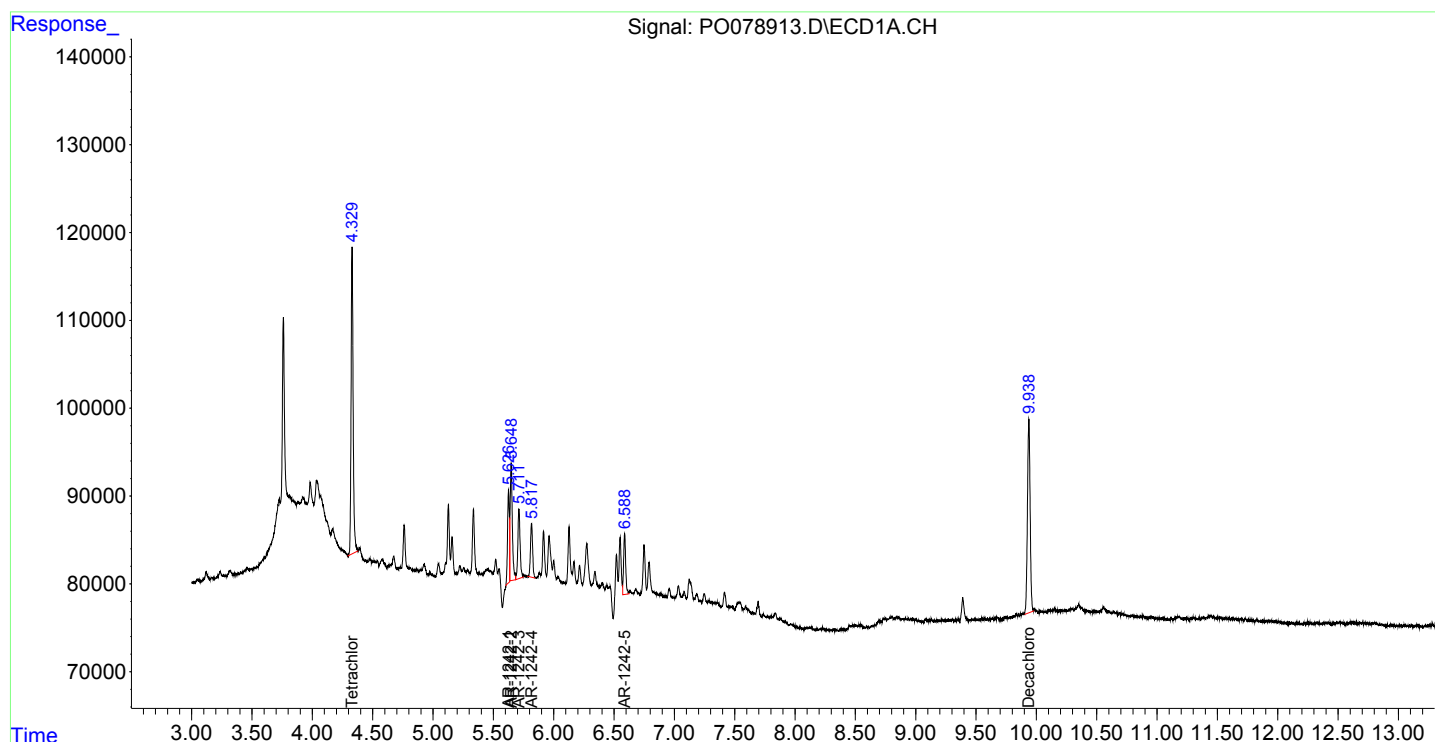

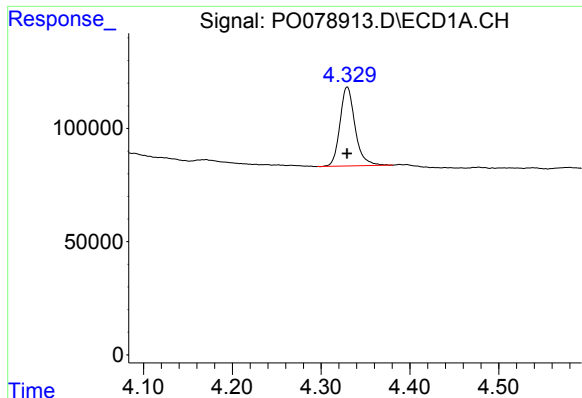


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: 0.000 min
Response: 412304
Conc: 5.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR12421CC050


Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:28 AM

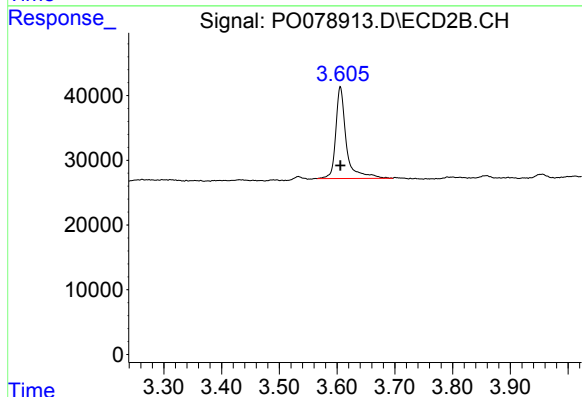


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 180126
Conc: 5.60 ng/ml

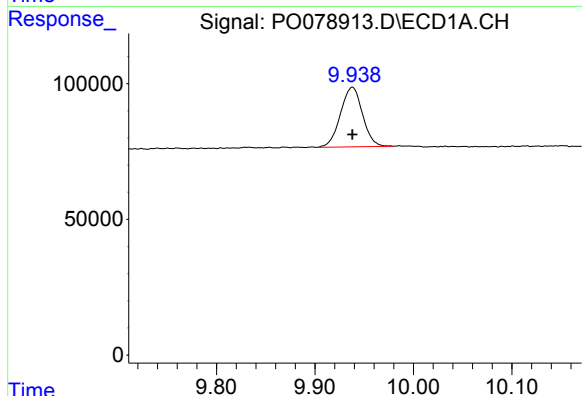


#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.000 min
Response: 342877
Conc: 5.78 ng/ml

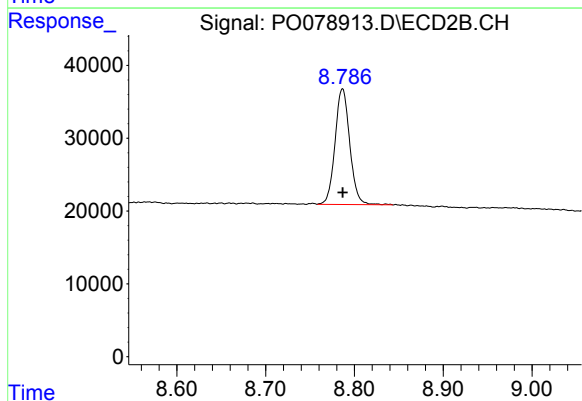

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 183057
Conc: 6.11 ng/ml

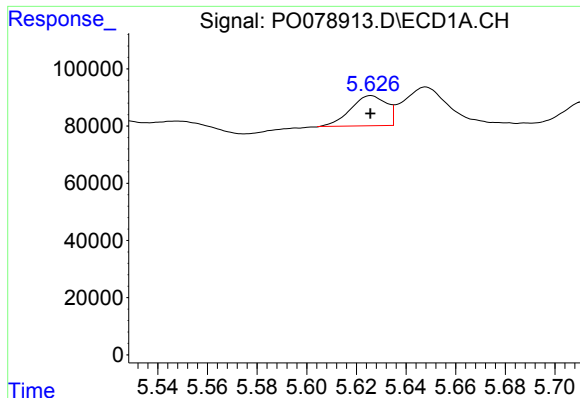


#16 AR-1242-1

R.T.: 5.626 min
Delta R.T.: 0.000 min
Response: 110922
Conc: 56.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:28 AM

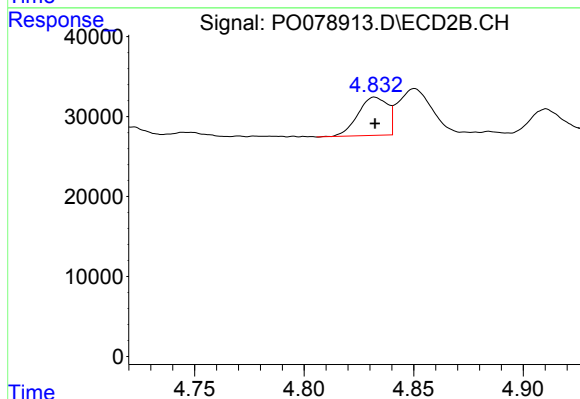


#16 AR-1242-1

R.T.: 4.832 min
Delta R.T.: 0.000 min
Response: 45120
Conc: 56.78 ng/ml

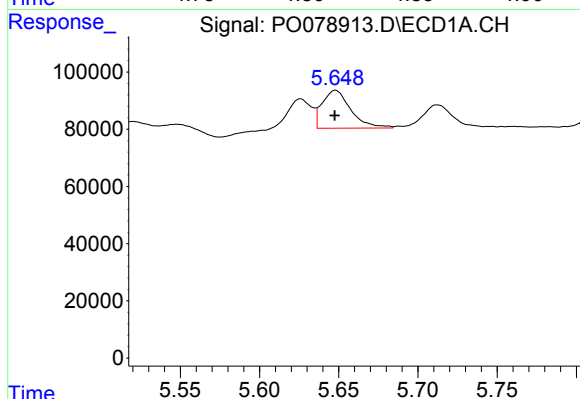


#17 AR-1242-2

R.T.: 5.648 min
Delta R.T.: 0.000 min
Response: 164472
Conc: 55.07 ng/ml m

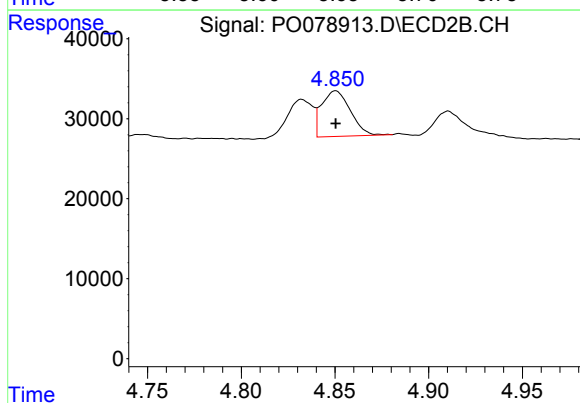

#17 AR-1242-2

R.T.: 4.850 min
Delta R.T.: 0.000 min
Response: 60732
Conc: 52.27 ng/ml

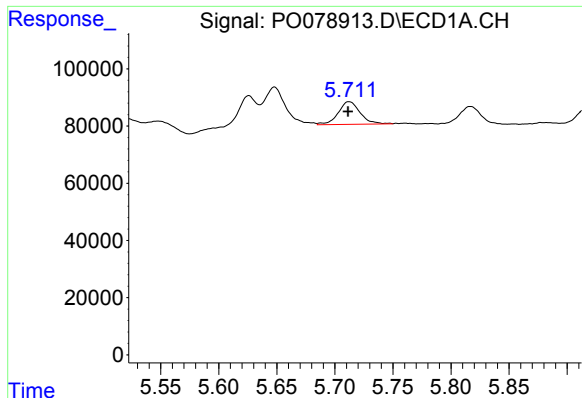


#18 AR-1242-3

R.T.: 5.711 min
Delta R.T.: 0.000 min
Response: 104408
Conc: 56.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:28 AM

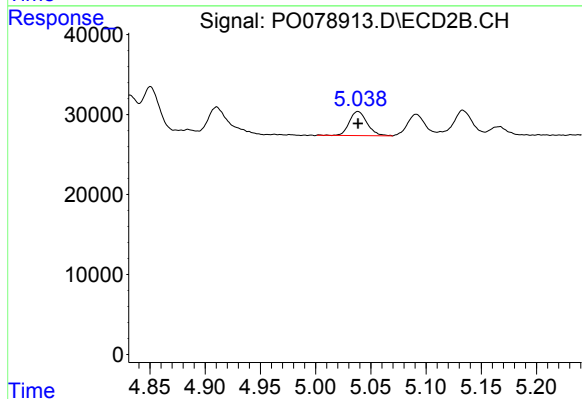


#18 AR-1242-3

R.T.: 5.038 min
Delta R.T.: 0.000 min
Response: 33646
Conc: 54.96 ng/ml

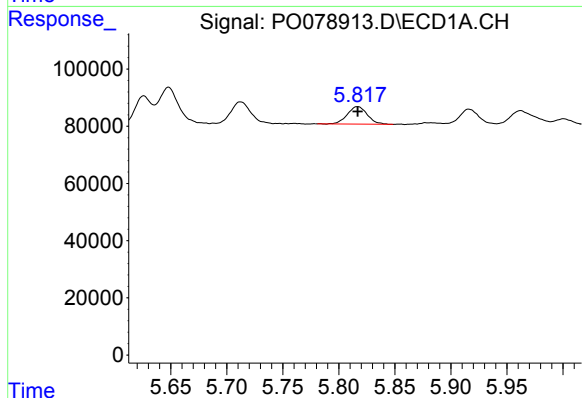


#19 AR-1242-4

R.T.: 5.817 min
Delta R.T.: 0.000 min
Response: 75817
Conc: 52.51 ng/ml

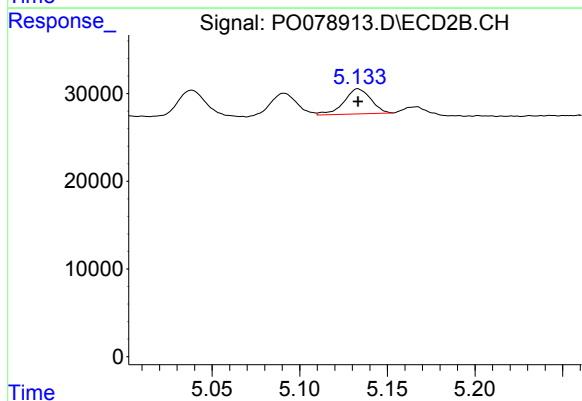


#19 AR-1242-4

R.T.: 5.133 min
Delta R.T.: 0.000 min
Response: 30543
Conc: 49.90 ng/ml

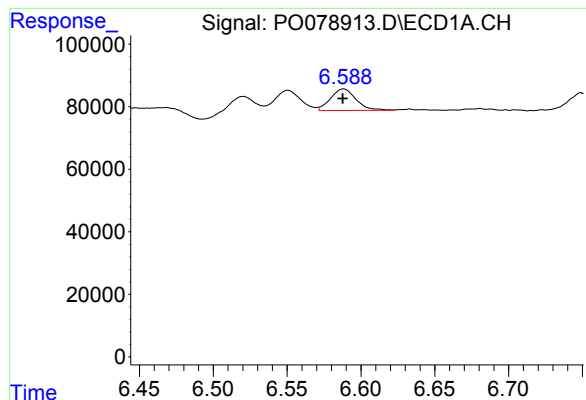

#20 AR-1242-5

R.T.: 6.588 min
Delta R.T.: 0.000 min
Response: 82646
Conc: 53.61 ng/ml m

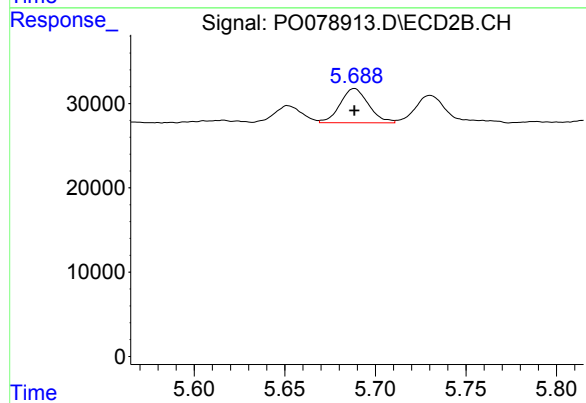

#20 AR-1242-5

R.T.: 5.688 min
Delta R.T.: 0.000 min
Response: 44435
Conc: 56.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR12421CC050

Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:28 AM