

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061921\
 Data File : P0078923.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 21:34
 Operator : DD\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 05:46:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 19 05:36:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.605	347503	146910	4.349	4.740
2) SA Decachlor...	9.935	8.786	298784	156482	5.196	5.351
Target Compounds						
26) L6 AR-1254-1	6.518	5.687	126555	86487	46.951m	52.057
27) L6 AR-1254-2	6.746	5.845	209046	77595	49.839	52.653
28) L6 AR-1254-3	7.122	6.257	231163	111465	51.905	50.114
29) L6 AR-1254-4	7.415	6.495	146846	68699	47.724	50.526
30) L6 AR-1254-5	7.838	6.917	146394	98256	44.846	49.346

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 6/21/2021 10:54:29 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061921\
Data File : P0078923.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 21:34
Operator : DD\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 05:46:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 19 05:36:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:29 AM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

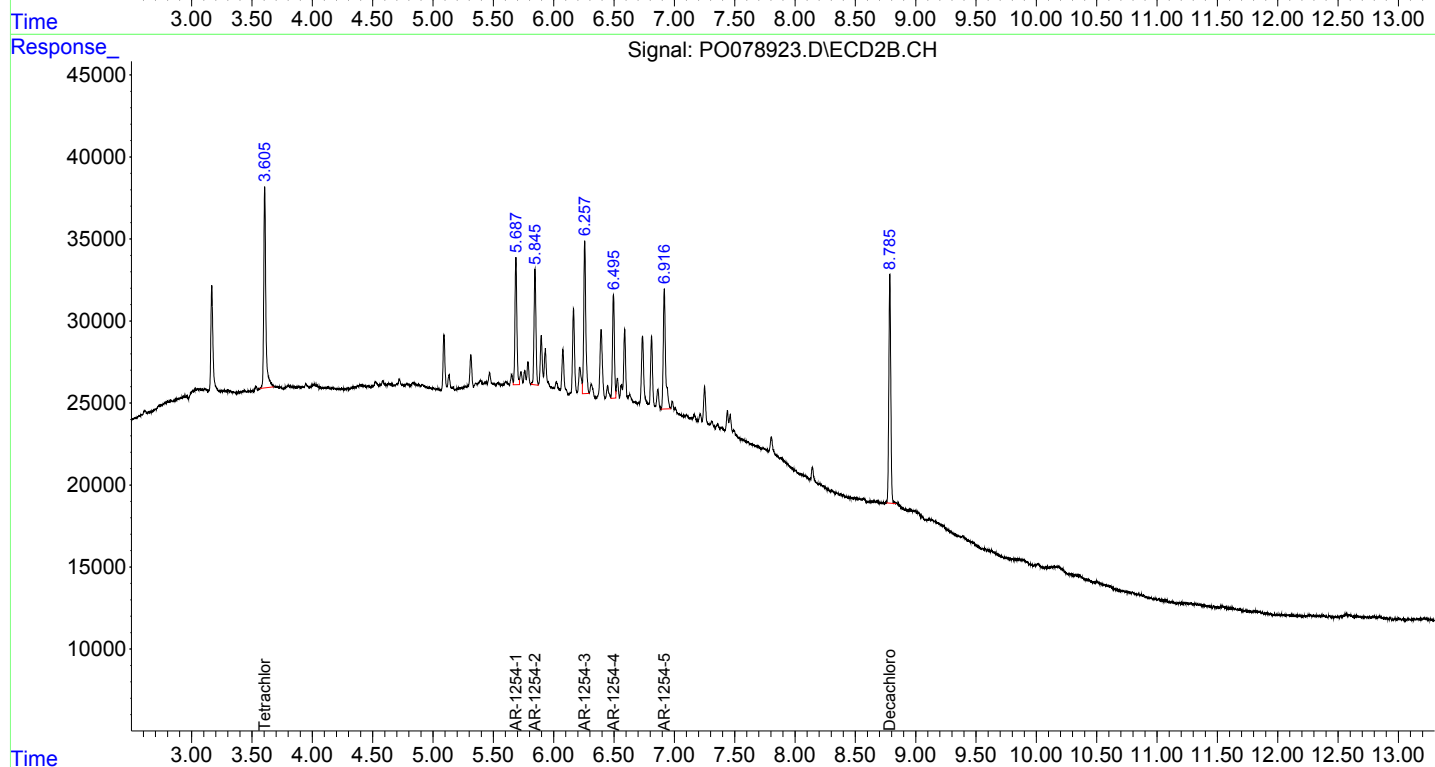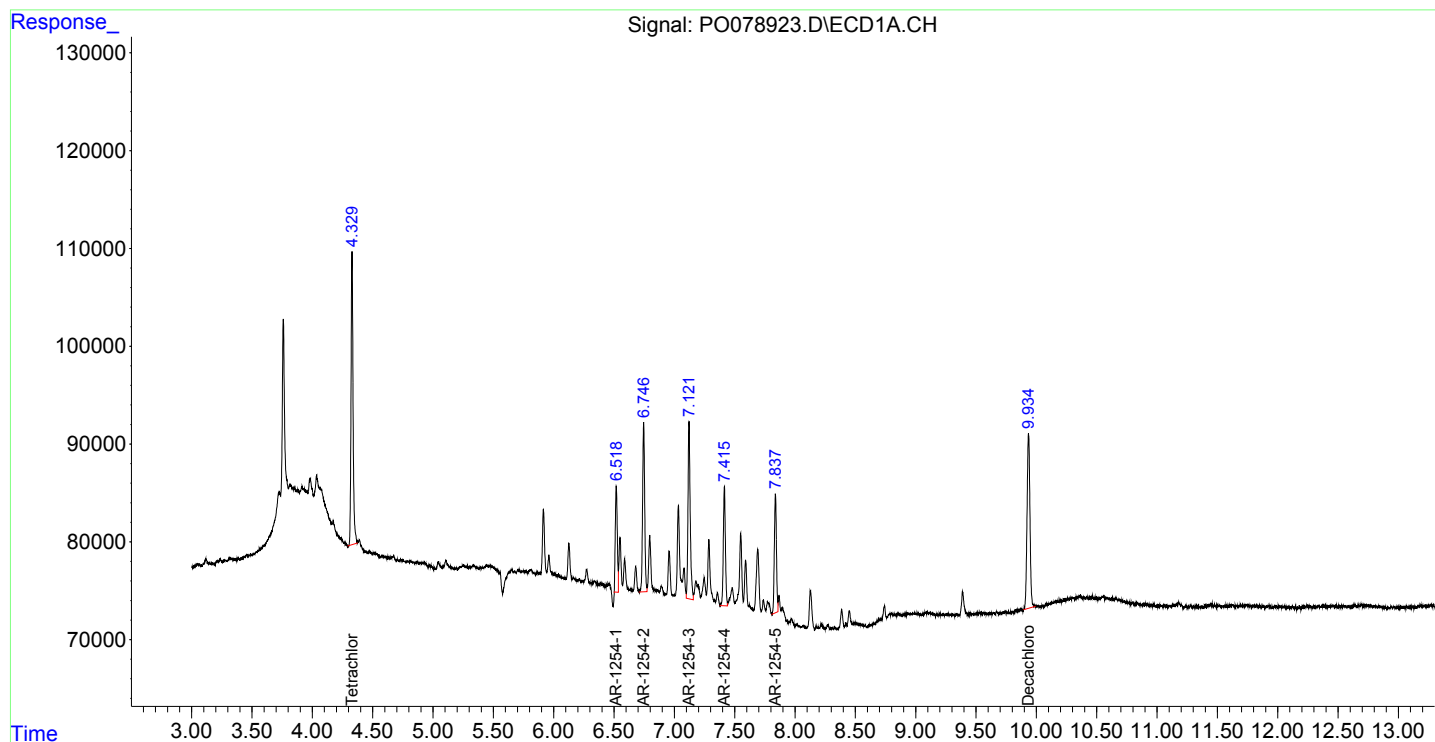

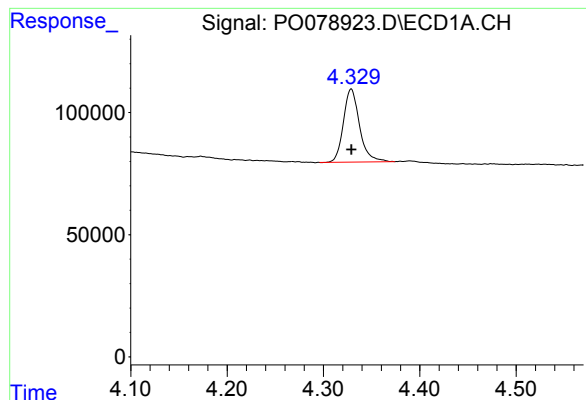


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: 0.000 min
Response: 347503
Conc: 4.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:29 AM

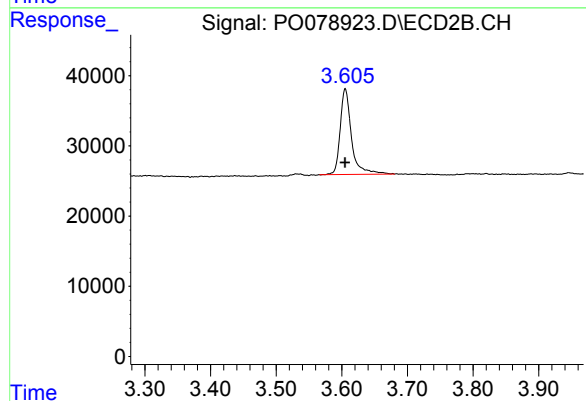


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 146910
Conc: 4.74 ng/ml

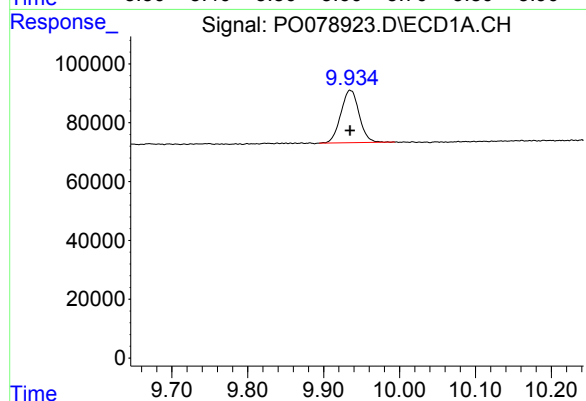


#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: 0.000 min
Response: 298784
Conc: 5.20 ng/ml

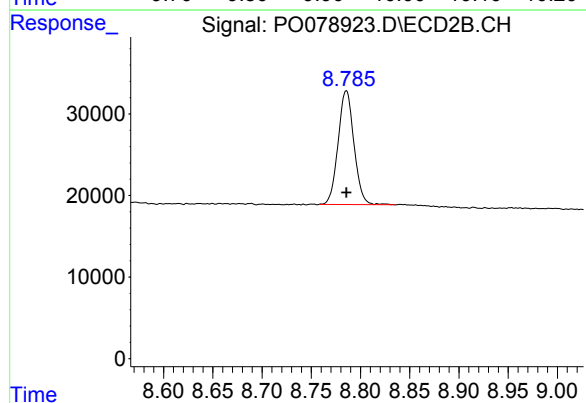

#2 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 156482
Conc: 5.35 ng/ml

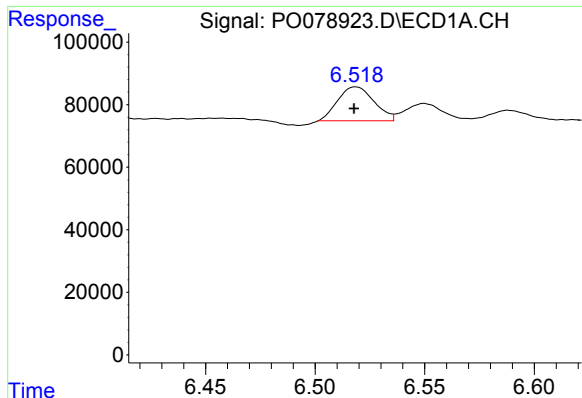


#26 AR-1254-1

R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 126555
Conc: 46.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:29 AM

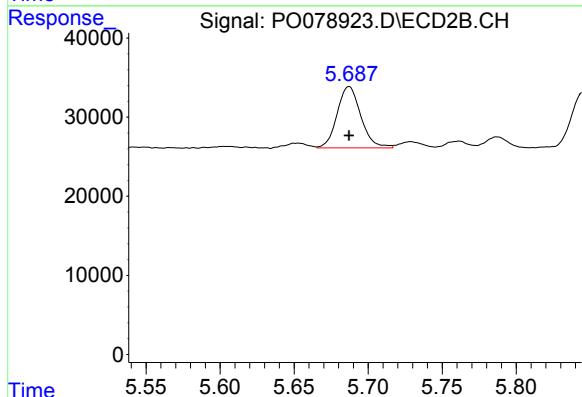


#26 AR-1254-1

R.T.: 5.687 min
Delta R.T.: 0.000 min
Response: 86487
Conc: 52.06 ng/ml

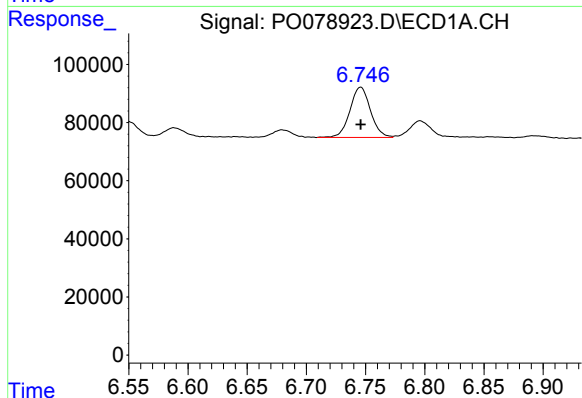


#27 AR-1254-2

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 209046
Conc: 49.84 ng/ml

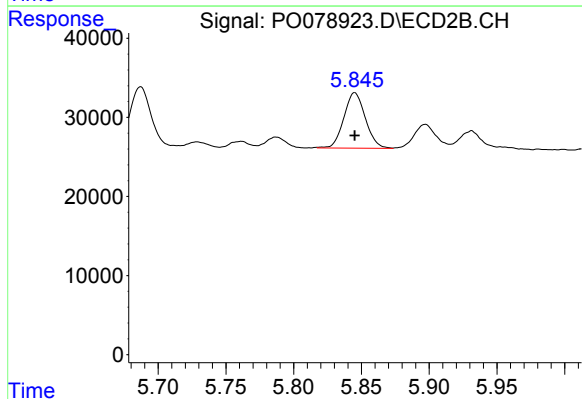

#27 AR-1254-2

R.T.: 5.845 min
Delta R.T.: 0.000 min
Response: 77595
Conc: 52.65 ng/ml

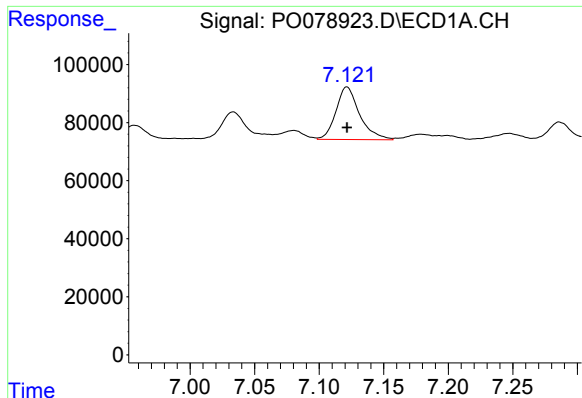


#28 AR-1254-3

R.T.: 7.122 min
Delta R.T.: 0.000 min
Response: 231163
Conc: 51.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:29 AM

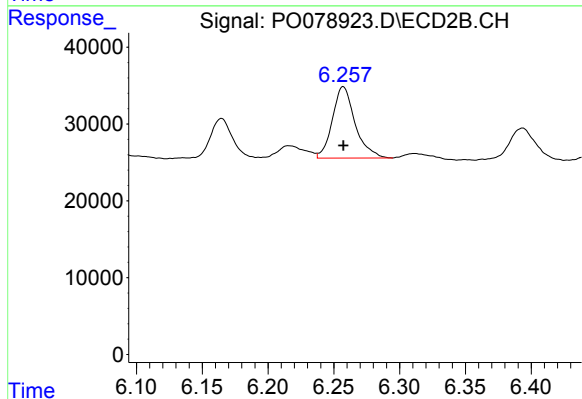


#28 AR-1254-3

R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 111465
Conc: 50.11 ng/ml

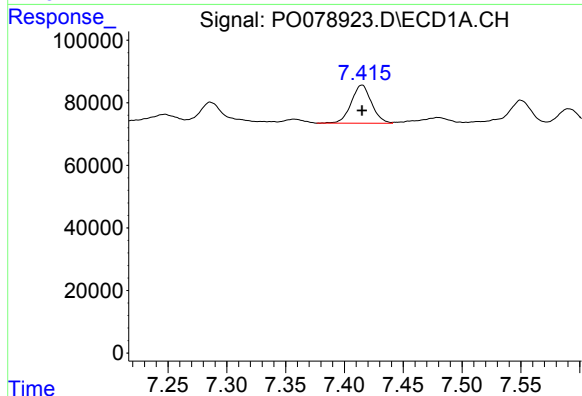


#29 AR-1254-4

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 146846
Conc: 47.72 ng/ml

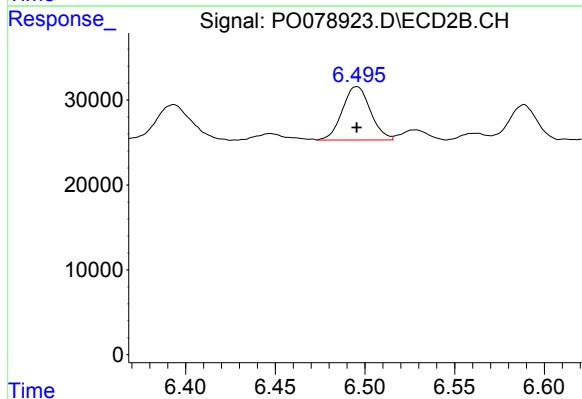


#29 AR-1254-4

R.T.: 6.495 min
Delta R.T.: 0.000 min
Response: 68699
Conc: 50.53 ng/ml

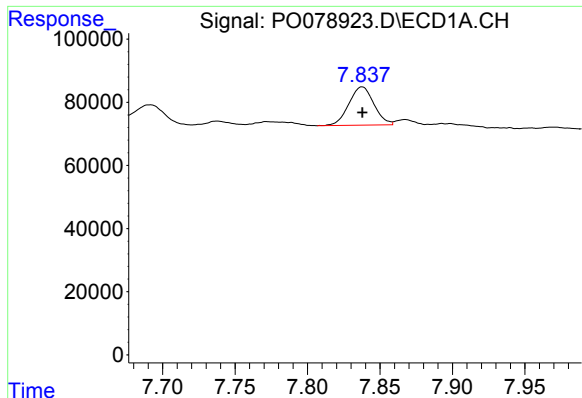

#30 AR-1254-5

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 146394
Conc: 44.85 ng/ml

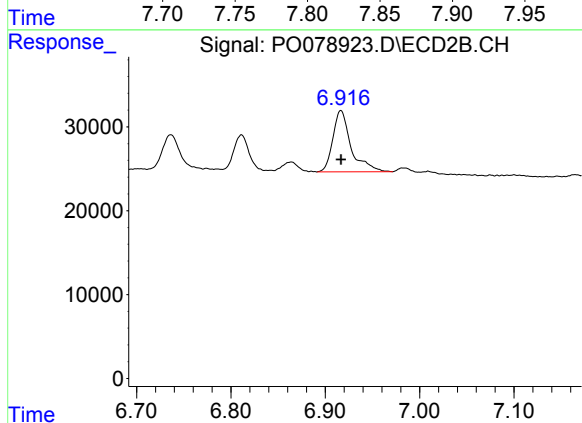

#30 AR-1254-5

R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 98256
Conc: 49.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
6/21/2021 10:54:29 AM