

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061923\
 Data File : P0095793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 14:15
 Operator : YP/AJ
 Sample : 03288-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAT-2-061523

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/20/2023
 Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:45:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 19 09:21:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.431	3.638	73140334	32663561	32.836	25.272
2) SA Decachlor...	10.306	8.679	18666171	26243349	28.972	26.004
Target Compounds						
31) L7 AR-1260-1	7.242	6.220	3103768	3670805	82.994	56.810 #
32) L7 AR-1260-2	7.491	6.410	4672673	3153912	110.520	42.282 #
33) L7 AR-1260-3	7.787	6.564	2890207	2575488	54.872	36.525 #
34) L7 AR-1260-4	8.094	7.038	1399481	1982016	37.149m	39.370
35) L7 AR-1260-5	8.422	7.281	2958649	4544780	48.937	39.813

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061923\
Data File : PO095793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 14:15
Operator : YP/AJ
Sample : 03288-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAT-2-061523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:45:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 19 09:21:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

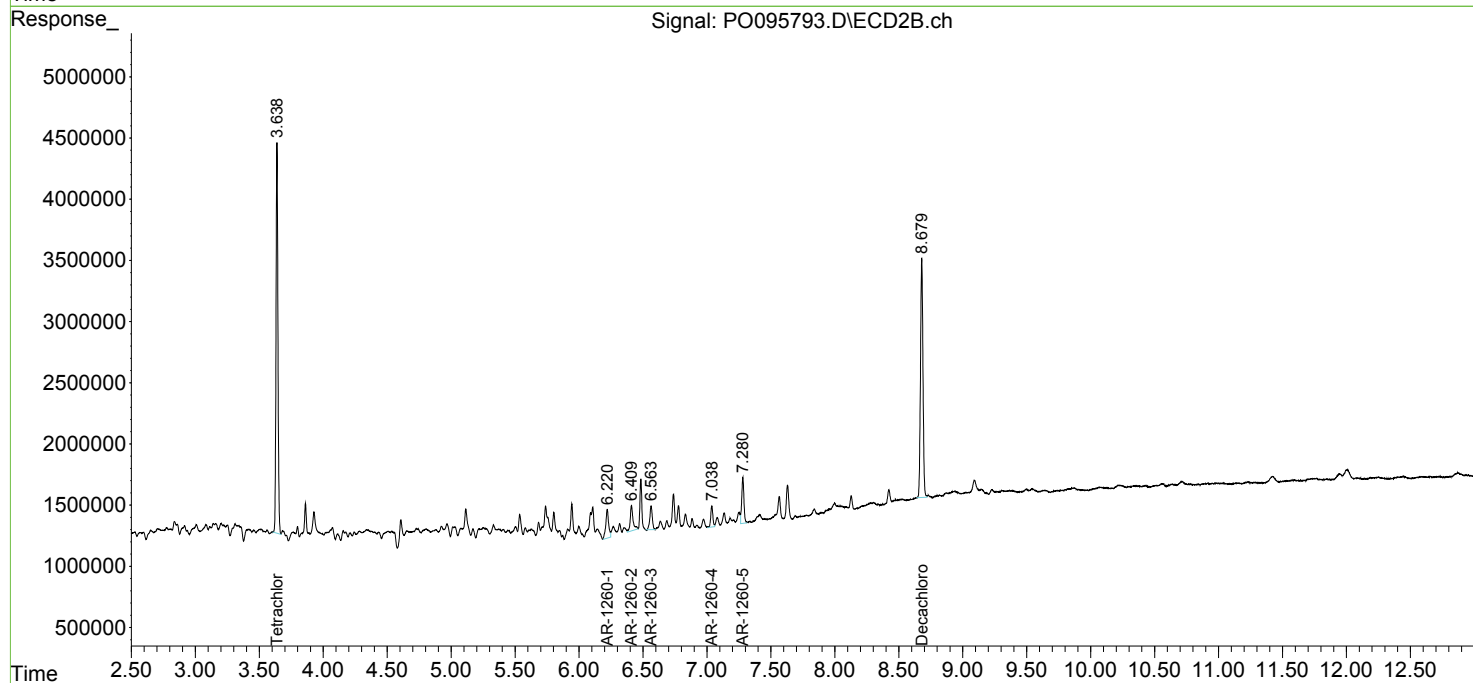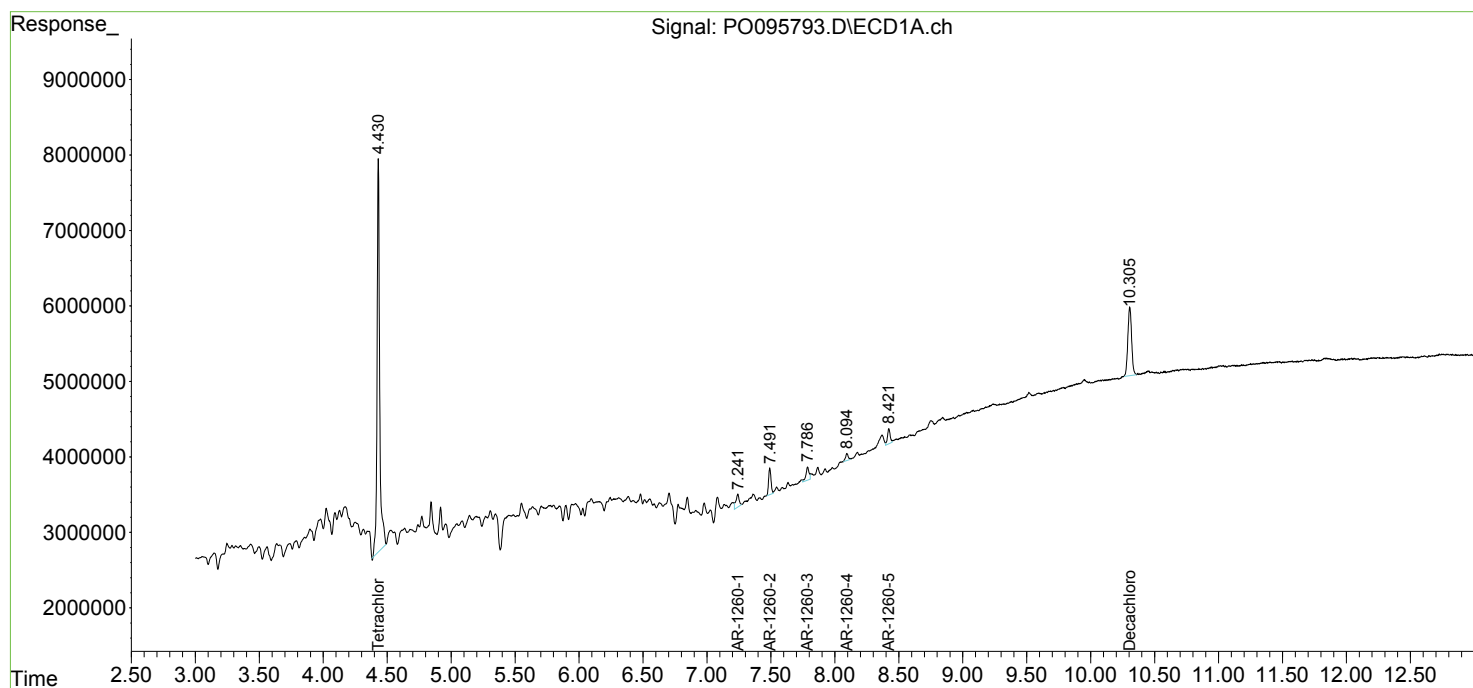

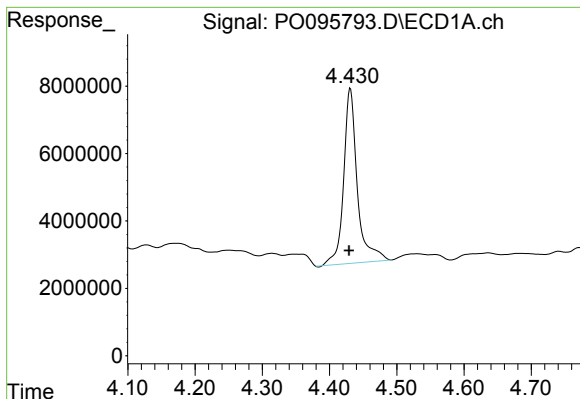


#1 Tetrachloro-m-xylene

R.T.: 4.431 min
Delta R.T.: 0.002 min
Response: 73140334
Conc: 32.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAT-2-061523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

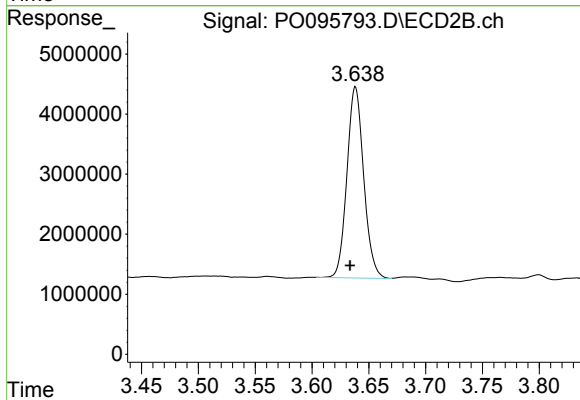


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.005 min
Response: 32663561
Conc: 25.27 ng/ml

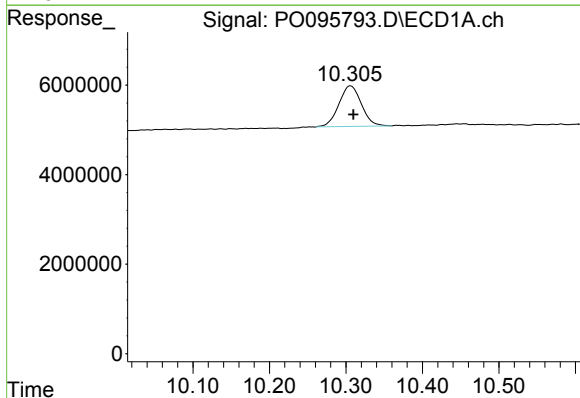


#2 Decachlorobiphenyl

R.T.: 10.306 min
Delta R.T.: -0.004 min
Response: 18666171
Conc: 28.97 ng/ml

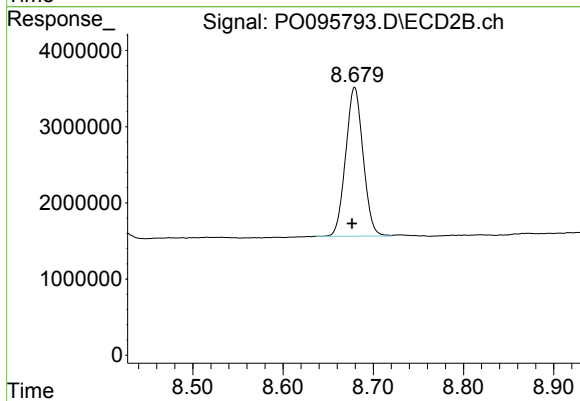

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: 0.003 min
Response: 26243349
Conc: 26.00 ng/ml

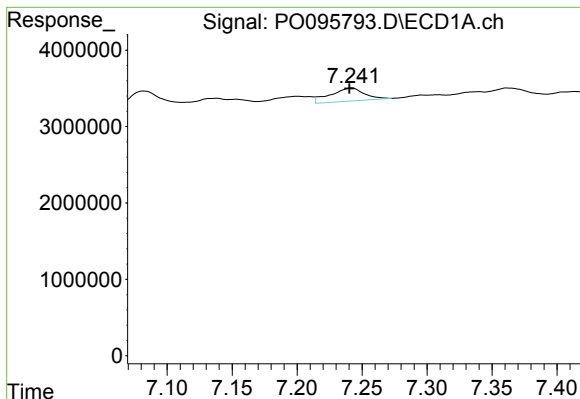


#31 AR-1260-1

R.T.: 7.242 min
Delta R.T.: 0.002 min
Response: 3103768
Conc: 82.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAT-2-061523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

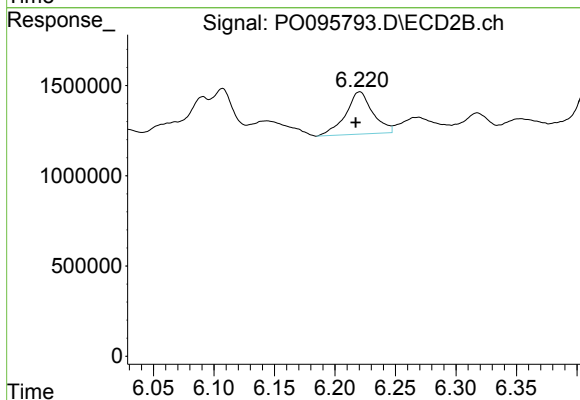


#31 AR-1260-1

R.T.: 6.220 min
Delta R.T.: 0.003 min
Response: 3670805
Conc: 56.81 ng/ml

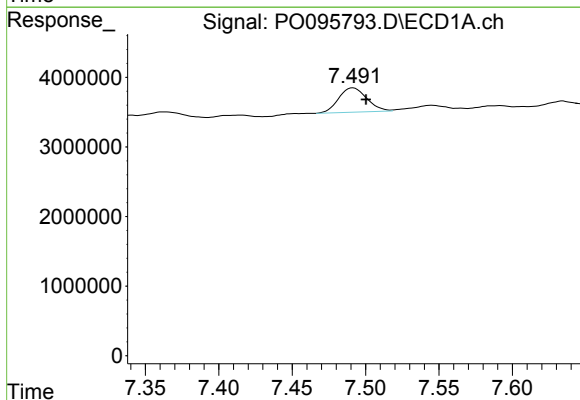


#32 AR-1260-2

R.T.: 7.491 min
Delta R.T.: -0.009 min
Response: 4672673
Conc: 110.52 ng/ml

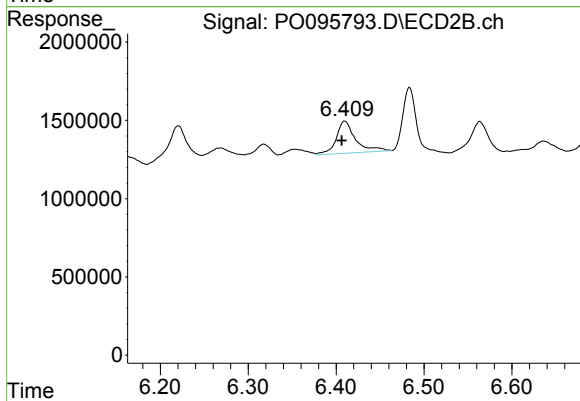

#32 AR-1260-2

R.T.: 6.410 min
Delta R.T.: 0.003 min
Response: 3153912
Conc: 42.28 ng/ml

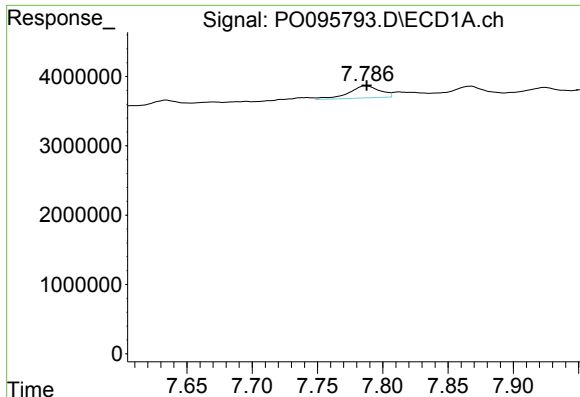


#33 AR-1260-3

R.T.: 7.787 min
Delta R.T.: 0.000 min
Response: 2890207
Conc: 54.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAT-2-061523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

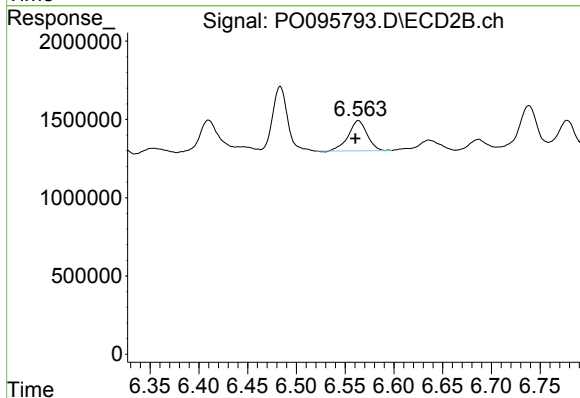


#33 AR-1260-3

R.T.: 6.564 min
Delta R.T.: 0.003 min
Response: 2575488
Conc: 36.52 ng/ml

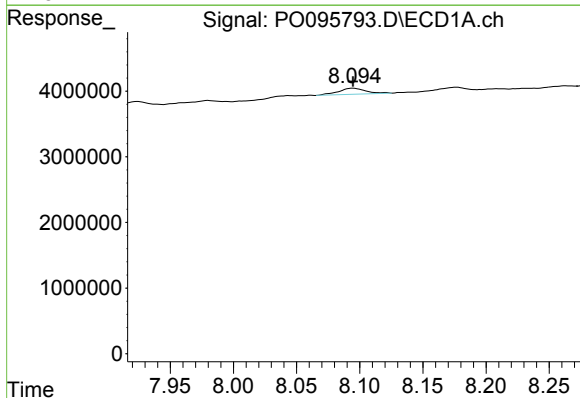


#34 AR-1260-4

R.T.: 8.094 min
Delta R.T.: 0.000 min
Response: 1399481
Conc: 37.15 ng/ml m

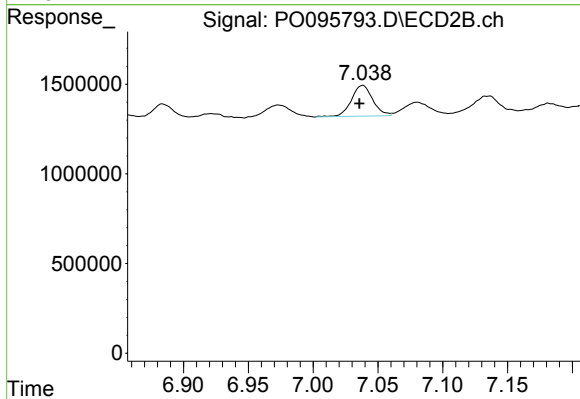

#34 AR-1260-4

R.T.: 7.038 min
Delta R.T.: 0.003 min
Response: 1982016
Conc: 39.37 ng/ml

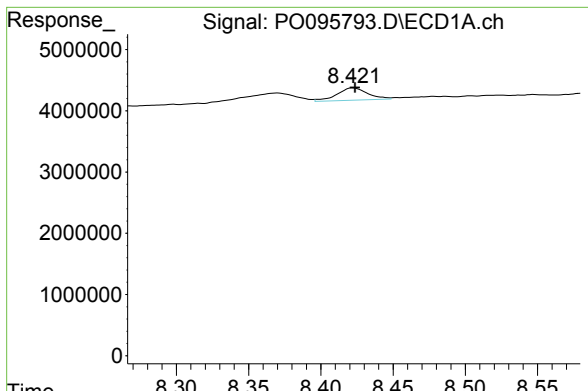


#35 AR-1260-5

R.T.: 8.422 min
Delta R.T.: -0.001 min
Response: 2958649
Conc: 48.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAT-2-061523

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

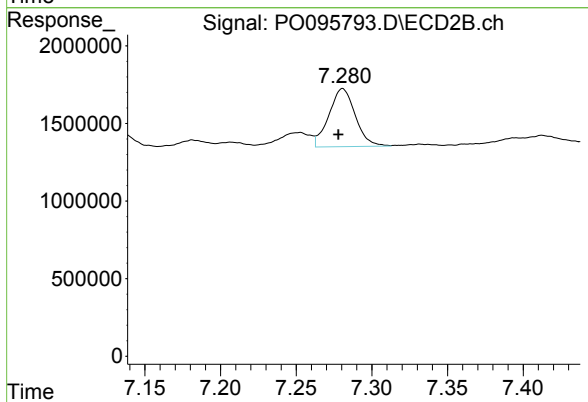

#35 AR-1260-5

R.T.: 7.281 min
Delta R.T.: 0.003 min
Response: 4544780
Conc: 39.81 ng/ml