

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061925\
 Data File : P0111721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 10:13
 Operator : YP/AJ
 Sample : Q2321-02RE 10X (Sig #1); Q2321-02 10X (Sig #2)
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 34880

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/20/2025
 Supervised By :mohammad ahmed 06/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 11:55:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.679	3.674	3298213	1603447	0.573m	0.285 #
2) SA Decachlor...	8.715	8.664	1551325	1086730	0.296m	0.611m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061925\
Data File : PO111721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 10:13
Operator : YP/AJ
Sample : Q2321-02RE 10X (Sig #1); Q2321-02 10X (Sig #2)
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
34880


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2025
Supervised By :mohammad ahmed 06/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 11:55:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

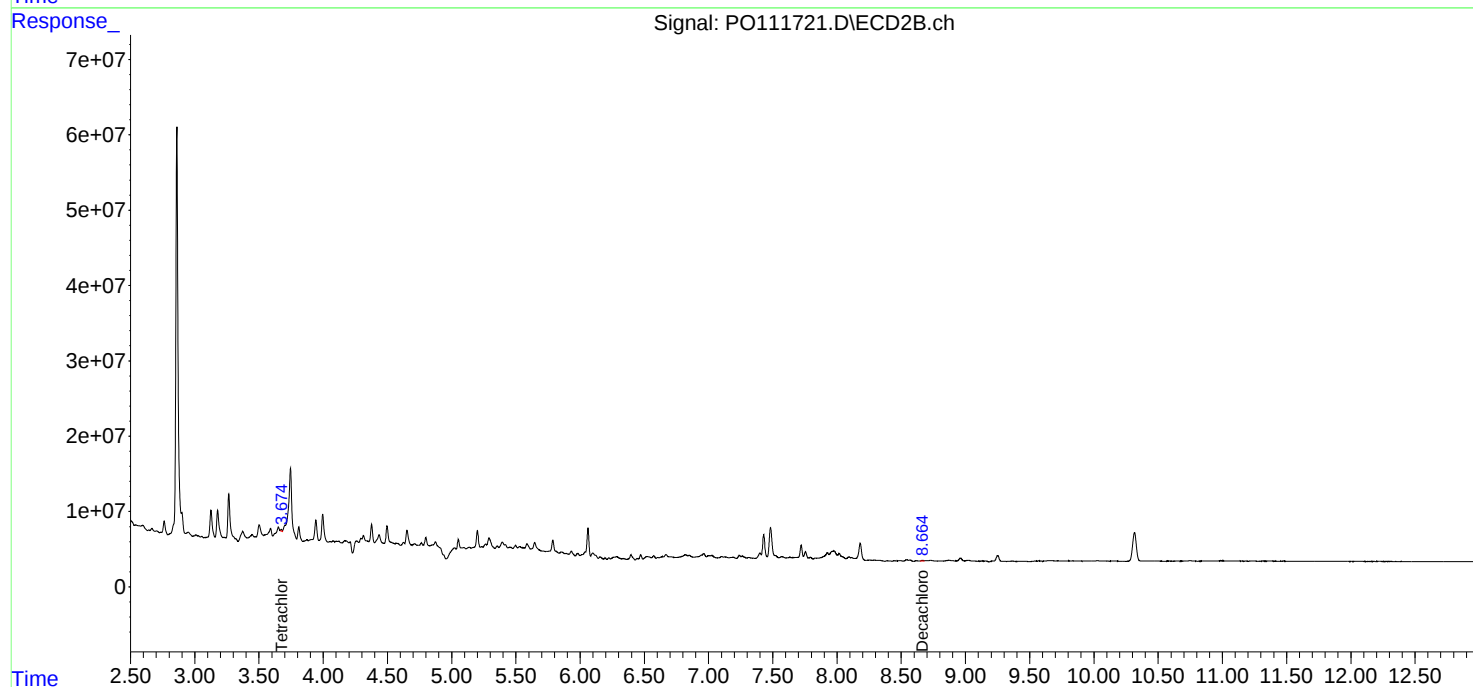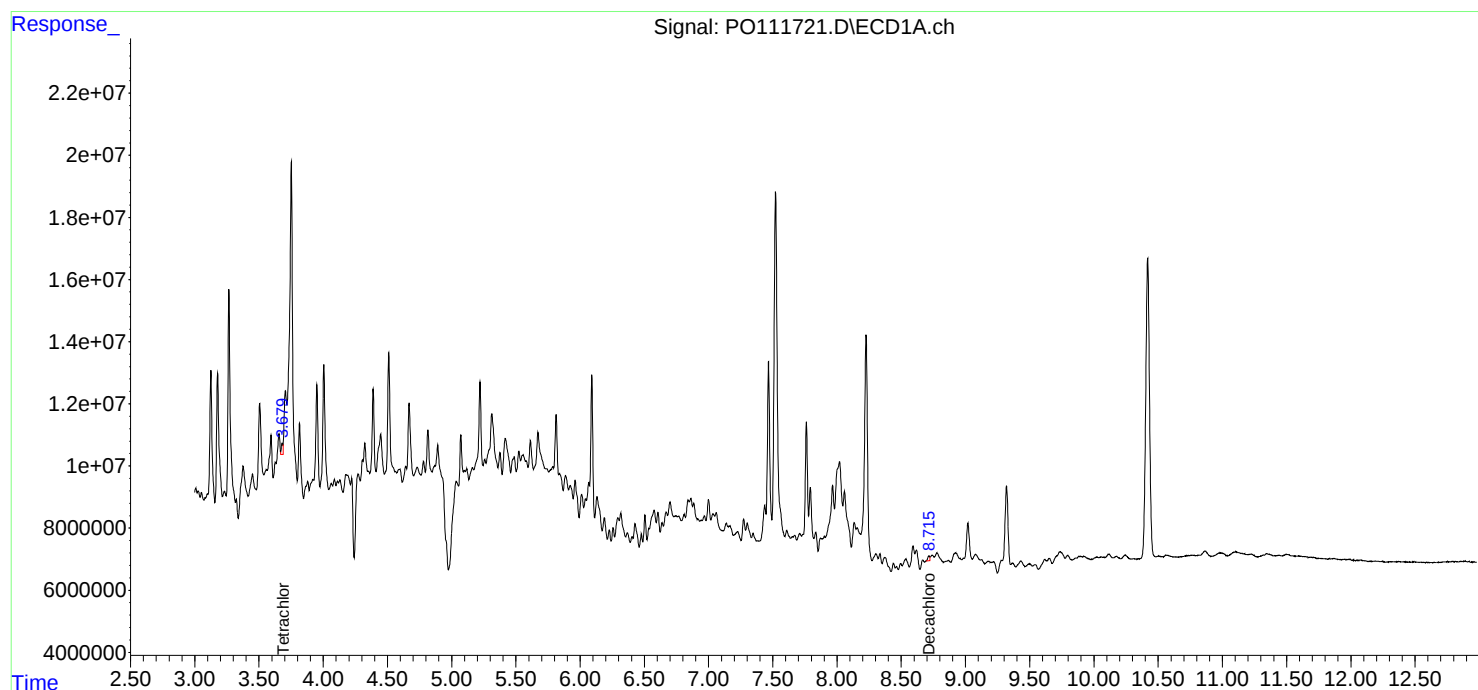

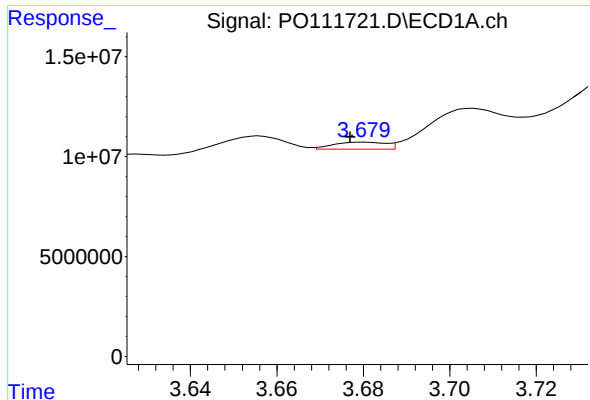


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: 0.002 min
Response: 3298213
Conc: 0.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
34880

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2025
Supervised By :mohammad ahmed 06/23/2025

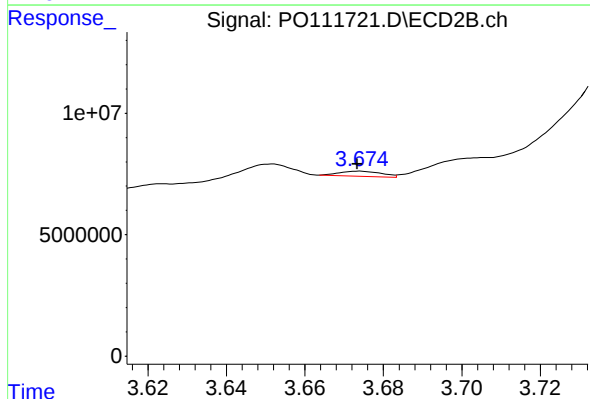

#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: 0.000 min
Response: 1603447
Conc: 0.29 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.715 min
Delta R.T.: 0.003 min
Response: 1551325
Conc: 0.30 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: 0.003 min
Response: 1086730
Conc: 0.61 ng/ml m