

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061925\
 Data File : P0111724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 13:40
 Operator : YP/AJ
 Sample : Q2357-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-06-06182025

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2025
 Supervised By :mohammad ahmed 06/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 18:39:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.676	3.672	104.3E6	88701423	18.111m	15.791m
2) SA Decachlor...	8.713	8.660	61637573	23669116	11.742	13.315

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061925\
Data File : PO111724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 13:40
Operator : YP/AJ
Sample : Q2357-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-06-06182025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2025
Supervised By :mohammad ahmed 06/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 18:39:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

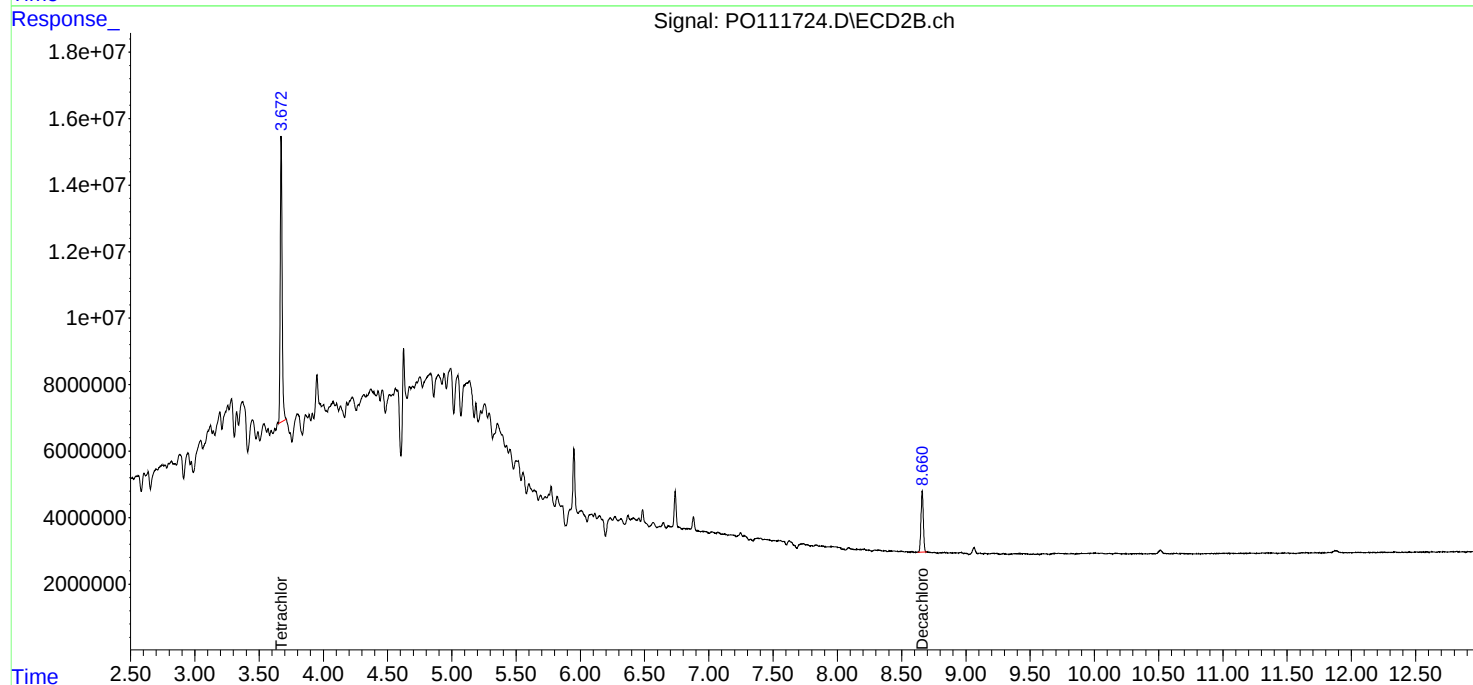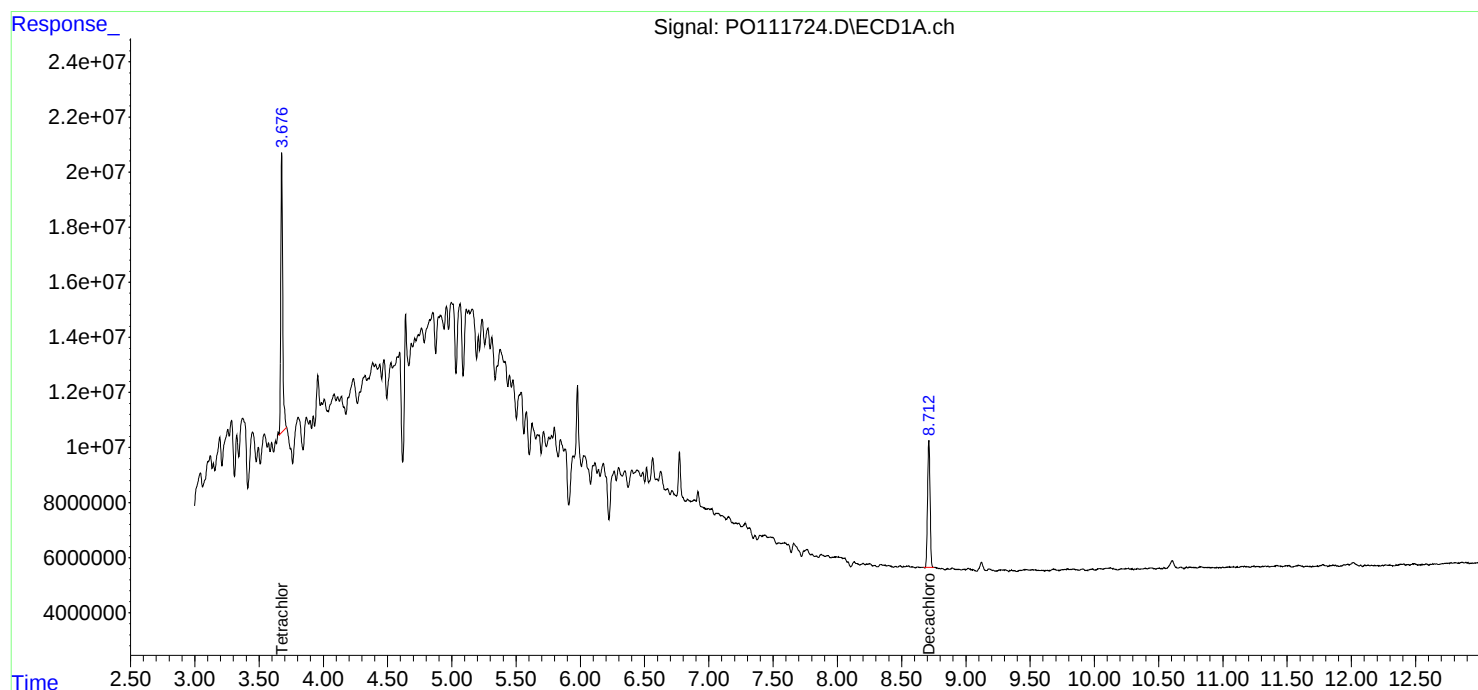

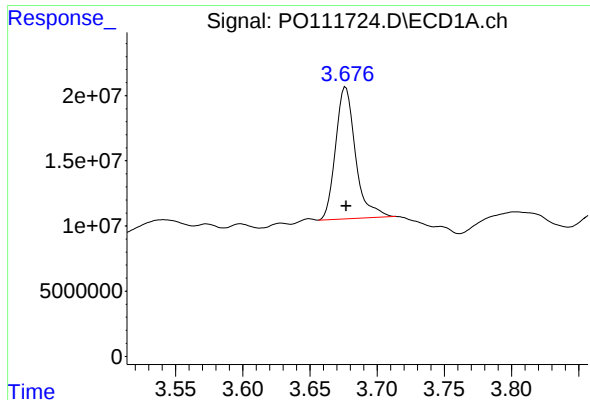


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: -0.001 min
Response: 104309915
Conc: 18.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-06-06182025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2025
Supervised By :mohammad ahmed 06/23/2025

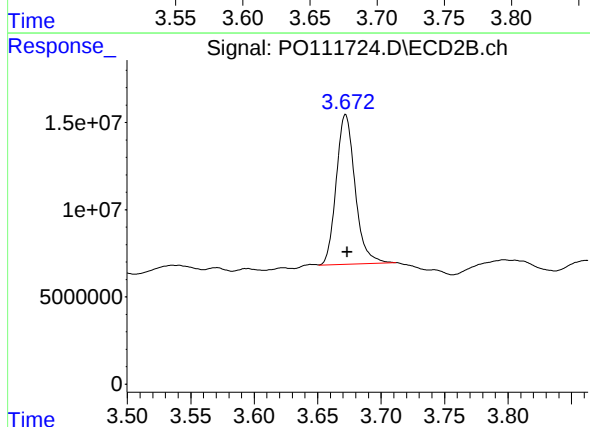


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.002 min
Response: 88701423
Conc: 15.79 ng/ml

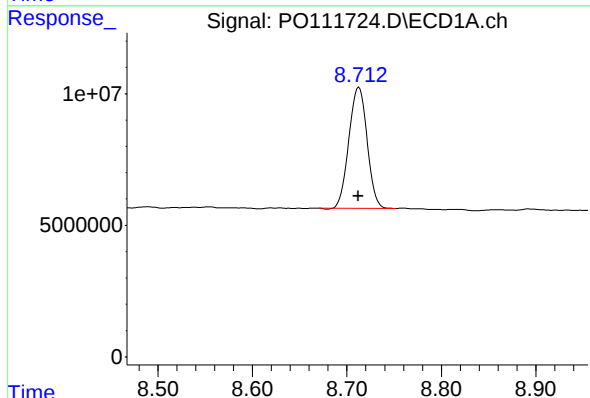

#2 Decachlorobiphenyl

R.T.: 8.713 min
Delta R.T.: 0.000 min
Response: 61637573
Conc: 11.74 ng/ml

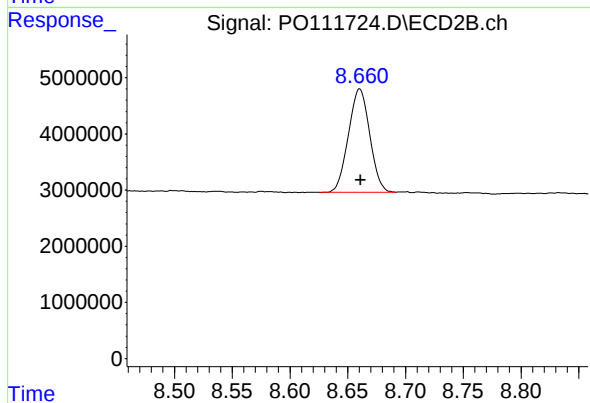

#2 Decachlorobiphenyl

R.T.: 8.660 min
Delta R.T.: 0.000 min
Response: 23669116
Conc: 13.31 ng/ml