

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062019\
 Data File : P0057297.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 10:36
 Operator : SM/SJ
 Sample : K3157-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-061719-A

Manual Integrations
 APPROVED

Ankita
 6/21/2019 3:28:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 10:56:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.234	3.559	1220692	1068786	31.886m	32.409
2) SA Decachlor...	9.791	8.484	1319814	810632	26.889m	22.734

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062019\
Data File : PO057297.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 10:36
Operator : SM/SJ
Sample : K3157-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-061719-A


Manual Integrations
APPROVED

Ankita
6/21/2019 3:28:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 10:56:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

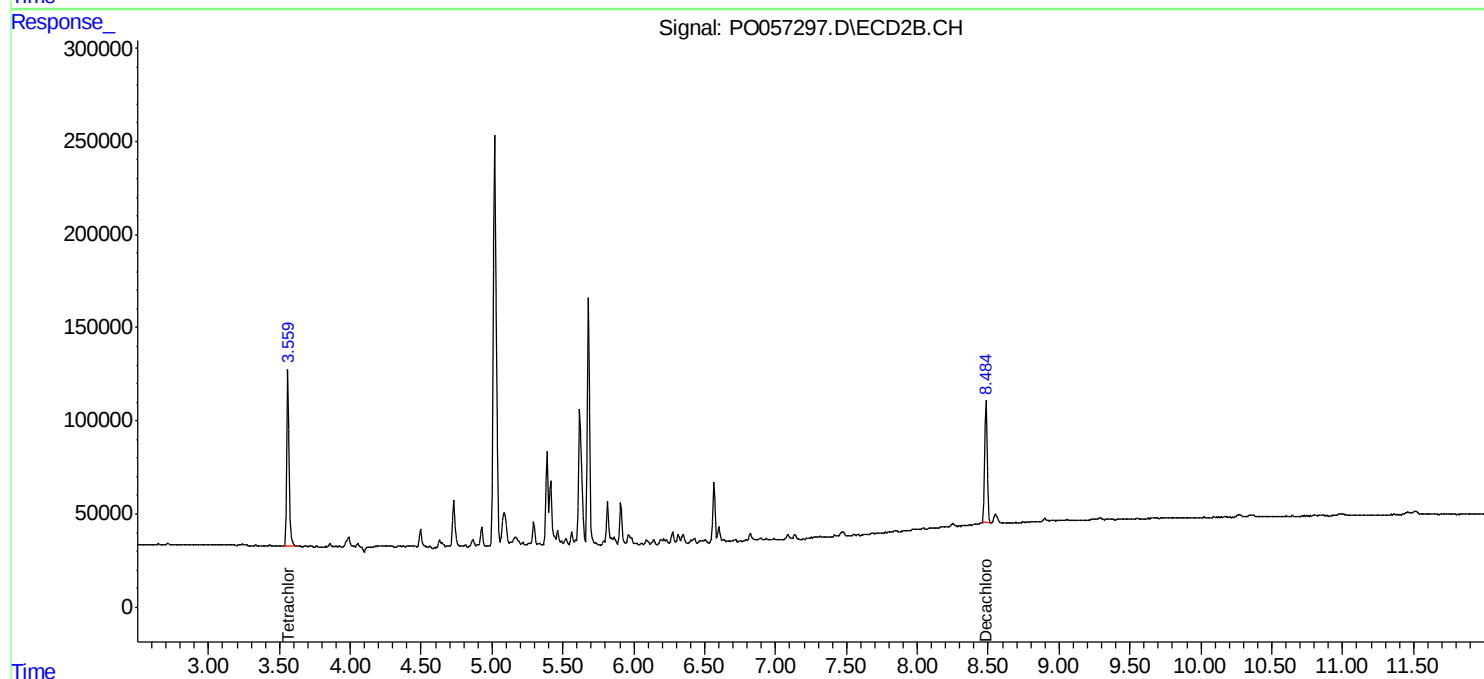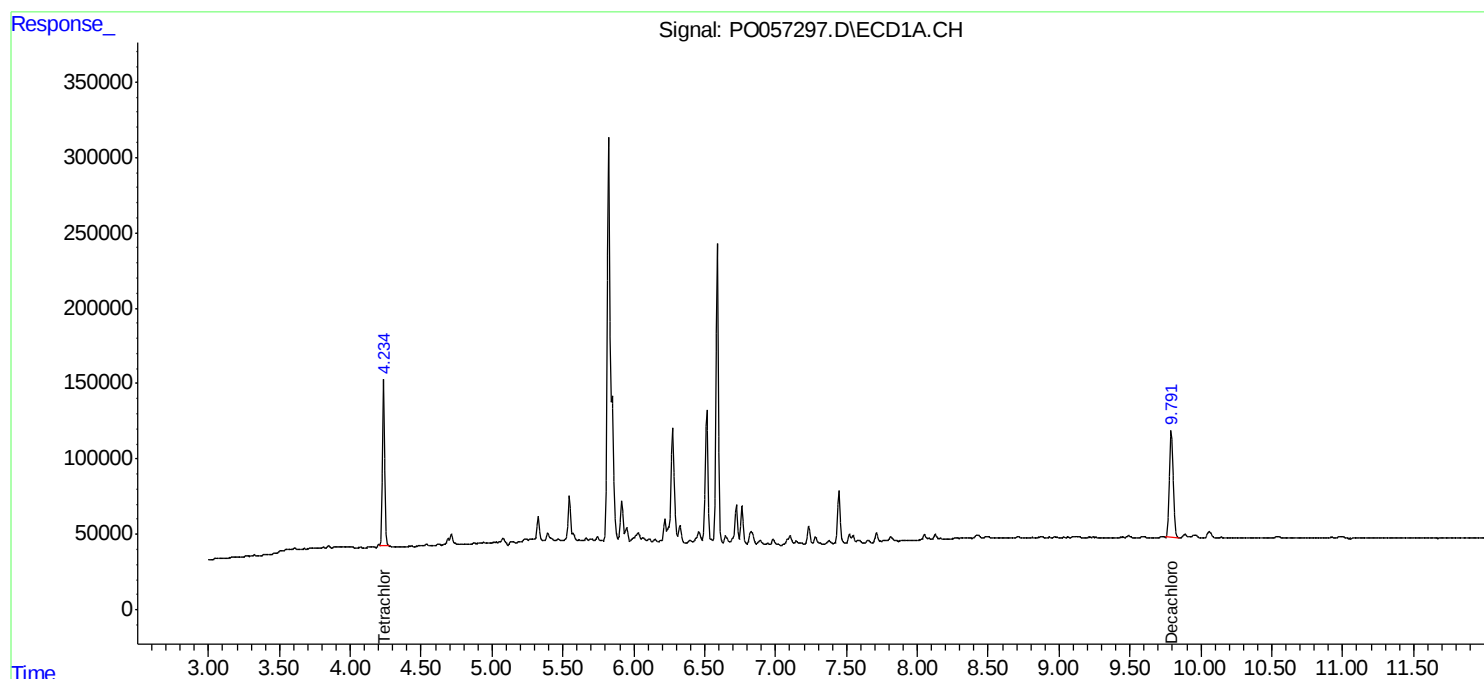

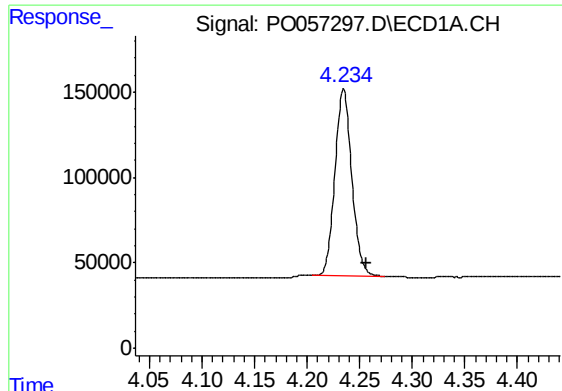


#1 Tetrachloro-m-xylene

R.T.: 4.234 min
Delta R.T.: -0.022 min
Response: 1220692
Conc: 31.89 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-061719-A


Manual Integrations
APPROVED

Ankita
6/21/2019 3:28:51 PM

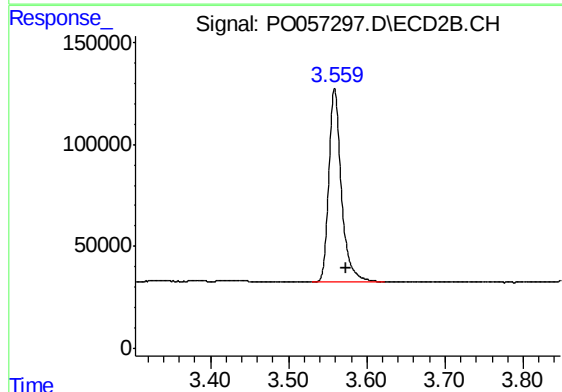


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 1068786
Conc: 32.41 ng/ml

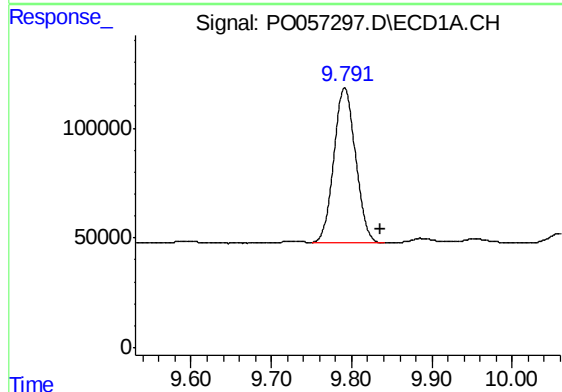

#2 Decachlorobiphenyl

R.T.: 9.791 min
Delta R.T.: -0.045 min
Response: 1319814
Conc: 26.89 ng/ml m

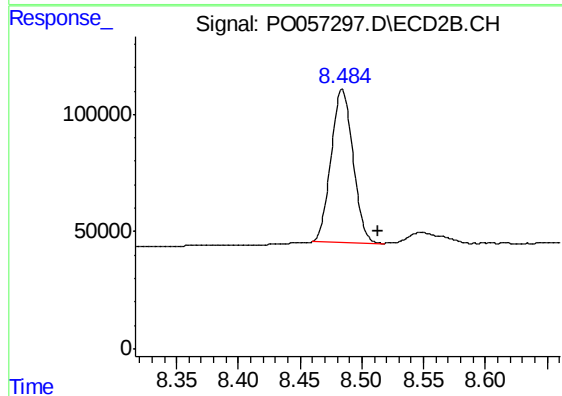

#2 Decachlorobiphenyl

R.T.: 8.484 min
Delta R.T.: -0.029 min
Response: 810632
Conc: 22.73 ng/ml