

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062019\
 Data File : P0057303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 12:55
 Operator : SM/SJ
 Sample : K3406-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BAT-B14

Manual Integrations
 APPROVED

Ankita
 6/21/2019 3:29:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 01:55:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.233	3.558	1027234	863896	26.832m	26.196
2) SA Decachlor...	9.793	8.482	1033274	663122	21.051	18.597m
Target Compounds						
31) L7 AR-1260-1	6.980	6.087	229540	169139	89.448m	84.553
32) L7 AR-1260-2	7.237	6.274	369731	274914	122.259	111.529
33) L7 AR-1260-3	7.593	6.426	191136	179044	79.341m	79.815
34) L7 AR-1260-4	7.818	6.892	191120	131418	72.969m	70.616m
35) L7 AR-1260-5	8.125	7.135	383997	330053	80.299m	76.537

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062019\
Data File : PO057303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 12:55
Operator : SM/SJ
Sample : K3406-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
Client Sampled :
BAT-B14


Manual Integrations
APPROVED

Ankita
6/21/2019 3:29:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 01:55:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

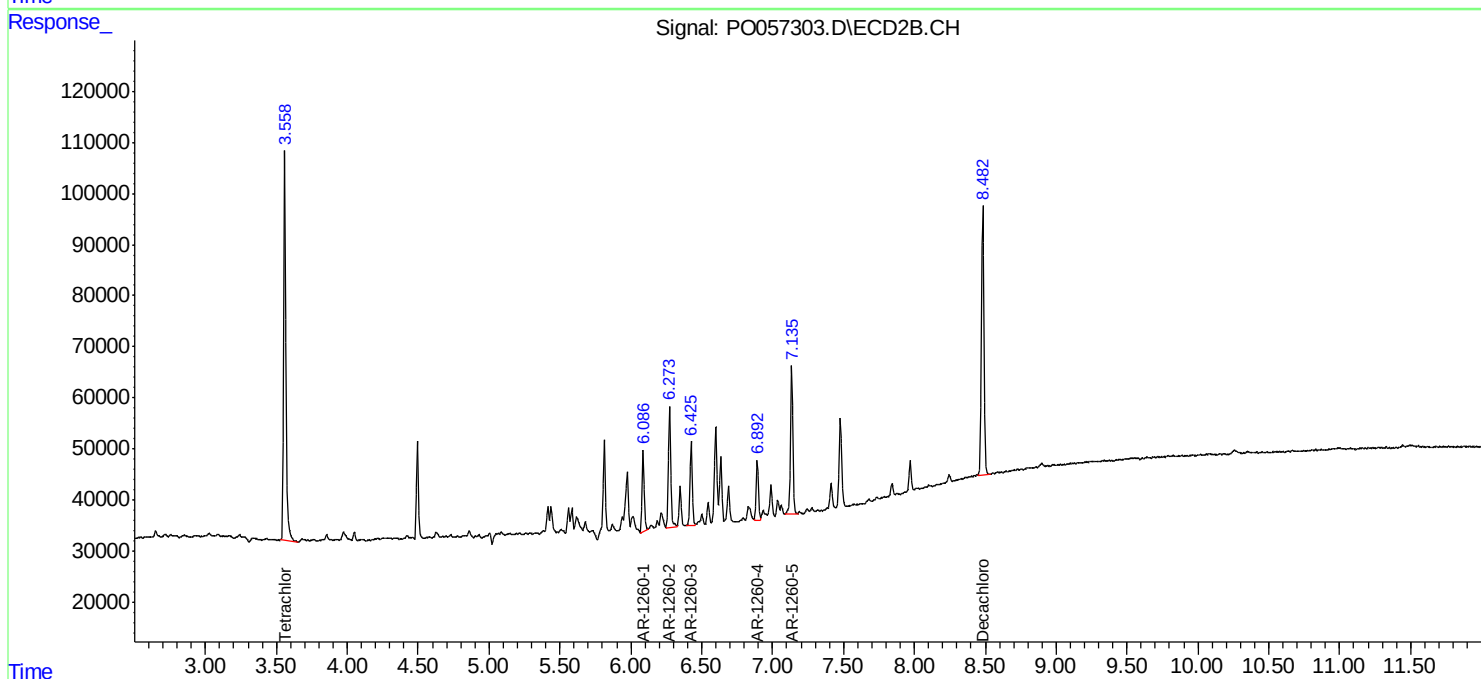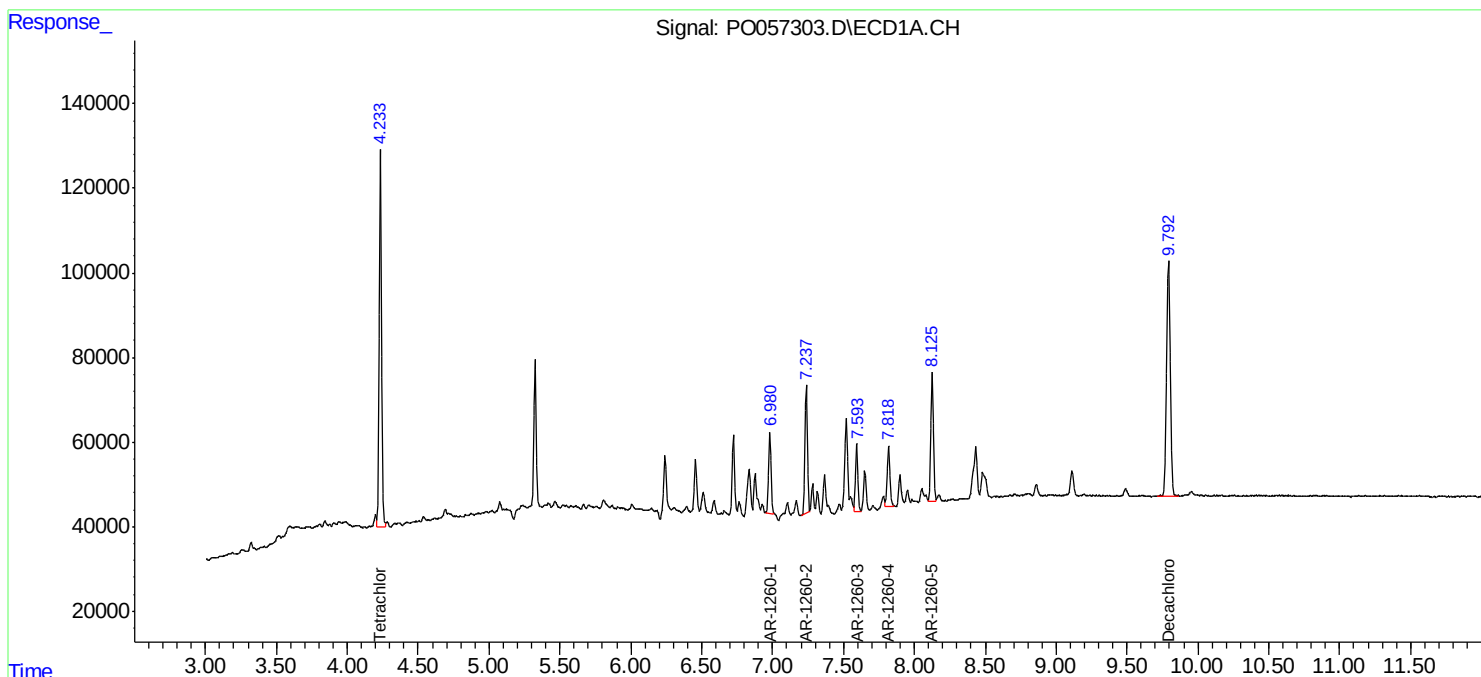

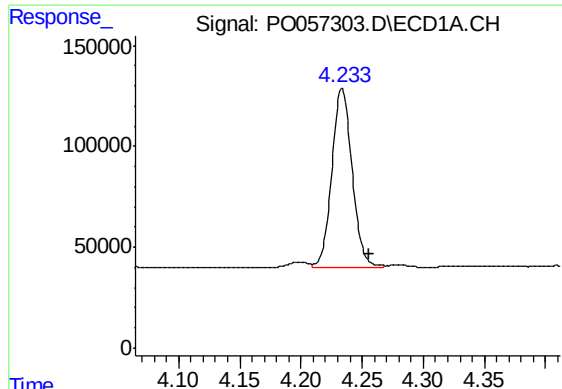


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.023 min
Response: 1027234
Conc: 26.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BAT-B14


Manual Integrations
APPROVED

Ankita
6/21/2019 3:29:07 PM

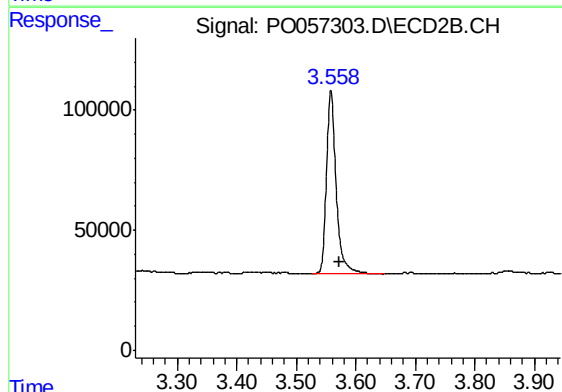


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: -0.015 min
Response: 863896
Conc: 26.20 ng/ml

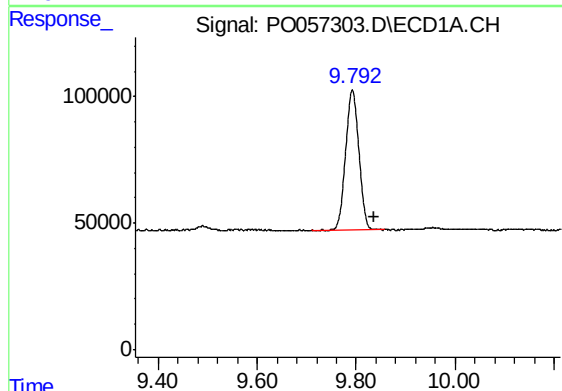


#2 Decachlorobiphenyl

R.T.: 9.793 min
Delta R.T.: -0.044 min
Response: 1033274
Conc: 21.05 ng/ml

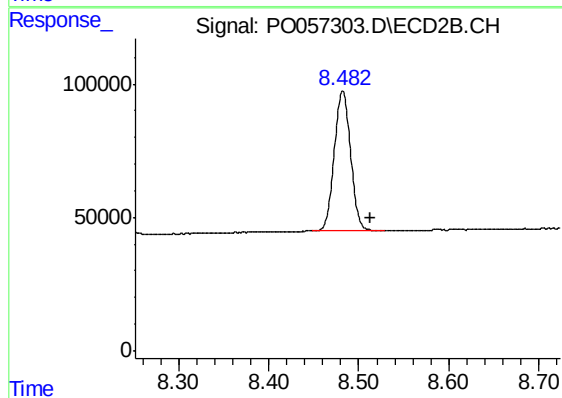

#2 Decachlorobiphenyl

R.T.: 8.482 min
Delta R.T.: -0.031 min
Response: 663122
Conc: 18.60 ng/ml m

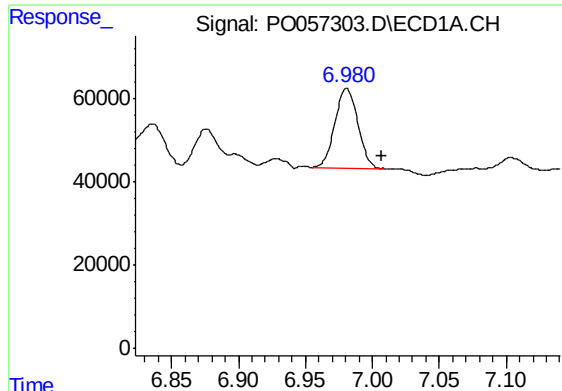


#31 AR-1260-1

R.T.: 6.980 min
Delta R.T.: -0.027 min
Response: 229540
Conc: 89.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BAT-B14


Manual Integrations
APPROVED

Ankita
6/21/2019 3:29:07 PM

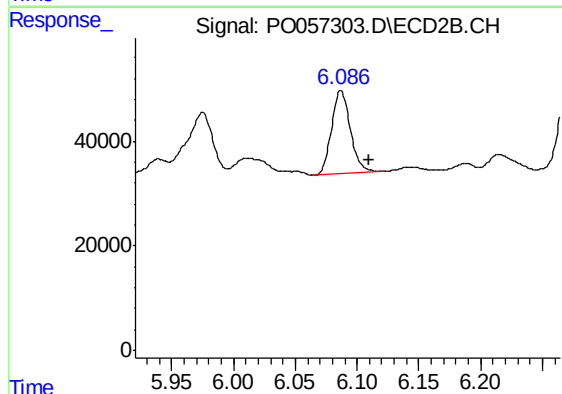


#31 AR-1260-1

R.T.: 6.087 min
Delta R.T.: -0.023 min
Response: 169139
Conc: 84.55 ng/ml

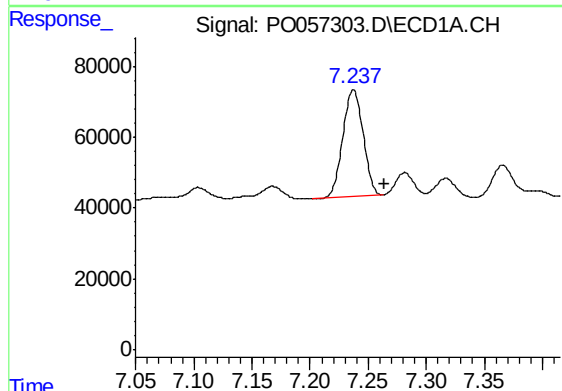


#32 AR-1260-2

R.T.: 7.237 min
Delta R.T.: -0.026 min
Response: 369731
Conc: 122.26 ng/ml

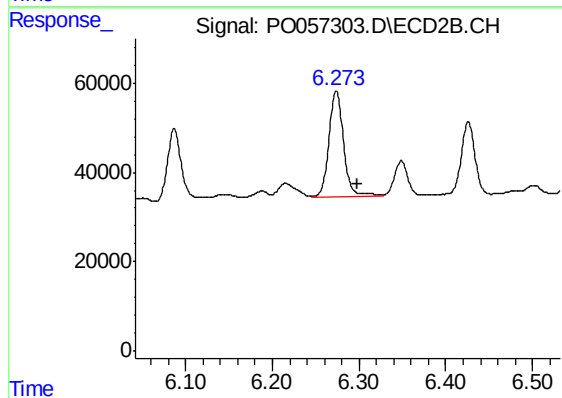

#32 AR-1260-2

R.T.: 6.274 min
Delta R.T.: -0.024 min
Response: 274914
Conc: 111.53 ng/ml

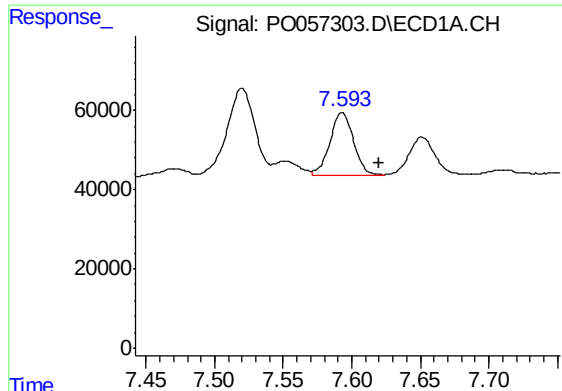


#33 AR-1260-3

R.T.: 7.593 min
Delta R.T.: -0.027 min
Response: 191136
Conc: 79.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BAT-B14


Manual Integrations
APPROVED

Ankita
6/21/2019 3:29:07 PM

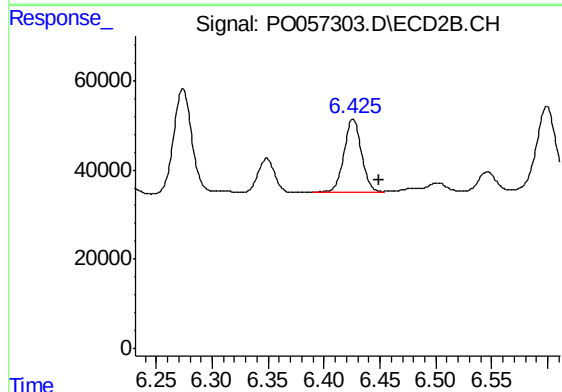


#33 AR-1260-3

R.T.: 6.426 min
Delta R.T.: -0.024 min
Response: 179044
Conc: 79.82 ng/ml

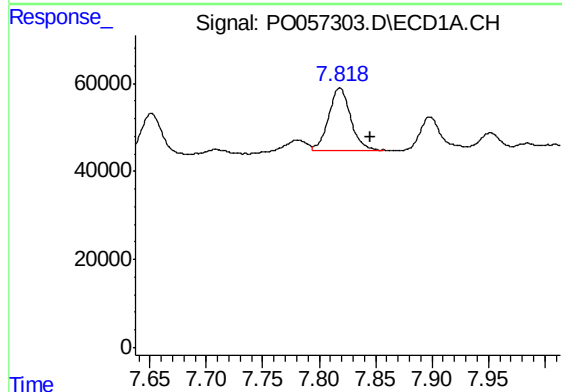


#34 AR-1260-4

R.T.: 7.818 min
Delta R.T.: -0.027 min
Response: 191120
Conc: 72.97 ng/ml m

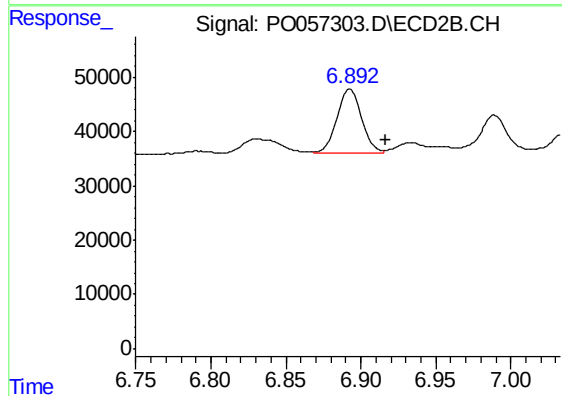

#34 AR-1260-4

R.T.: 6.892 min
Delta R.T.: -0.025 min
Response: 131418
Conc: 70.62 ng/ml m

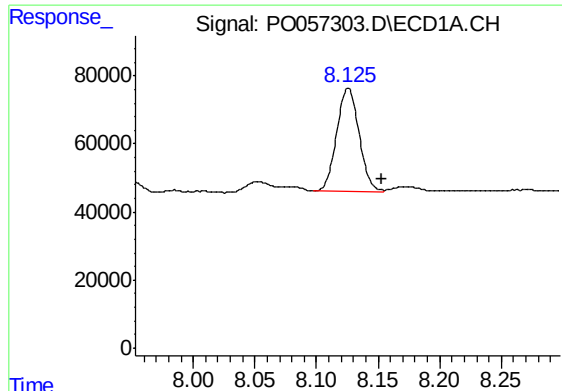


#35 AR-1260-5

R.T.: 8.125 min
Delta R.T.: -0.028 min
Response: 383997
Conc: 80.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BAT-B14

Manual Integrations
APPROVED

Ankita
6/21/2019 3:29:07 PM

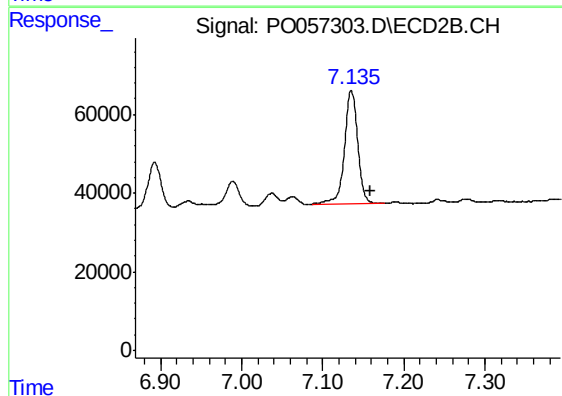

#35 AR-1260-5

R.T.: 7.135 min
Delta R.T.: -0.023 min
Response: 330053
Conc: 76.54 ng/ml