

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062019\
 Data File : P0057310.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 15:37
 Operator : SM/SJ
 Sample : PB120789BSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB120789BSD

Manual Integrations
 APPROVED

Ankita
 6/21/2019 3:29:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 01:57:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	3.559	1060414	617907	27.699	18.737 #
2)	SA Decachlor...	9.795	8.483	866088	555843	17.645	15.589m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062019\
Data File : PO057310.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 15:37
Operator : SM/SJ
Sample : PB120789BSD
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB120789BSD


Manual Integrations
APPROVED

Ankita
6/21/2019 3:29:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 01:57:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

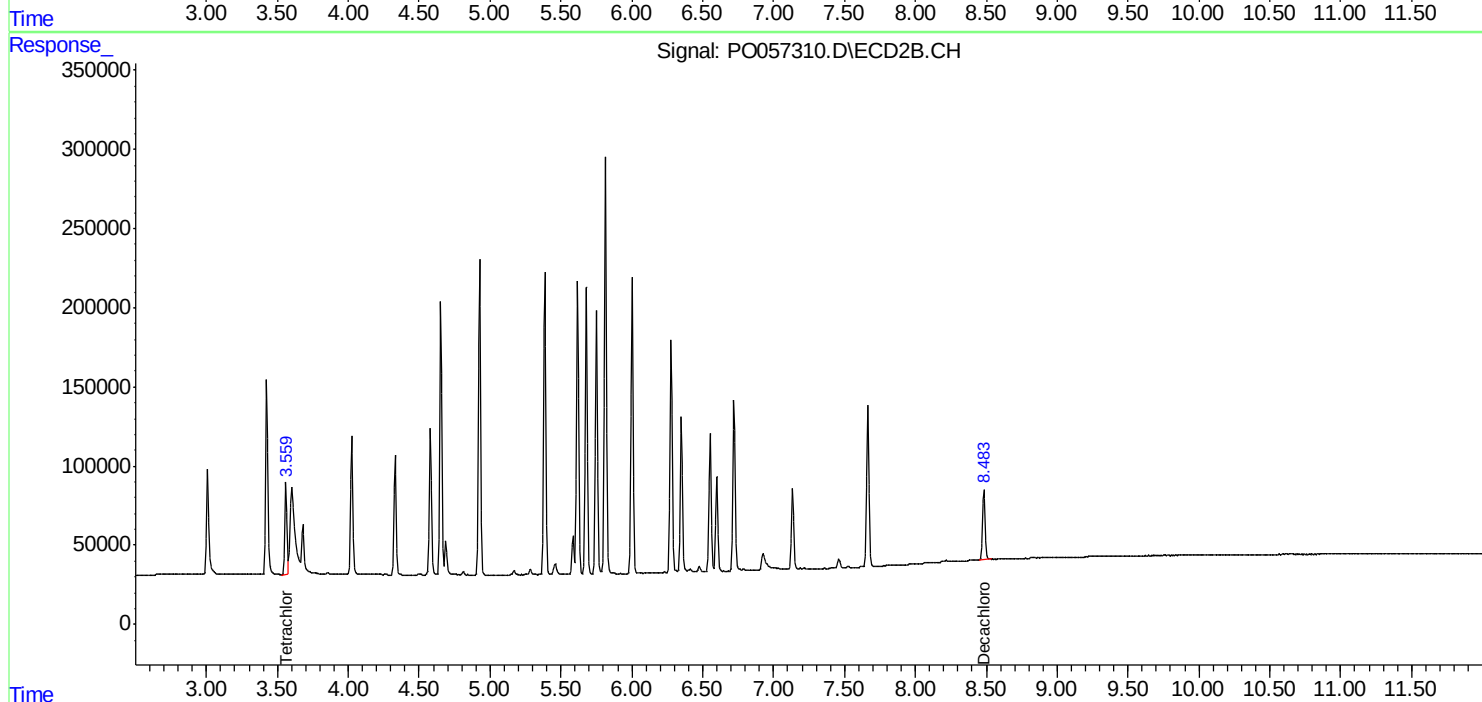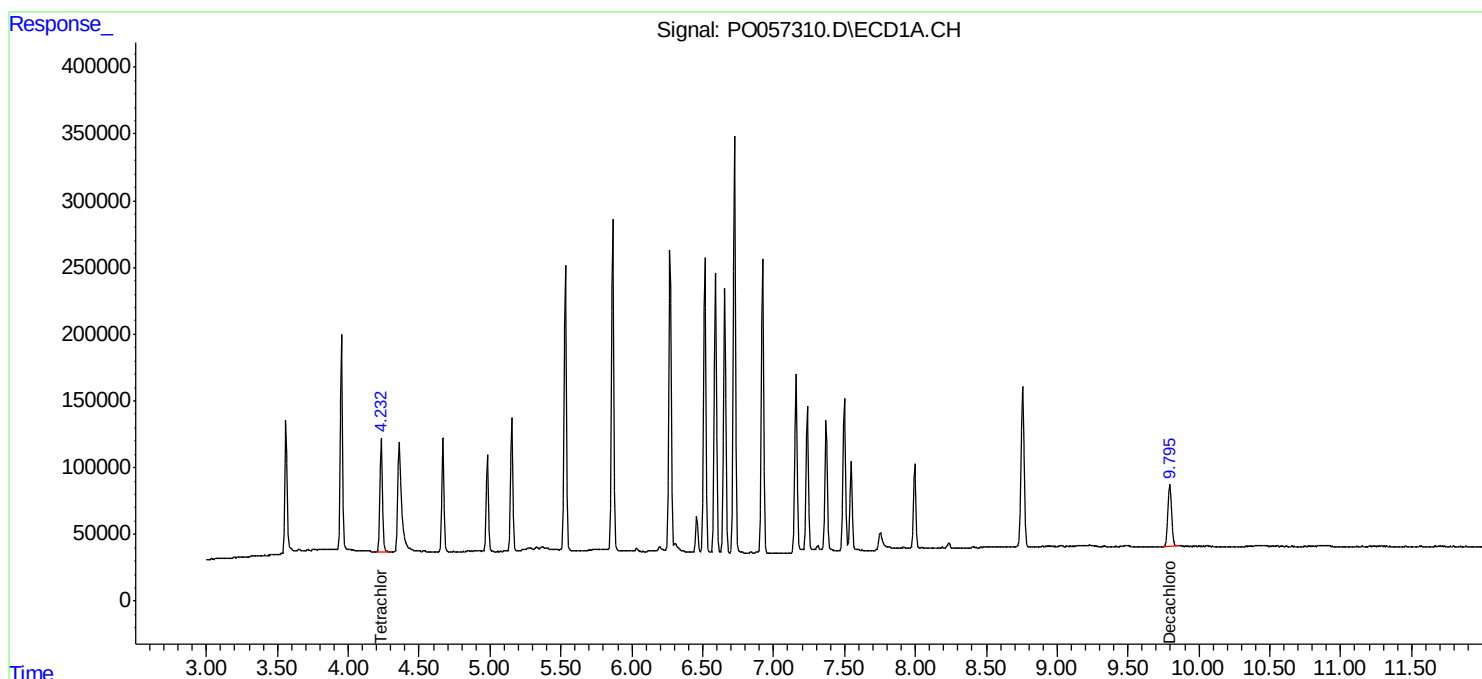

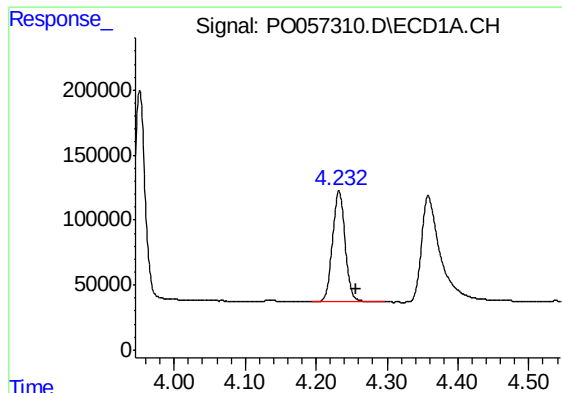


#1 Tetrachloro-m-xylene

R.T.: 4.232 min
Delta R.T.: -0.024 min
Response: 1060414
Conc: 27.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB120789BSD


Manual Integrations
APPROVED

Ankita
6/21/2019 3:29:18 PM

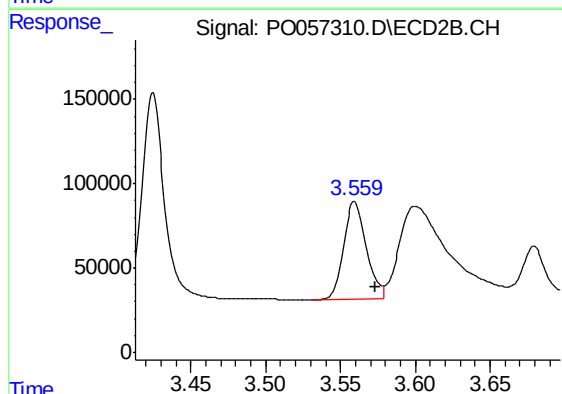


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 617907
Conc: 18.74 ng/ml

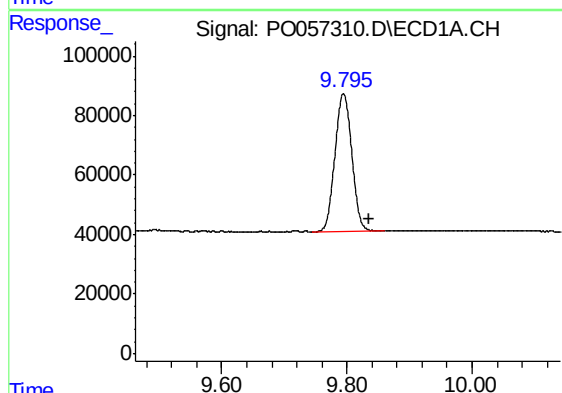

#2 Decachlorobiphenyl

R.T.: 9.795 min
Delta R.T.: -0.042 min
Response: 866088
Conc: 17.65 ng/ml

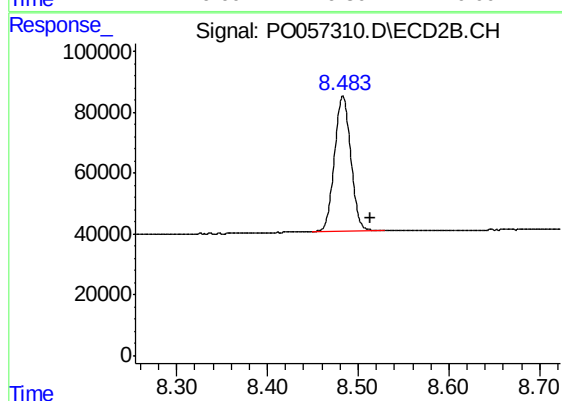

#2 Decachlorobiphenyl

R.T.: 8.483 min
Delta R.T.: -0.030 min
Response: 555843
Conc: 15.59 ng/ml m