

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062019\
 Data File : P0057326.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 20:26
 Operator : SM/SJ
 Sample : K3458-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 POST-CARTRIDGE-FILTER

Manual Integrations
 APPROVED

Ankita
 6/21/2019 3:30:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:06:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	3.557	656022	524673	17.136m	15.910m
2)	SA Decachlor...	9.793	8.482	519652	349211	10.587m	9.794m
Target Compounds							
21)	L5 AR-1248-1	5.393	4.624	702848	494100	545.471m	527.592m
22)	L5 AR-1248-2	5.662	4.856	1122668	983268	602.647m	773.955 #
23)	L5 AR-1248-3	5.864	4.896	1990274	1032528	970.224m	790.663m
24)	L5 AR-1248-4	6.265	5.068	3185206	1398551	1376.681m	883.131m#
25)	L5 AR-1248-5	6.303	5.455	3533518	2277443	1606.594m	1376.039

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062019\
Data File : PO057326.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 20:26
Operator : SM/SJ
Sample : K3458-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTER


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:06:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

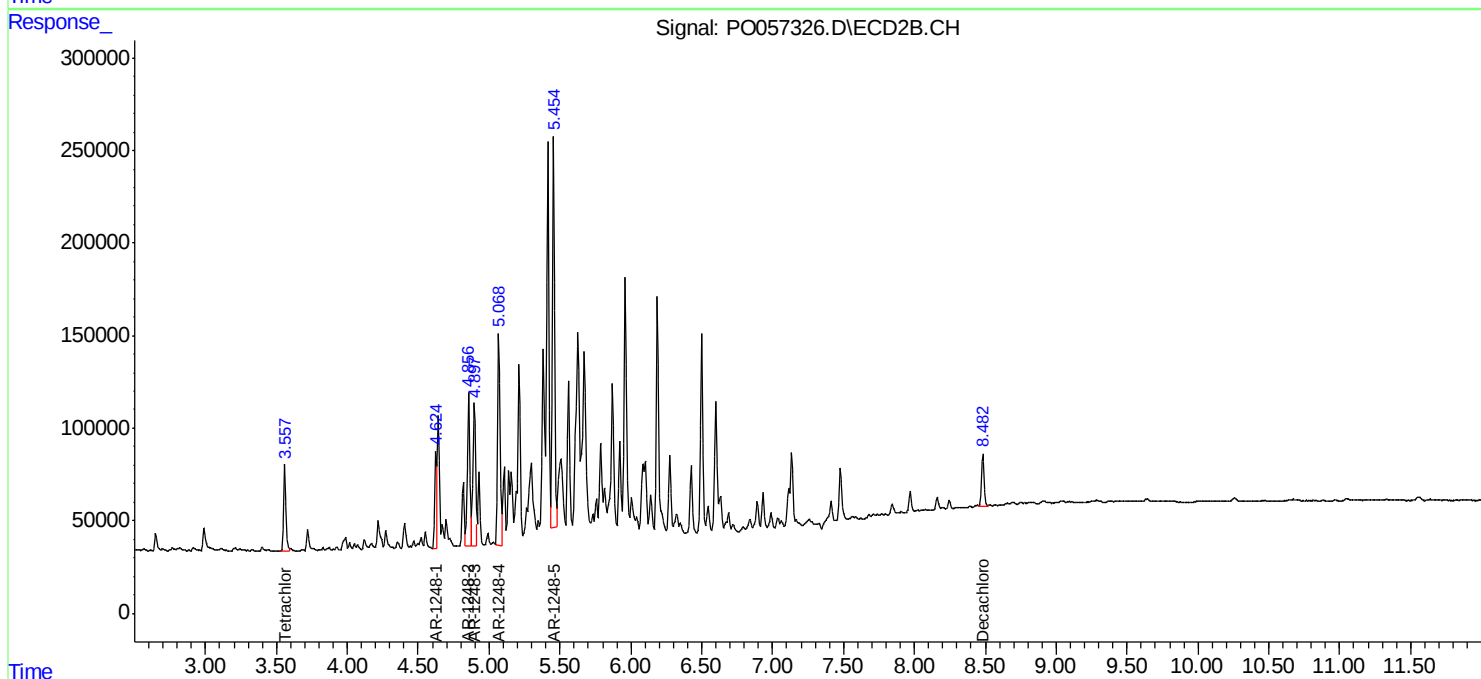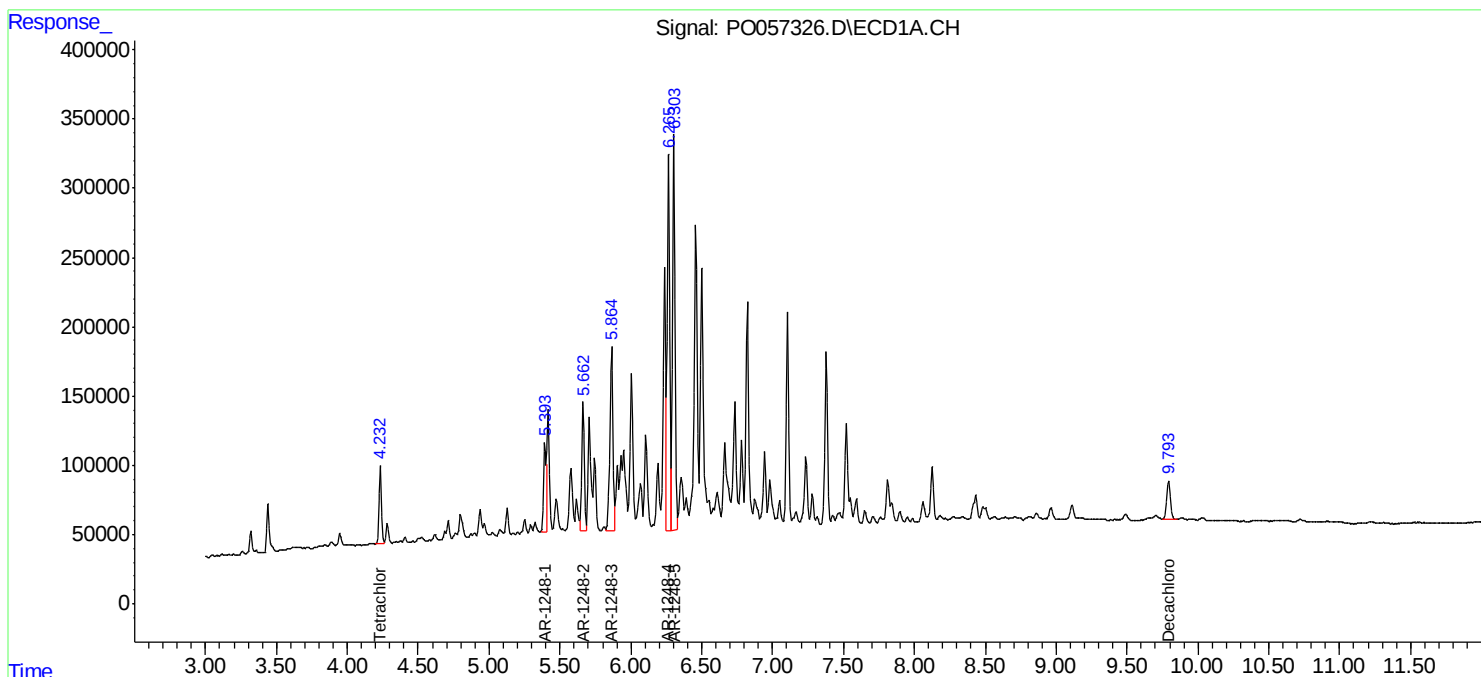

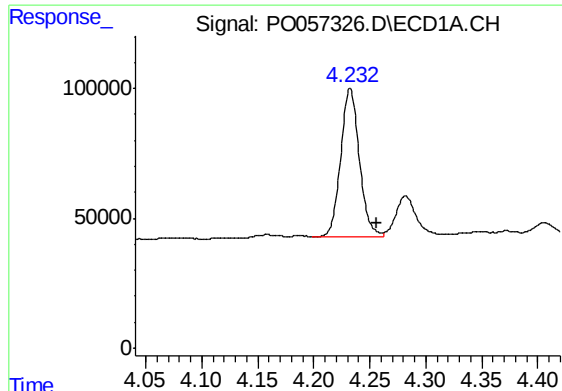


#1 Tetrachloro-m-xylene

R.T.: 4.232 min
Delta R.T.: -0.024 min
Response: 656022
Conc: 17.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTER


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:04 PM

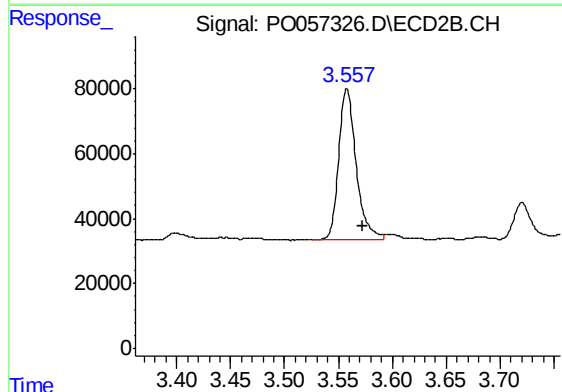


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.016 min
Response: 524673
Conc: 15.91 ng/ml m

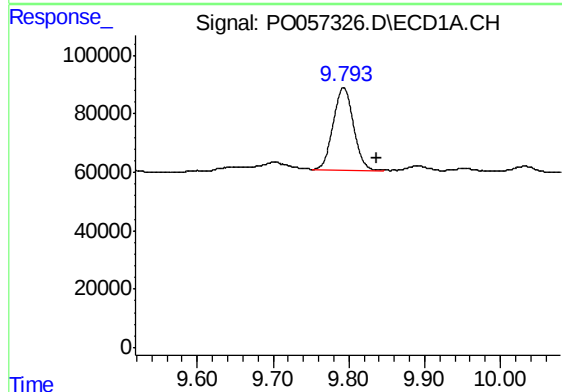


#2 Decachlorobiphenyl

R.T.: 9.793 min
Delta R.T.: -0.043 min
Response: 519652
Conc: 10.59 ng/ml m

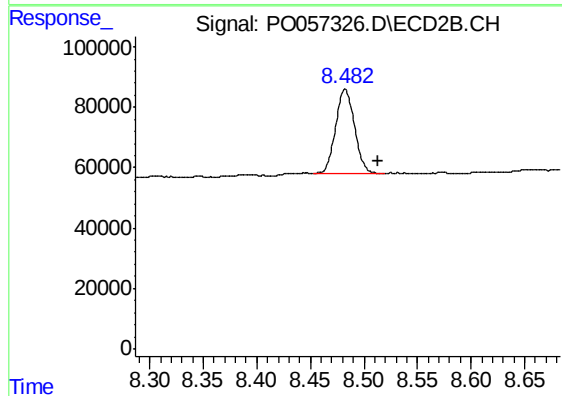

#2 Decachlorobiphenyl

R.T.: 8.482 min
Delta R.T.: -0.031 min
Response: 349211
Conc: 9.79 ng/ml m

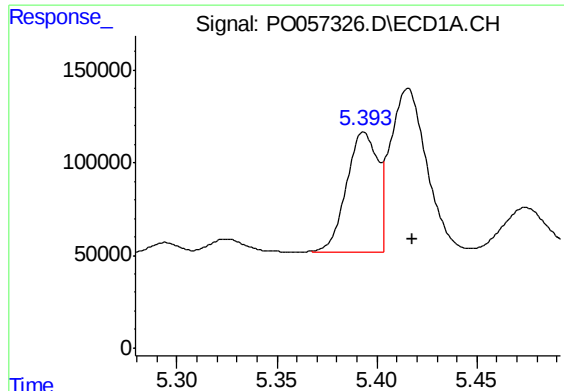


#21 AR-1248-1

R.T.: 5.393 min
Delta R.T.: -0.025 min
Response: 702848
Conc: 545.47 ng/ml m

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTER


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:04 PM

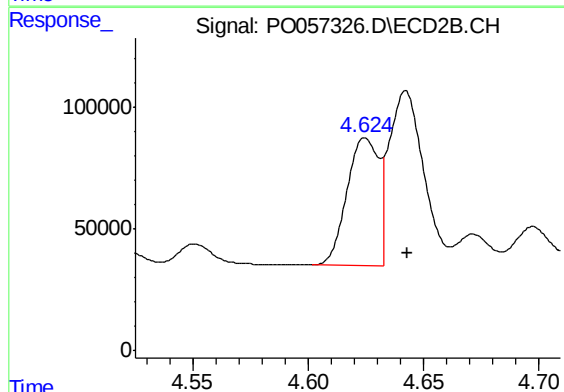


#21 AR-1248-1

R.T.: 4.624 min
Delta R.T.: -0.019 min
Response: 494100
Conc: 527.59 ng/ml m

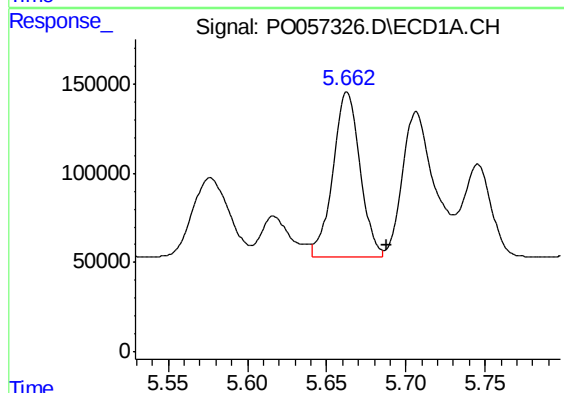


#22 AR-1248-2

R.T.: 5.662 min
Delta R.T.: -0.025 min
Response: 1122668
Conc: 602.65 ng/ml m

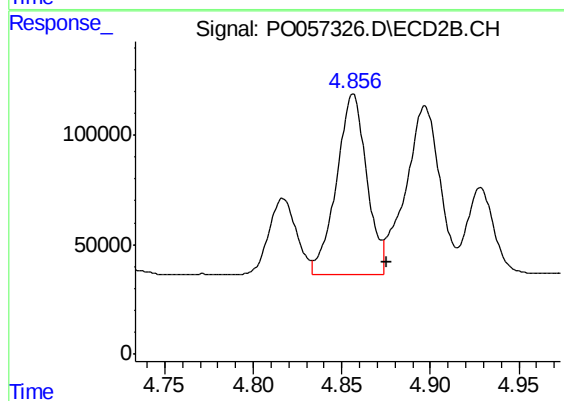

#22 AR-1248-2

R.T.: 4.856 min
Delta R.T.: -0.019 min
Response: 983268
Conc: 773.96 ng/ml

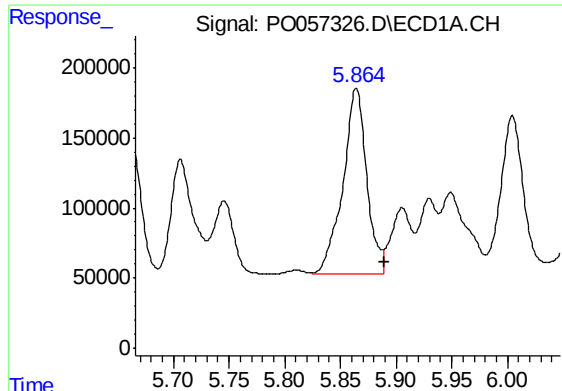


#23 AR-1248-3

R.T.: 5.864 min
Delta R.T.: -0.026 min
Response: 1990274
Conc: 970.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTER


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:04 PM

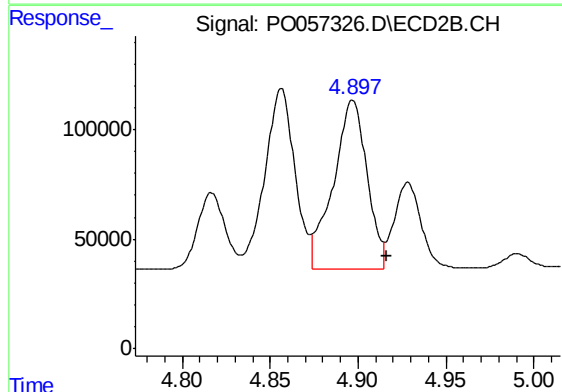


#23 AR-1248-3

R.T.: 4.896 min
Delta R.T.: -0.020 min
Response: 1032528
Conc: 790.66 ng/ml m

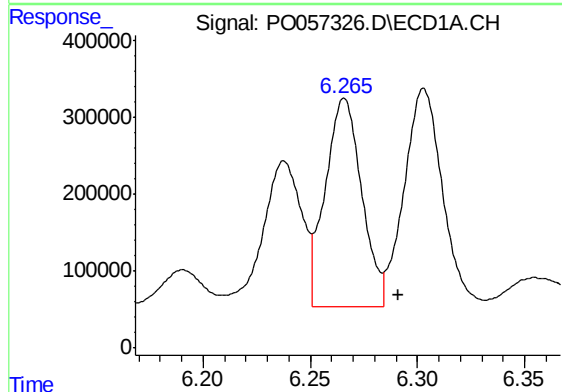


#24 AR-1248-4

R.T.: 6.265 min
Delta R.T.: -0.025 min
Response: 3185206
Conc: 1376.68 ng/ml m

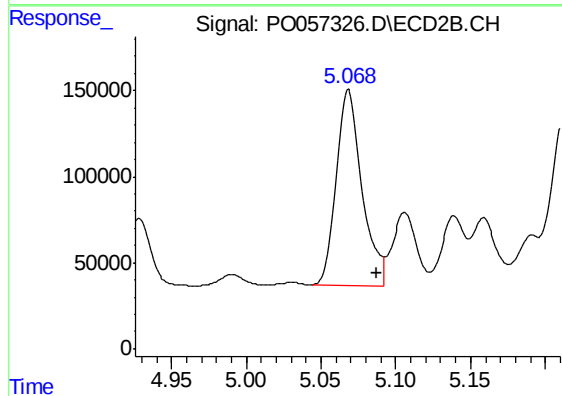

#24 AR-1248-4

R.T.: 5.068 min
Delta R.T.: -0.019 min
Response: 1398551
Conc: 883.13 ng/ml m

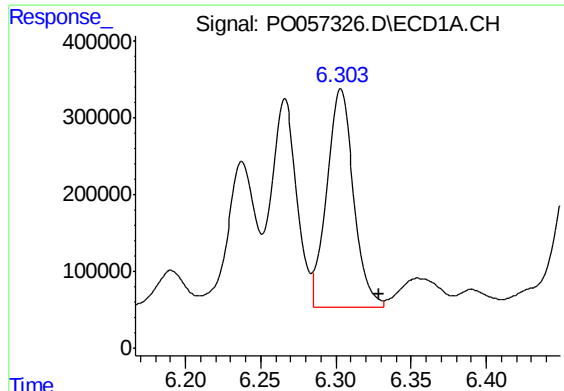


#25 AR-1248-5

R.T.: 6.303 min
Delta R.T.: -0.026 min
Response: 3533518
Conc: 1606.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTER

Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:04 PM

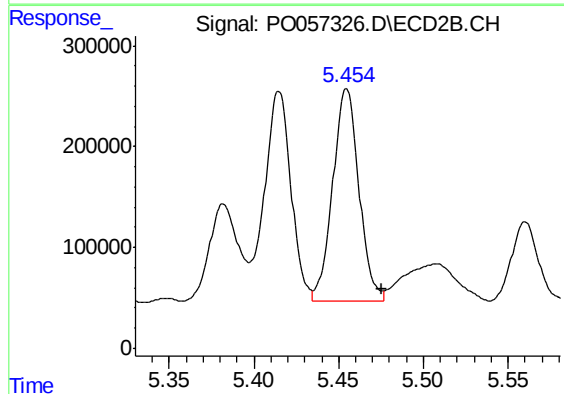

#25 AR-1248-5

R.T.: 5.455 min
Delta R.T.: -0.021 min
Response: 2277443
Conc: 1376.04 ng/ml